


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082624\
Data File : BN033617.D
Acq On : 26 Aug 2024 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 23 00:22:18 2024

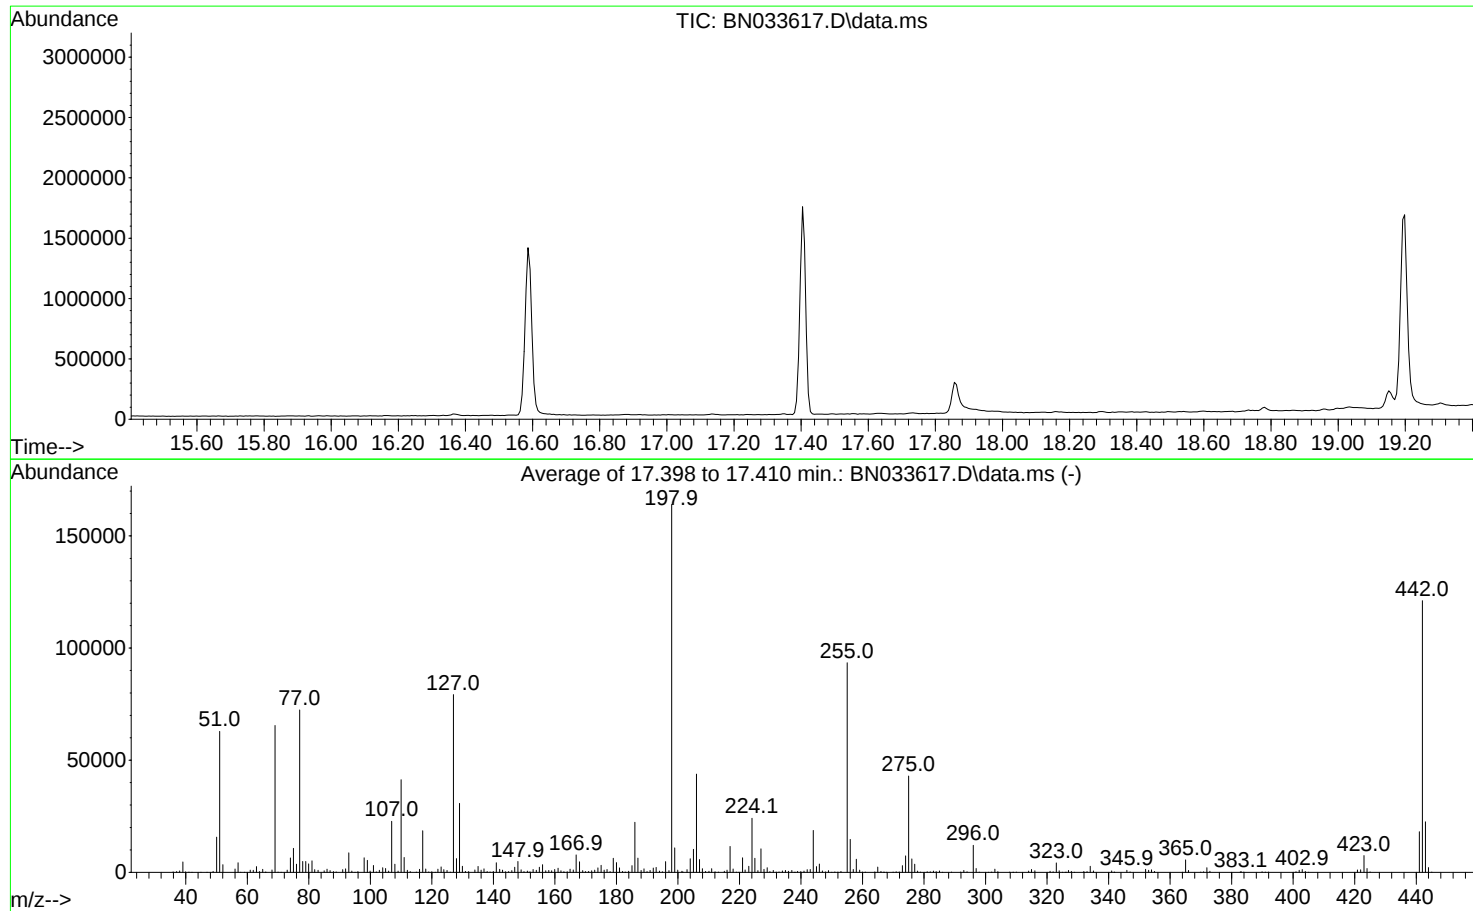

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	62871	PASS
68	69	0.00	2	1.7	1095	PASS
69	198	0.00	100	39.9	65518	PASS
70	69	0.00	2	0.3	181	PASS
127	198	10	80	48.3	79261	PASS
197	198	0.00	2	0.5	754	PASS
198	198	100	100	100.0	164011	PASS
199	198	5	9	6.7	10913	PASS
275	198	10	60	26.2	42933	PASS
365	198	1	100	3.4	5548	PASS
441	198	0.01	100	11.1	18152	PASS
442	442	50	100	100.0	121147	PASS
443	442	15	24	18.6	22535	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/26/2024	BNA_N	<u>BN033617.D</u>
Compound Name	Response	Retention Time
DDT	663399	20.445
DDD	13947	20.004
DDE	1916	19.498
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15863	679262	2.34

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082624\
Data File : BN033617.D
Acq On : 26 Aug 2024 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 26 14:34:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 06:44:36 2024
Response via : Initial Calibration

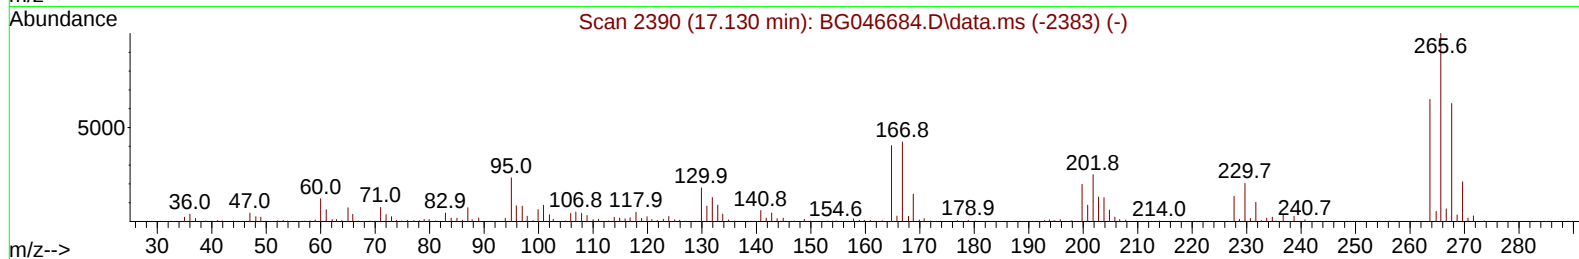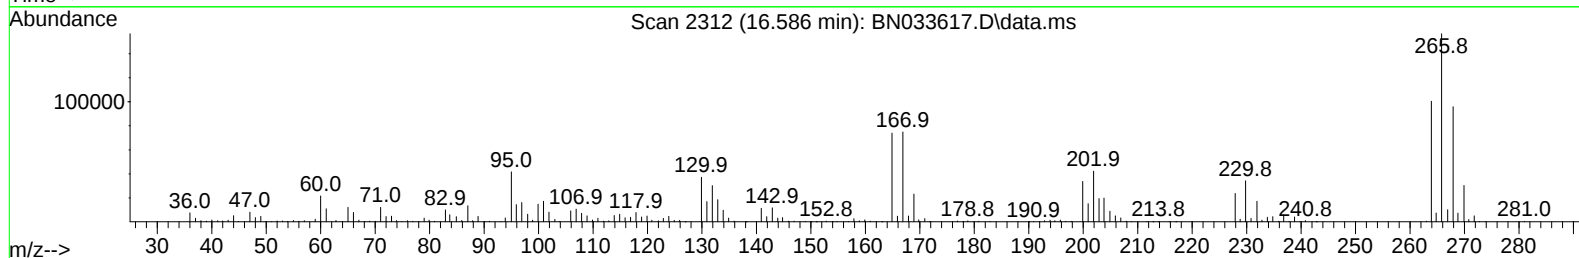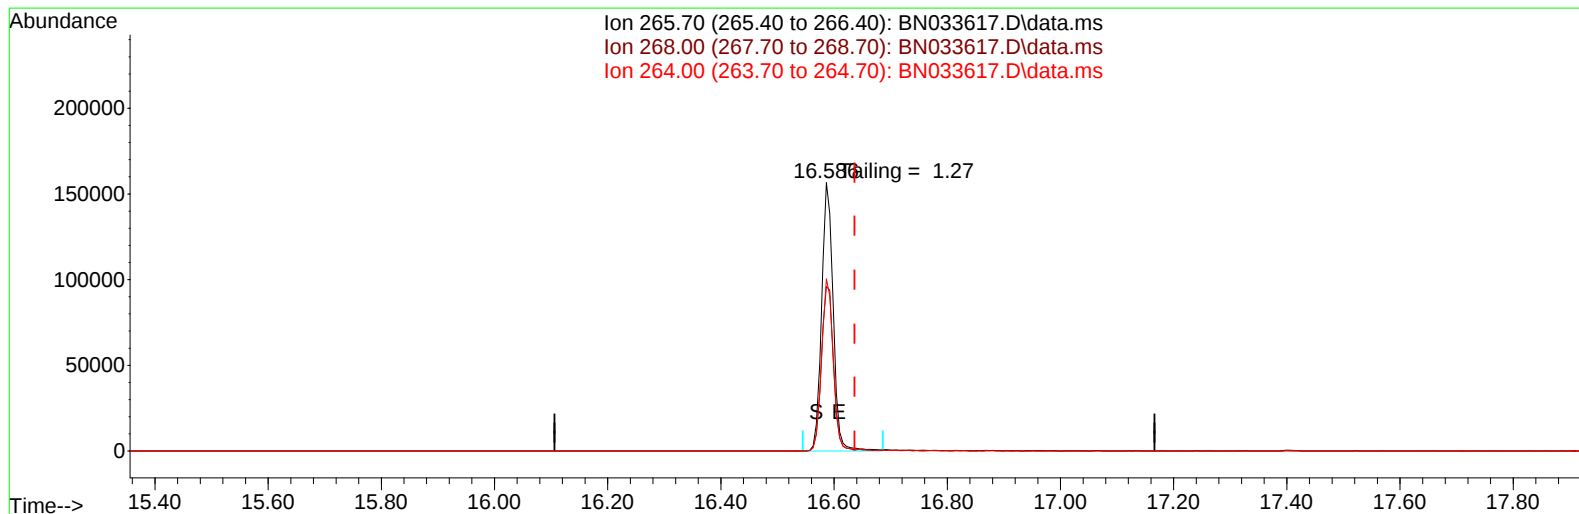

TIC: BN033617.D\data.ms

(70) Pentachlorophenol (C)

16.586min (-0.050) 23086.22 ng




response 221758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.27
264.00	61.60	64.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082624\
Data File : BN033617.D
Acq On : 26 Aug 2024 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 26 14:34:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 06:44:36 2024
Response via : Initial Calibration

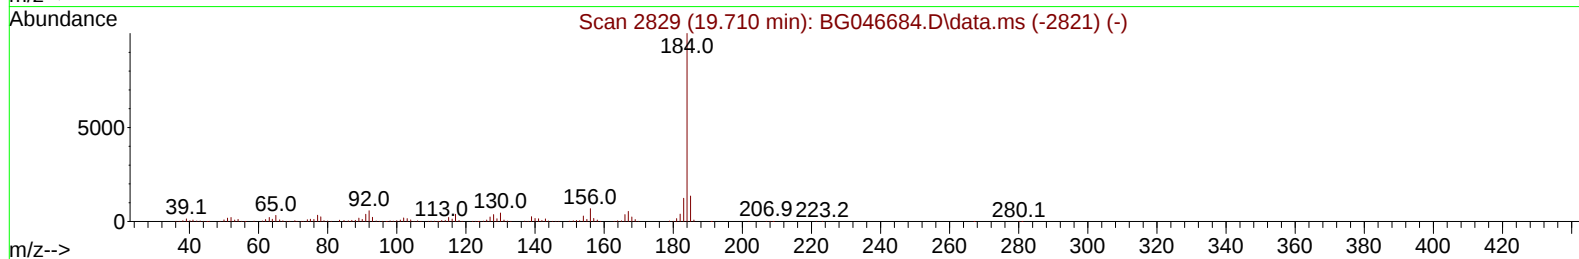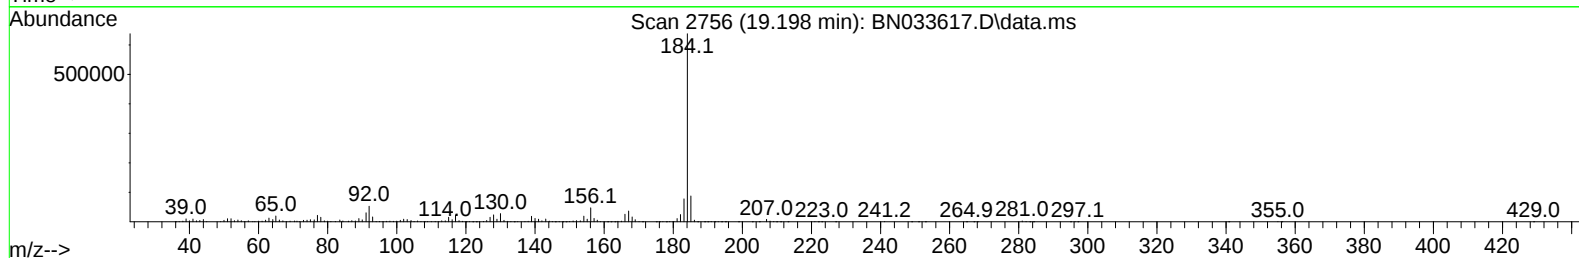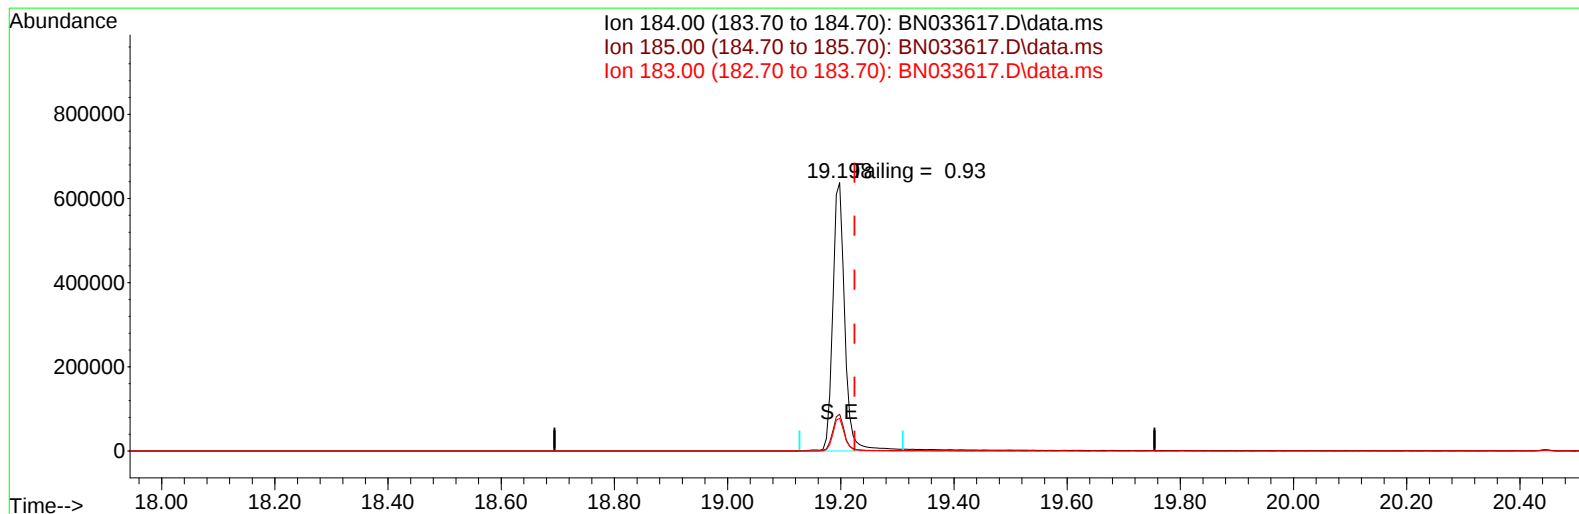

TIC: BN033617.D\data.ms

(77) Benzidine

19.198min (-0.026) 149307.71 ng

response 938903

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.75
183.00	13.20	12.20
0.00	0.00	0.00