
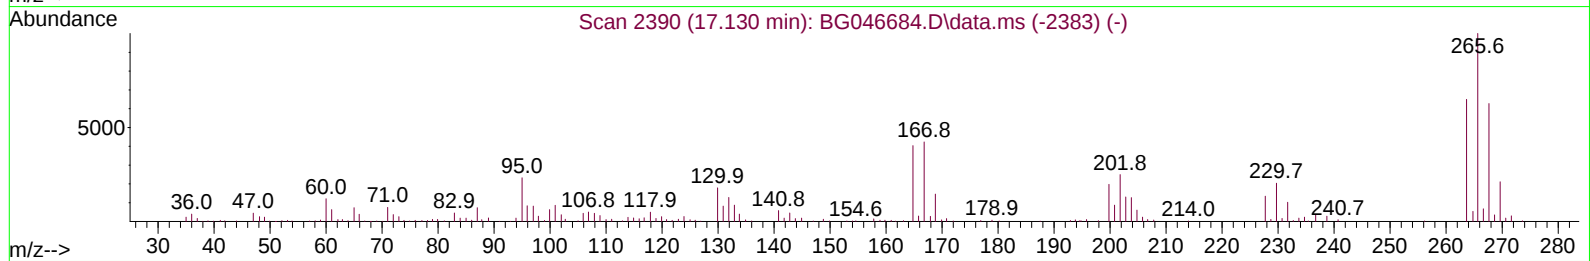
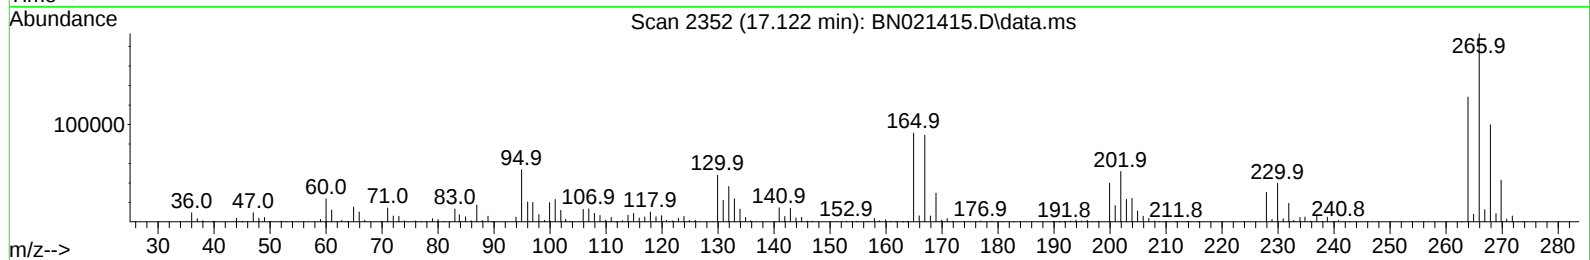


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
Data File : BN021415.D
Acq On : 29 Aug 2022 09:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 14:49:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

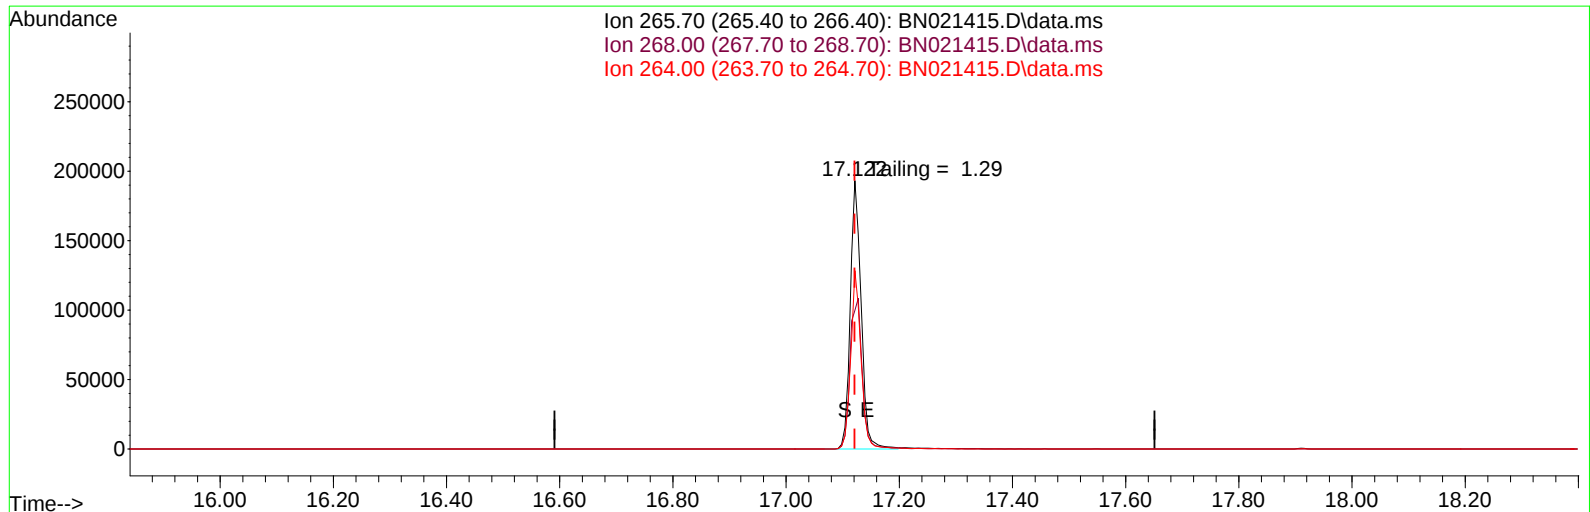

TIC: BN021415.D\data.ms




(70) Pentachlorophenol (C)

17.122min (+ 0.001) 19651.27 ng

response 262171

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	51.63
264.00	61.60	66.42
0.00	0.00	0.00

Quant Time: Aug 29 14:49:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

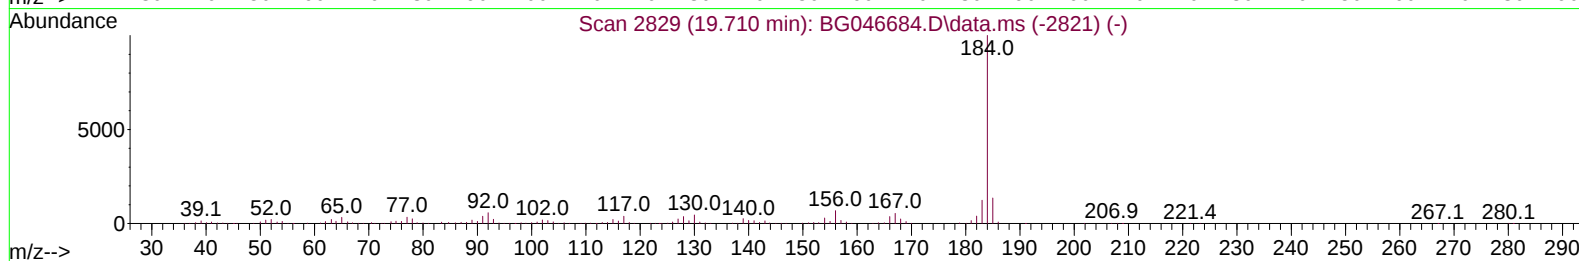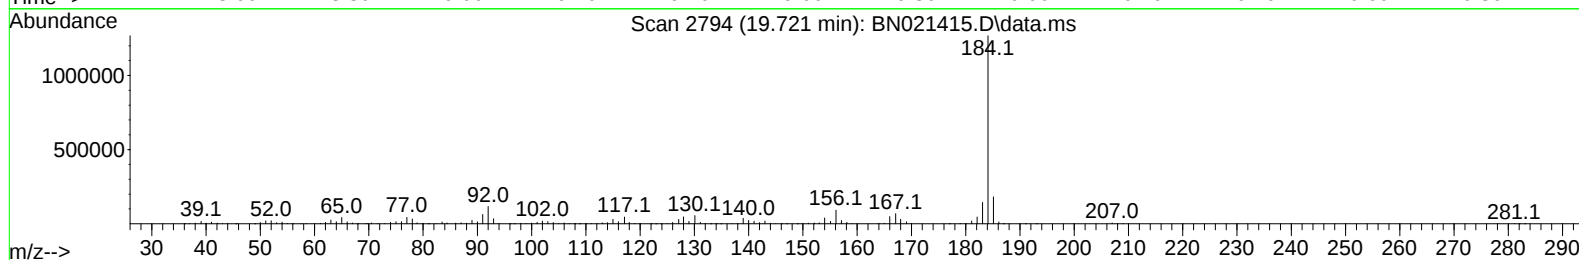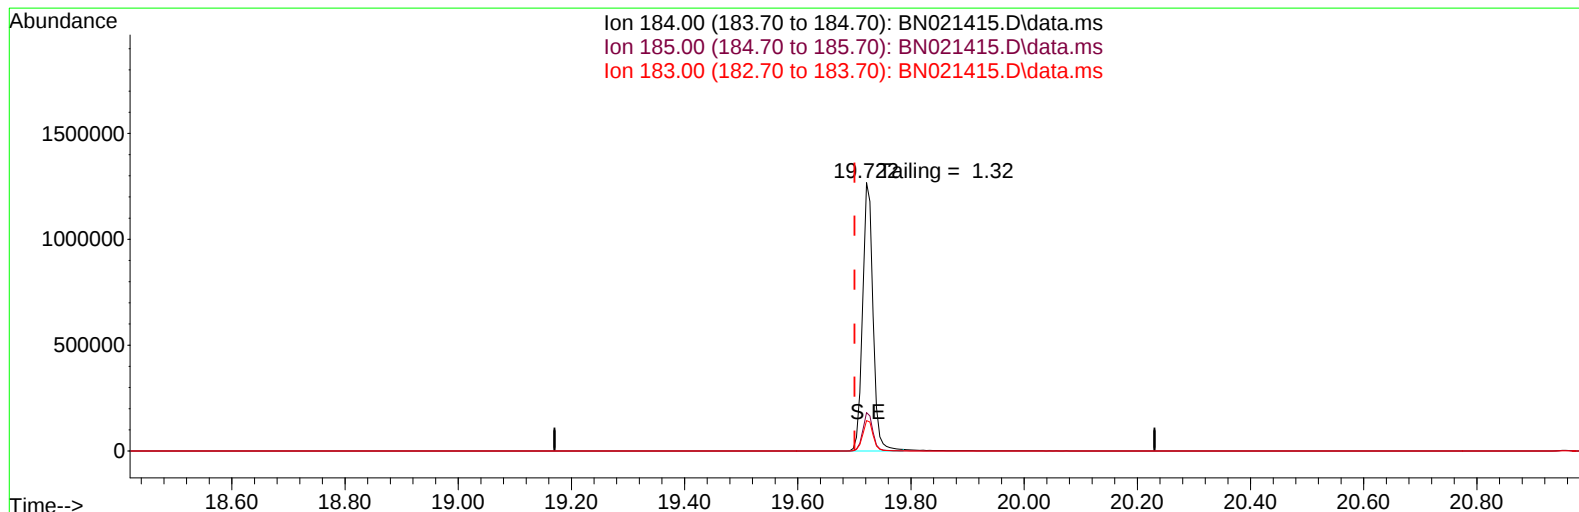

TIC: BN021415.D\data.ms

(77) Benzidine

19.721min (+ 0.021) 0.00 ng

```
response      1642830
```

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.50	14.33
--------	-------	-------

183.00	13.20	11.35
--------	-------	-------

0.00 0.00 0.00