

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
 Data File : BN021422.D
 Acq On : 29 Aug 2022 14:20
 Operator : CG/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Aug 29 15:18:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 29 14:52:01 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.076	152	4691	0.400	ng	0.00
7) Naphthalene-d8	10.909	136	14028	0.400	ng	0.00
13) Acenaphthene-d10	14.728	164	8049	0.400	ng	0.00
19) Phenanthrene-d10	17.480	188	15356	0.400	ng	0.00
29) Chrysene-d12	21.673	240	13605	0.400	ng	0.00
35) Perylene-d12	24.199	264	8793	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.599	112	28394	2.237	ng	0.00
5) Phenol-d6	7.224	99	37872	2.380	ng	0.00
8) Nitrobenzene-d5	9.254	82	30869	2.908	ng	0.00
11) 2-Methylnaphthalene-d10	12.493	152	103224	4.357	ng	0.00
14) 2,4,6-Tribromophenol	16.218	330	9280	2.517	ng	0.00
15) 2-Fluorobiphenyl	13.360	172	105040	2.918	ng	0.00
27) Fluoranthene-d10	19.510	212	132077	2.879	ng	0.00
31) Terphenyl-d14	20.097	244	86474	3.008	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.410	88	17644	2.711	ng	# 89
3) n-Nitrosodimethylamine	3.743	42	17193	2.762	ng	# 94
6) bis(2-Chloroethyl)ether	7.491	93	44071	2.768	ng	98
9) Naphthalene	10.962	128	127816	2.771	ng	98
10) Hexachlorobutadiene	11.240	225	21630	2.843	ng	# 100
12) 2-Methylnaphthalene	12.191	142	21824	2.780	ng	# 85
16) Acenaphthylene	14.450	152	127349	3.156	ng	100
17) Acenaphthene	14.792	154	83744	2.990	ng	98
18) Fluorene	15.776	166	102764	2.929	ng	100
21) 4-Bromophenyl-phenylether	16.670	248	31586	3.004	ng	97
22) Hexachlorobenzene	16.782	284	36484	2.990	ng	99
23) Atrazine	16.926	200	20456	3.078	ng	96
24) Pentachlorophenol	17.121	266	10822	2.567	ng	99
25) Phenanthrene	17.521	178	169385	3.016	ng	100
26) Anthracene	17.613	178	146871	3.183	ng	100
28) Fluoranthene	19.539	202	188015	3.041	ng	100
30) Pyrene	19.902	202	211825	3.092	ng	# 92
32) Benzo(a)anthracene	21.655	228	156391	3.036	ng	99
33) Chrysene	21.709	228	172221	3.068	ng	99
34) Bis(2-ethylhexyl)phtha...	21.574	149	58722	2.365	ng	99
36) Indeno(1,2,3-cd)pyrene	26.860	276	134795	3.014	ng	99
37) Benzo(b)fluoranthene	23.422	252	140612	3.626	ng	# 93
38) Benzo(k)fluoranthene	23.471	252	144737	3.612	ng	95
39) Benzo(a)pyrene	24.085	252	103955	3.303	ng	# 90
40) Dibenzo(a,h)anthracene	26.881	278	109209	2.968	ng	94
41) Benzo(g,h,i)perylene	27.679	276	111636	2.883	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
Data File : BN021422.D
Acq On : 29 Aug 2022 14:20
Operator : CG/JU
Sample : SSTDICC3.2
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Aug 29 15:18:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 29 14:52:01 2022
Response via : Initial Calibration



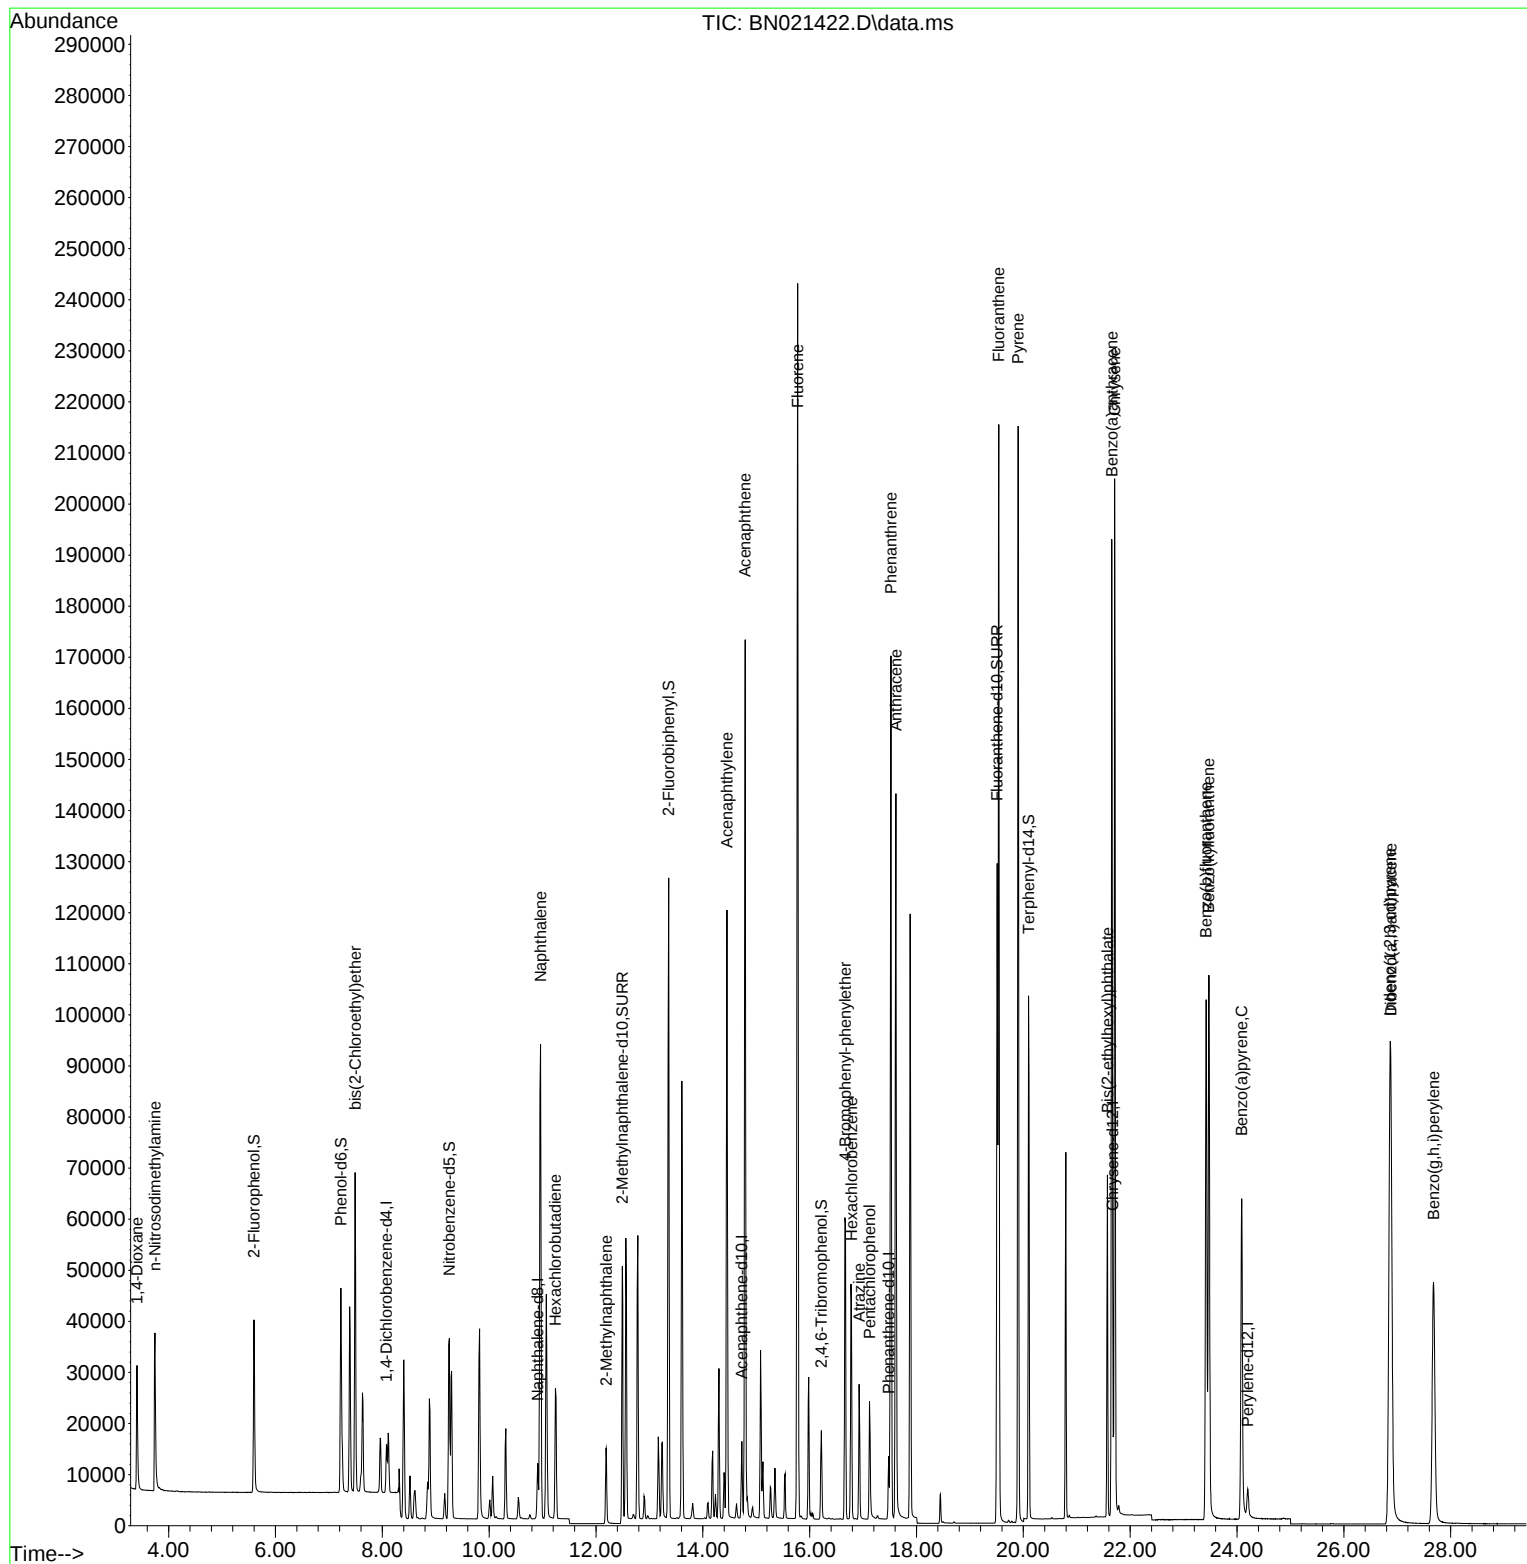




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.076 min Scan# 6
 Delta R.T. -0.007 min
 Lab File: BN021422.D
 Acq: 29 Aug 2022 14:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:152 Resp: 4691
 Ion Ratio Lower Upper
 152 100
 150 155.7 121.4 182.0
 115 61.0 48.6 72.8

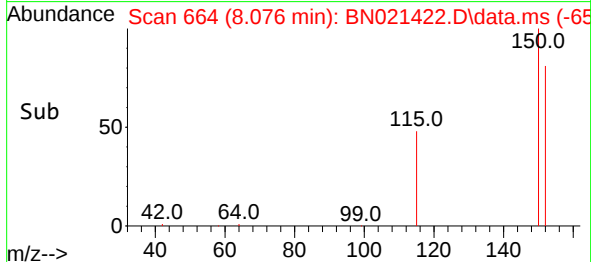

#2
 1,4-Dioxane
 Concen: 2.711 ng
 RT: 3.410 min Scan# 18
 Delta R.T. -0.000 min
 Lab File: BN021422.D
 Acq: 29 Aug 2022 14:20

Tgt Ion: 88 Resp: 17644
 Ion Ratio Lower Upper
 88 100
 43 27.1 35.8 53.8#
 58 71.5 57.1 85.7

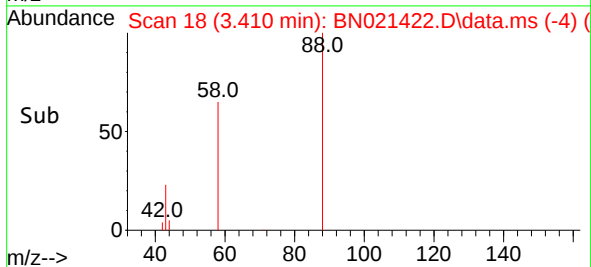

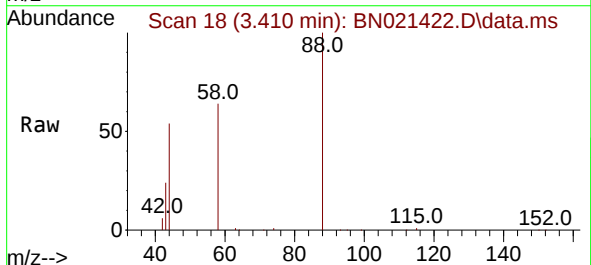




#3
 n-Nitrosodimethylamine
 Concen: 2.762 ng
 RT: 3.743 min Scan# 64
 Delta R.T. -0.007 min
 Lab File: BN021422.D
 Acq: 29 Aug 2022 14:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion: 42 Resp: 17193
 Ion Ratio Lower Upper
 42 100
 74 135.0 113.0 169.6
 44 7.3 10.5 15.7#

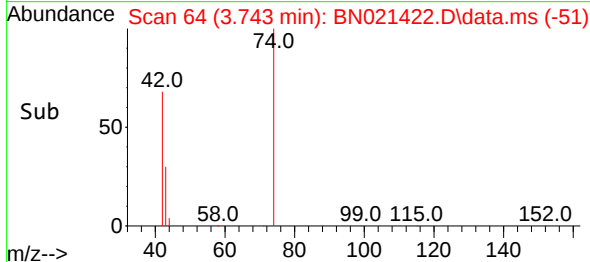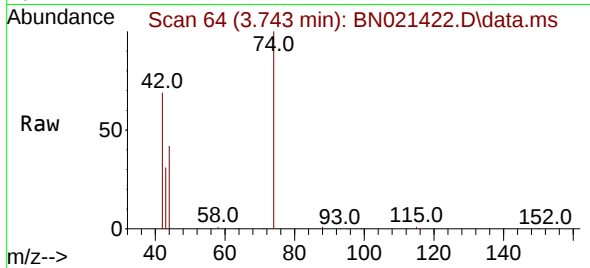

#4
 2-Fluorophenol
 Concen: 2.237 ng
 RT: 5.599 min Scan# 321
 Delta R.T. -0.000 min
 Lab File: BN021422.D
 Acq: 29 Aug 2022 14:20

Tgt Ion: 112 Resp: 28394
 Ion Ratio Lower Upper
 112 100
 64 55.8 43.5 65.3
 63 28.8 22.6 34.0


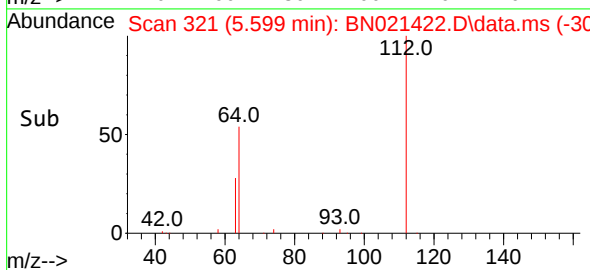

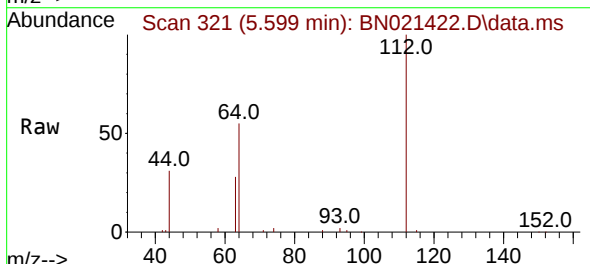




#5
Phenol-d6
Concen: 2.380 ng
RT: 7.224 min Scan# 546
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion: 99 Resp: 37872
Ion Ratio Lower Upper
99 100
42 18.3 15.5 23.3
71 31.1 24.2 36.2

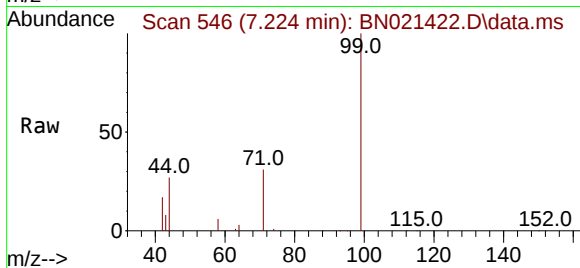

#6
bis(2-Chloroethyl)ether
Concen: 2.768 ng
RT: 7.491 min Scan# 583
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion: 93 Resp: 44071
Ion Ratio Lower Upper
93 100
63 74.6 57.8 86.8
95 32.4 25.9 38.9


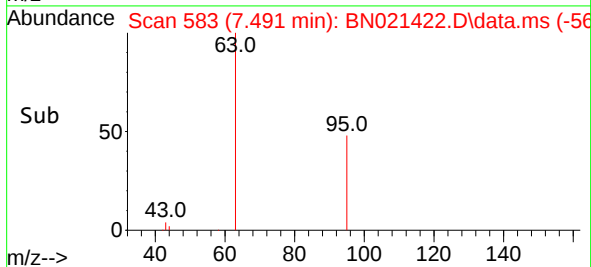

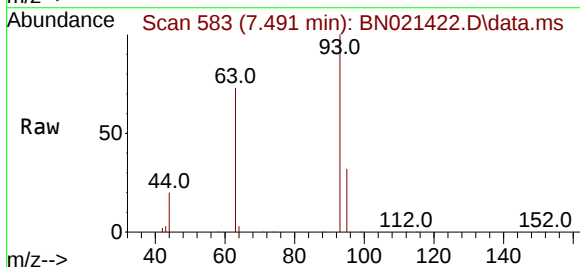




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.909 min Scan# 940
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	136	Resp:	14028
Ion Ratio	Lower	Upper	
136	100		
137	11.3	9.3	13.9
54	7.7	6.9	10.3
68	6.7	6.1	9.1

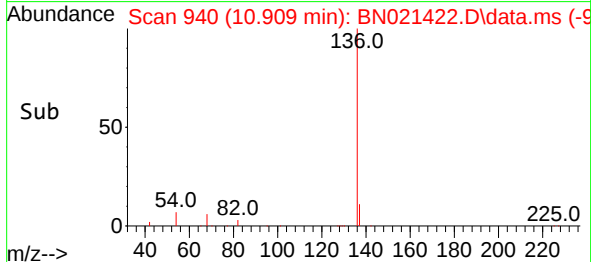

#8
Nitrobenzene-d5
Concen: 2.908 ng
RT: 9.254 min Scan# 785
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:	82	Resp:	30869
Ion Ratio	Lower	Upper	
82	100		
128	45.1	30.9	46.3
54	43.4	42.7	64.1


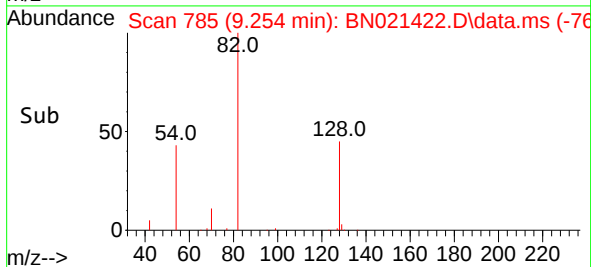

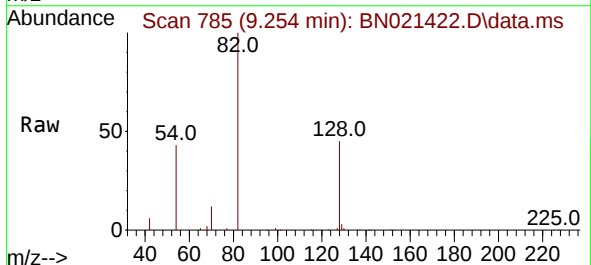




#9
Naphthalene
Concen: 2.771 ng
RT: 10.962 min Scan# 945
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:128 Resp: 127816
Ion Ratio Lower Upper
128 100
129 10.9 9.3 13.9
127 12.7 11.0 16.4



#10
Hexachlorobutadiene
Concen: 2.843 ng
RT: 11.240 min Scan# 971
Delta R.T. -0.011 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:225 Resp: 21630
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.2 76.8

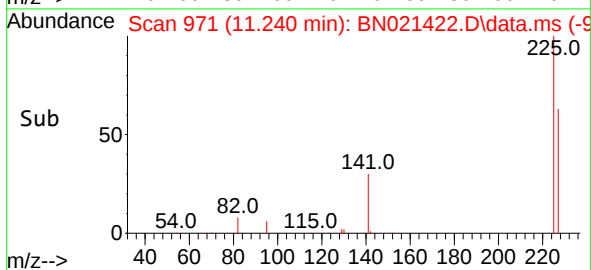






#11
2-Methylnaphthalene-d10
Concen: 4.357 ng
RT: 12.493 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:152 Resp: 103224
Ion Ratio Lower Upper
152 100
151 18.7 14.5 21.7

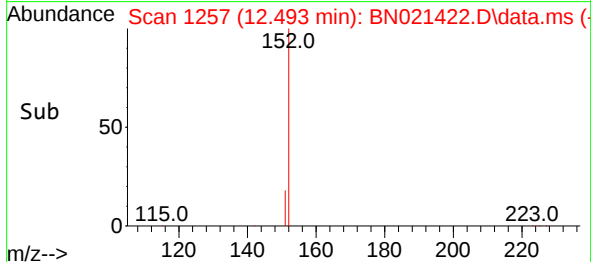

#12
2-Methylnaphthalene
Concen: 2.780 ng
RT: 12.191 min Scan# 1177
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:142 Resp: 21824
Ion Ratio Lower Upper
142 100
141 10.6 12.2 18.2#
115 2.3 7.9 11.9#

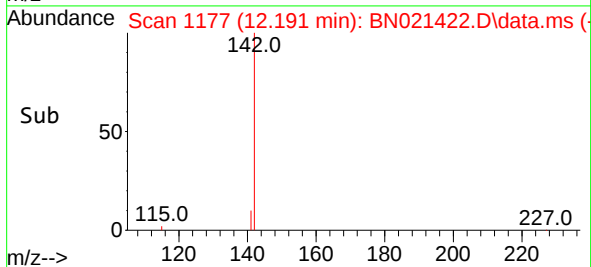

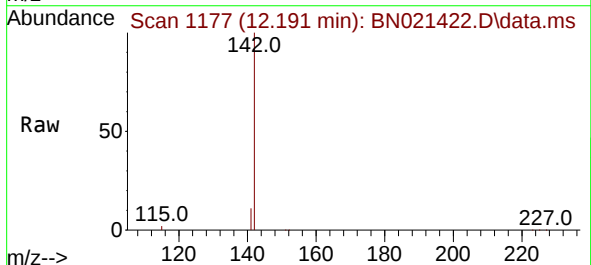




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.728 min Scan# 1468
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:164 Resp: 8049
Ion Ratio Lower Upper
164 100
162 102.9 82.2 123.4
160 49.2 39.5 59.3

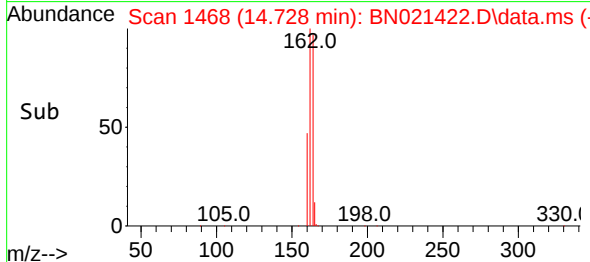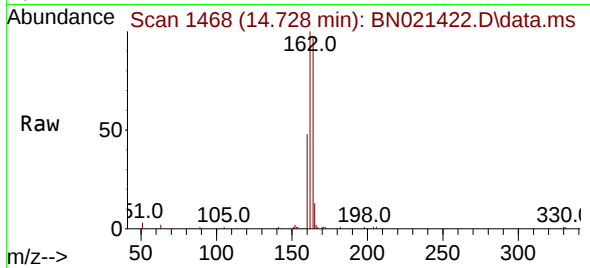

#14
2,4,6-Tribromophenol
Concen: 2.517 ng
RT: 16.218 min Scan# 1609
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:330 Resp: 9280
Ion Ratio Lower Upper
330 100
332 96.8 79.3 118.9
141 44.1 37.1 55.7

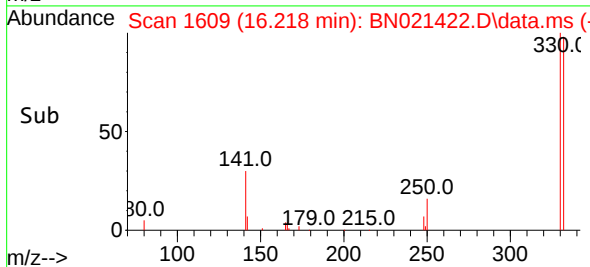

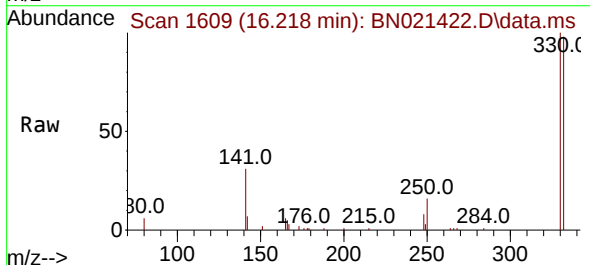




#15
2-Fluorobiphenyl
Concen: 2.918 ng
RT: 13.360 min Scan# 1340
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:172 Resp: 105040
Ion Ratio Lower Upper
172 100
171 34.1 27.8 41.6
170 22.7 18.6 28.0

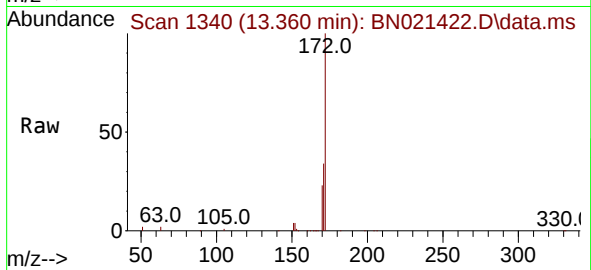

#16
Acenaphthylene
Concen: 3.156 ng
RT: 14.450 min Scan# 1442
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:152 Resp: 127349
Ion Ratio Lower Upper
152 100
151 19.3 15.4 23.2
153 12.9 10.3 15.5

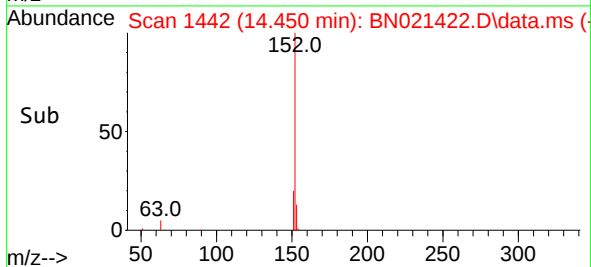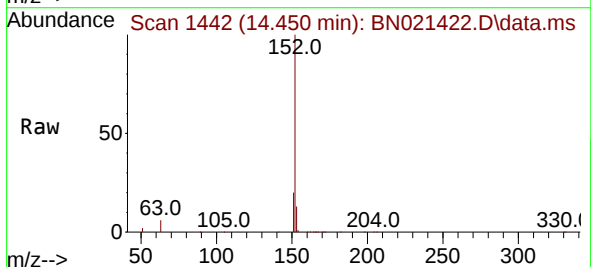



#17

Acenaphthene

Concen: 2.990 ng

RT: 14.792 min Scan# 1474

Delta R.T. -0.000 min

Lab File: BN021422.D

Acq: 29 Aug 2022 14:20

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:154 Resp: 83744

Ion Ratio Lower Upper

154 100

153 109.9 89.5 134.3

152 55.4 45.5 68.3

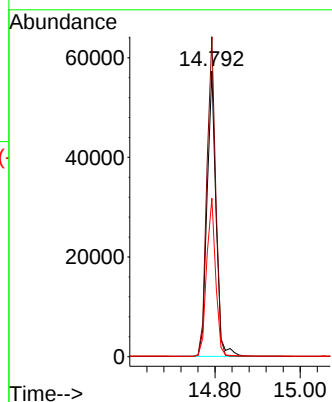

#18

Fluorene

Concen: 2.929 ng

RT: 15.776 min Scan# 1566

Delta R.T. -0.000 min

Lab File: BN021422.D

Acq: 29 Aug 2022 14:20




Tgt Ion:166 Resp: 102764


Ion Ratio Lower Upper

166 100

165 98.0 78.7 118.1

167 13.4 10.6 16.0


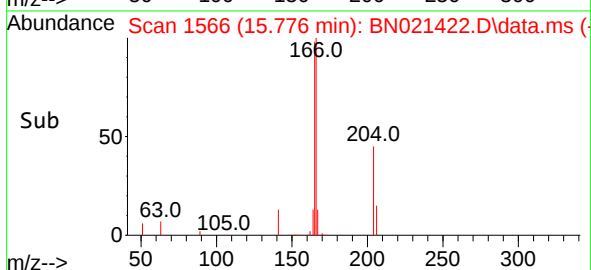






#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.480 min Scan# 1732
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:188 Resp: 15356
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.3 9.5 14.3



#21
4-Bromophenyl-phenylether
Concen: 3.004 ng
RT: 16.670 min Scan# 1653
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:248 Resp: 31586
Ion Ratio Lower Upper
248 100
250 101.3 81.8 122.6
141 43.3 38.5 57.7

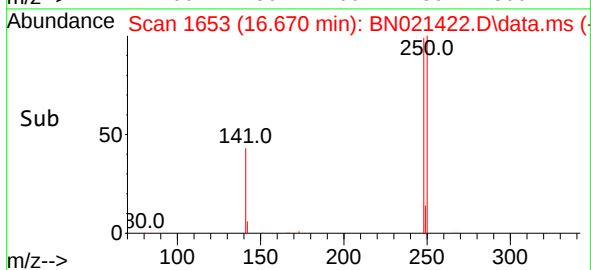






#22
Hexachlorobenzene
Concen: 2.990 ng
RT: 16.782 min Scan# 1664
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:284 Resp: 36484
Ion Ratio Lower Upper
284 100
142 41.0 32.3 48.5
249 31.1 25.4 38.2

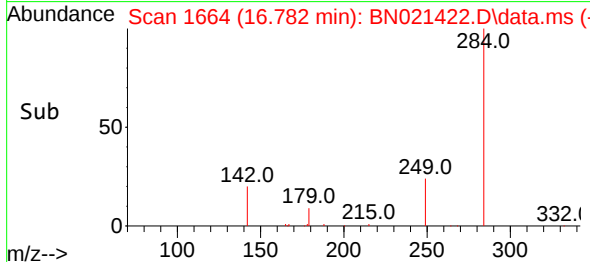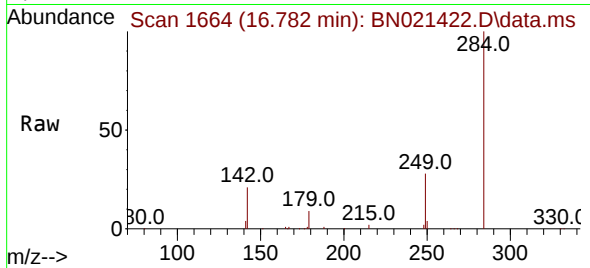

#23
Atrazine
Concen: 3.078 ng
RT: 16.926 min Scan# 1678
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:200 Resp: 20456
Ion Ratio Lower Upper
200 100
173 29.9 24.3 36.5
215 44.5 38.4 57.6


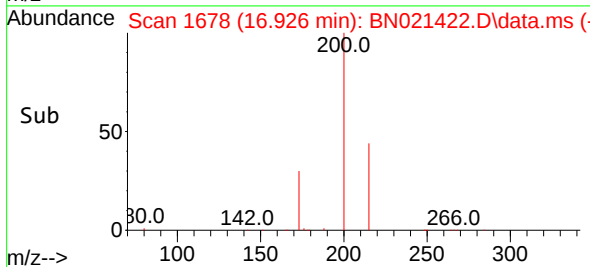

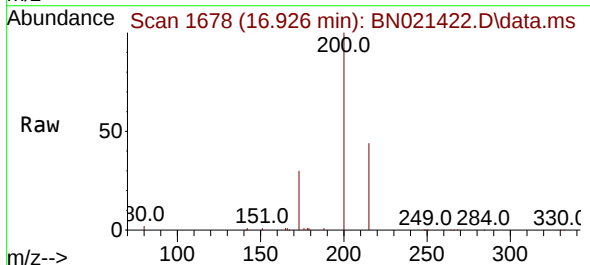


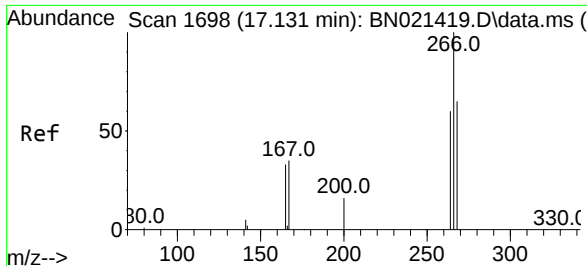

#24
 Pentachlorophenol
 Concen: 2.567 ng
 RT: 17.121 min Scan# 1697
 Delta R.T. -0.010 min
 Lab File: BN021422.D
 Acq: 29 Aug 2022 14:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:266 Resp: 10822
 Ion Ratio Lower Upper
 266 100
 264 62.0 49.0 73.6
 268 63.8 50.9 76.3

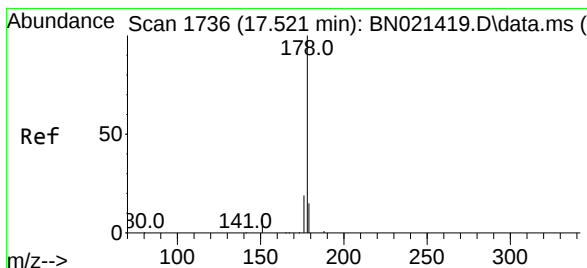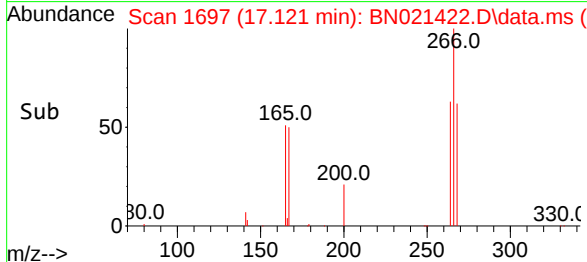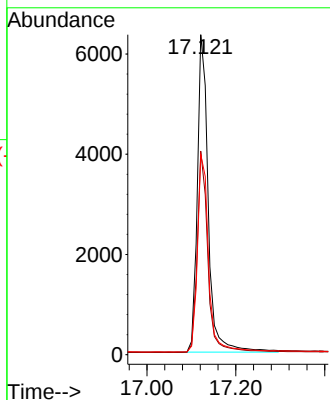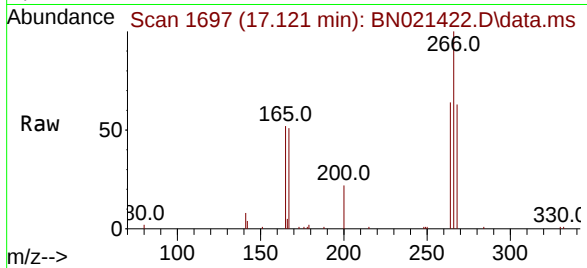

#25
 Phenanthrene
 Concen: 3.016 ng
 RT: 17.521 min Scan# 1736
 Delta R.T. -0.000 min
 Lab File: BN021422.D
 Acq: 29 Aug 2022 14:20

Tgt Ion:178 Resp: 169385
 Ion Ratio Lower Upper
 178 100
 176 19.3 15.4 23.2
 179 15.1 12.2 18.4

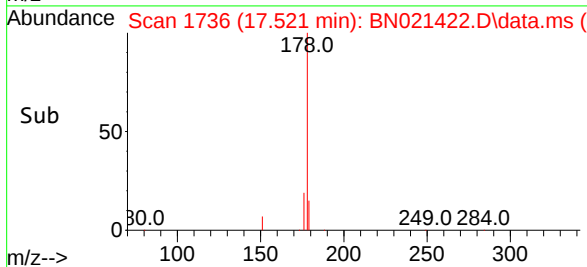
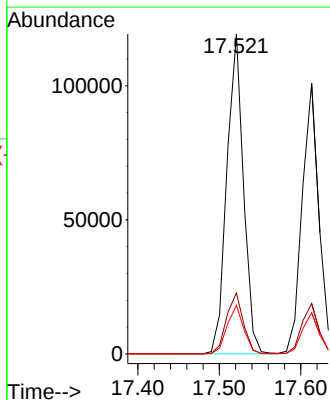
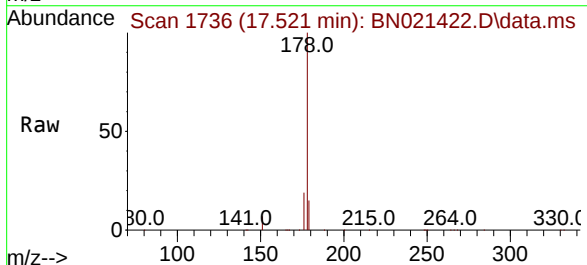




#26
 Anthracene
 Concen: 3.183 ng
 RT: 17.613 min Scan# 1745
 Delta R.T. -0.000 min
 Lab File: BN021422.D
 Acq: 29 Aug 2022 14:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:178 Resp: 146871
 Ion Ratio Lower Upper
 178 100
 176 18.7 14.6 22.0
 179 15.2 12.2 18.2

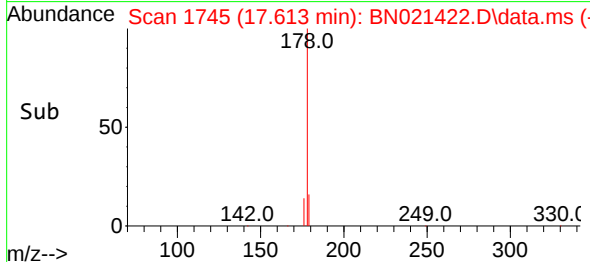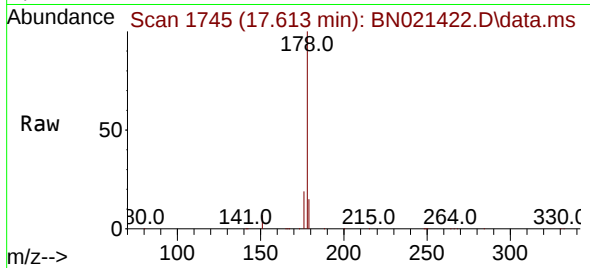

#27
 Fluoranthene-d10
 Concen: 2.879 ng
 RT: 19.510 min Scan# 2139
 Delta R.T. -0.000 min
 Lab File: BN021422.D
 Acq: 29 Aug 2022 14:20

Tgt Ion:212 Resp: 132077
 Ion Ratio Lower Upper
 212 100
 106 18.1 14.2 21.2
 104 10.1 7.8 11.6


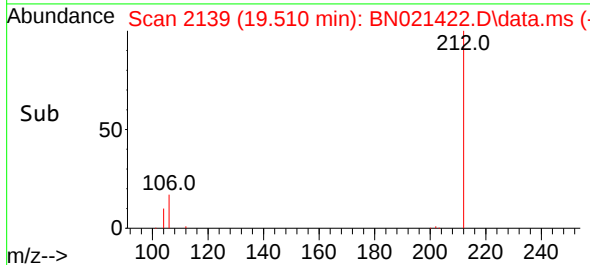

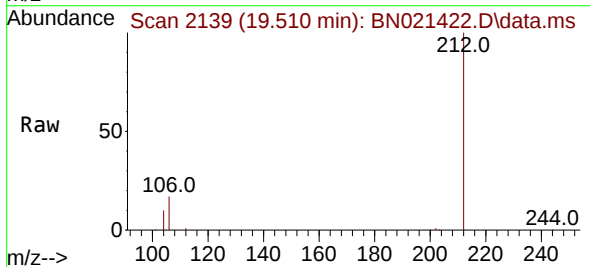




#28
Fluoranthene
Concen: 3.041 ng
RT: 19.539 min Scan# 2146
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:202 Resp: 188015
Ion Ratio Lower Upper
202 100
101 13.5 10.9 16.3
203 17.2 13.8 20.6

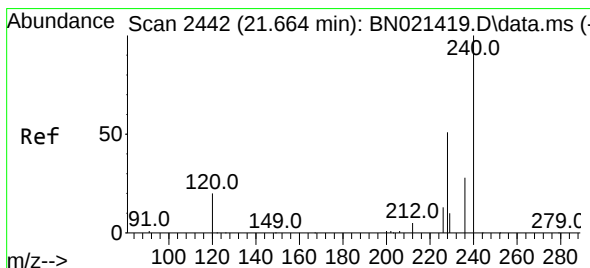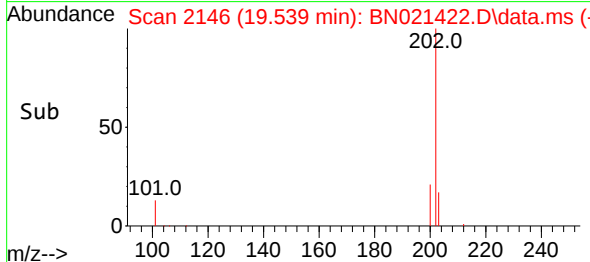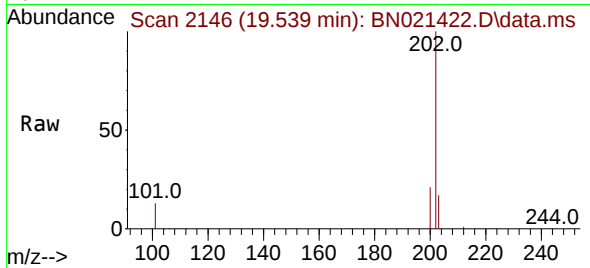

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.673 min Scan# 2443
Delta R.T. 0.009 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:240 Resp: 13605
Ion Ratio Lower Upper
240 100
120 15.2 10.2 15.4
236 27.7 22.1 33.1


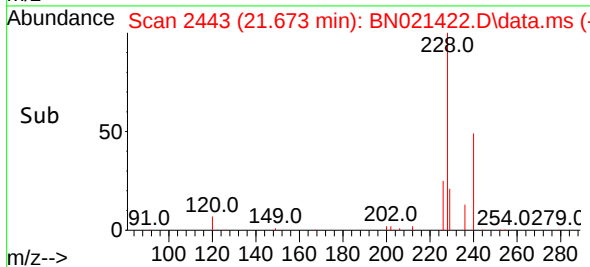

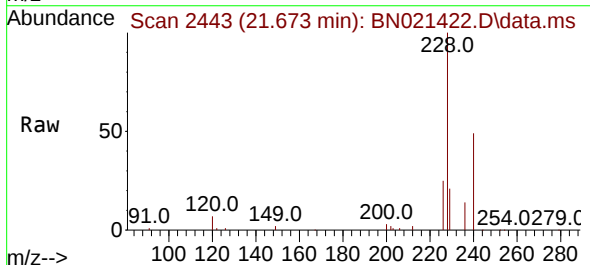




#30
Pyrene
Concen: 3.092 ng
RT: 19.902 min Scan# 211825
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:202 Resp: 211825
Ion Ratio Lower Upper
202 100
200 21.3 13.9 20.9#
203 17.9 11.9 17.9#



#31
Terphenyl-d14
Concen: 3.008 ng
RT: 20.097 min Scan# 2267
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:244 Resp: 86474
Ion Ratio Lower Upper
244 100
212 9.8 6.5 9.7#
122 21.4 9.1 13.7#

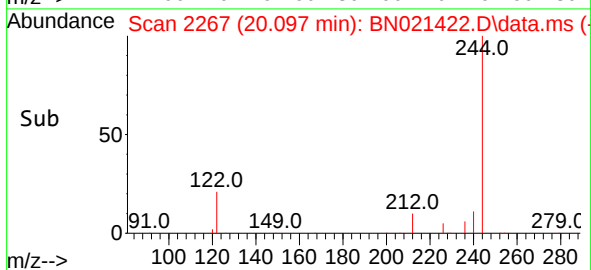






#32
Benzo(a)anthracene
Concen: 3.036 ng
RT: 21.655 min Scan# 2441
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:228 Resp: 156391
Ion Ratio Lower Upper
228 100
226 28.2 22.0 33.0
229 19.5 15.9 23.9

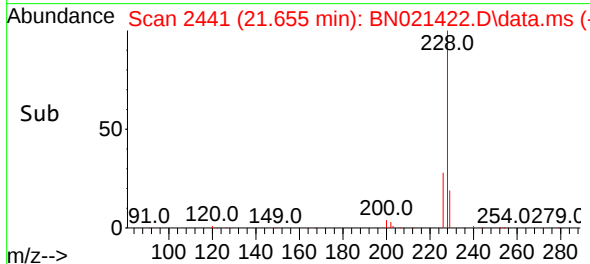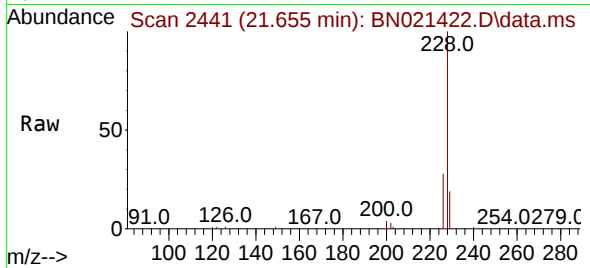

#33
Chrysene
Concen: 3.068 ng
RT: 21.709 min Scan# 2447
Delta R.T. -0.000 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:228 Resp: 172221
Ion Ratio Lower Upper
228 100
226 30.6 24.2 36.2
229 19.0 15.9 23.9

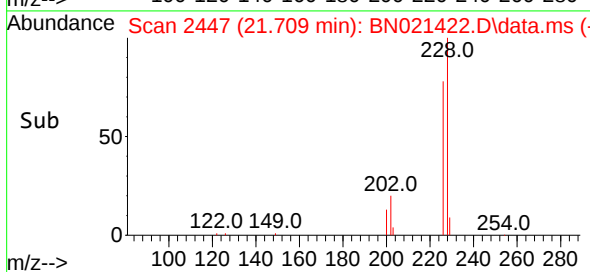

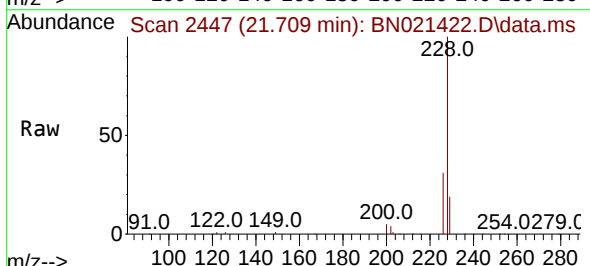




#34
Bis(2-ethylhexyl)phthalate
Concen: 2.365 ng
RT: 21.574 min Scan# 2431
Delta R.T. 0.009 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:149 Resp: 58722
Ion Ratio Lower Upper
149 100
167 25.9 21.4 32.0
279 2.4 2.2 3.2

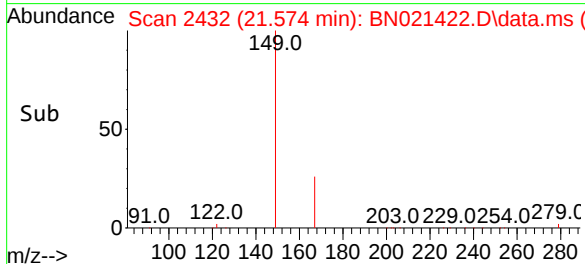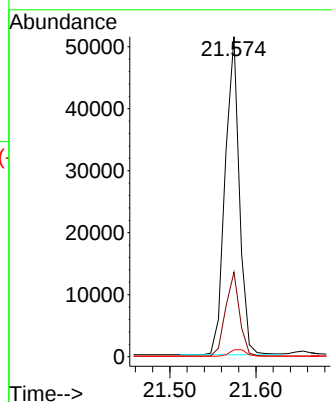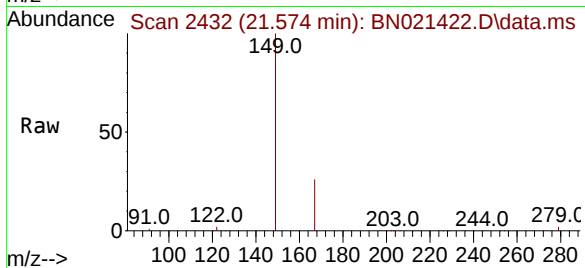

#35
Perylene-d12
Concen: 0.400 ng
RT: 24.199 min Scan# 3138
Delta R.T. 0.006 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:264 Resp: 8793
Ion Ratio Lower Upper
264 100
260 26.7 21.0 31.6
265 37.8 32.2 48.2

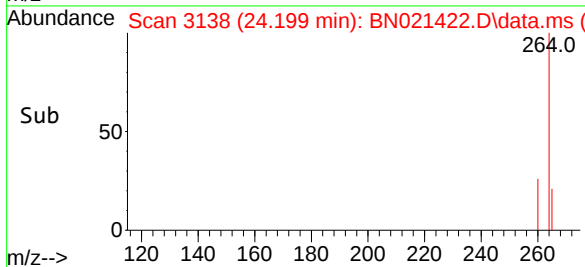
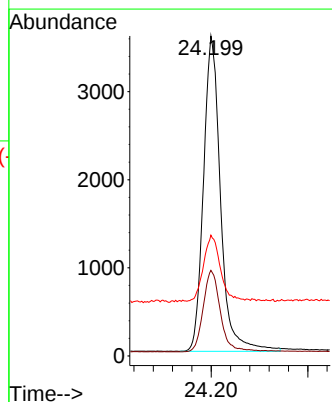
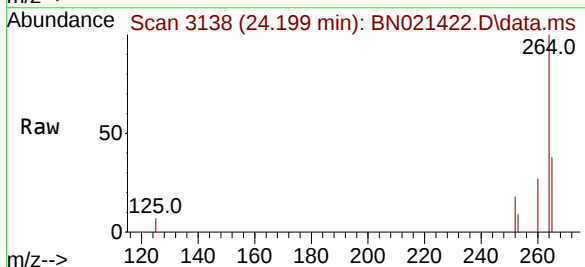




#36
Indeno(1,2,3-cd)pyrene
Concen: 3.014 ng
RT: 26.860 min Scan# 4044
Delta R.T. 0.012 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:276 Resp: 134795
Ion Ratio Lower Upper
276 100
138 33.7 27.4 41.2
277 24.8 19.9 29.9

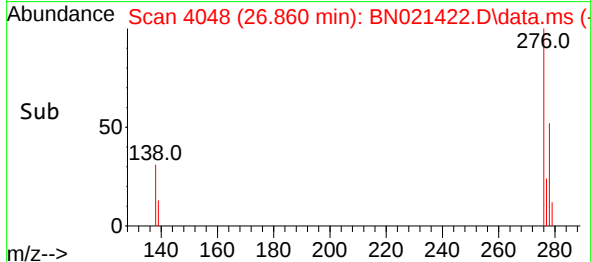

#37
Benzo(b)fluoranthene
Concen: 3.626 ng
RT: 23.422 min Scan# 2872
Delta R.T. 0.009 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:252 Resp: 140612
Ion Ratio Lower Upper
252 100
253 21.9 19.8 29.6
125 13.3 13.7 20.5#

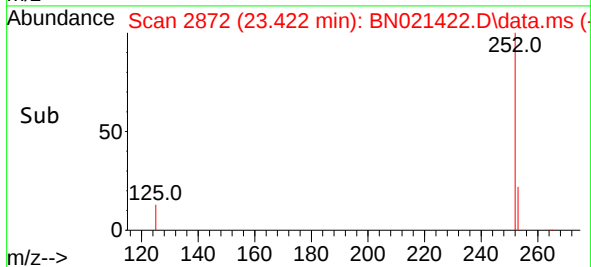

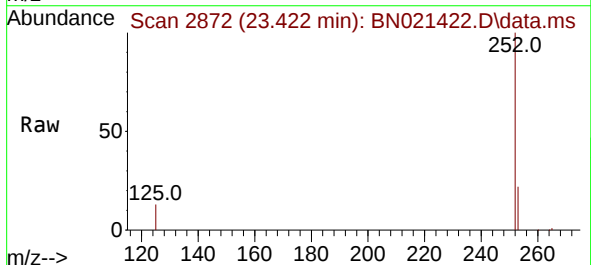




#38
Benzo(k)fluoranthene
Concen: 3.612 ng
RT: 23.471 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:252 Resp: 144737
Ion Ratio Lower Upper
252 100
253 21.8 19.5 29.3
125 13.2 12.3 18.5

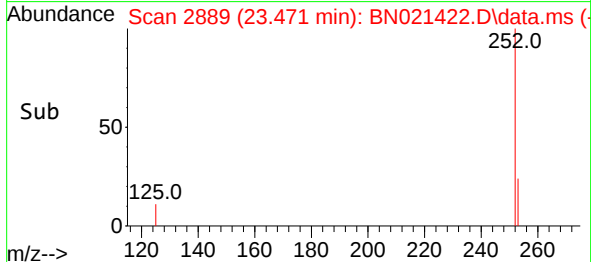

#39
Benzo(a)pyrene
Concen: 3.303 ng
RT: 24.085 min Scan# 3099
Delta R.T. 0.009 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:252 Resp: 103955
Ion Ratio Lower Upper
252 100
253 22.1 21.1 31.7
125 15.0 16.6 25.0#


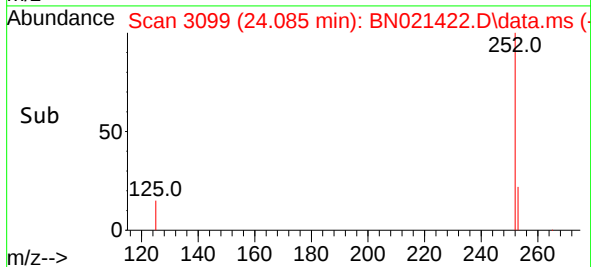

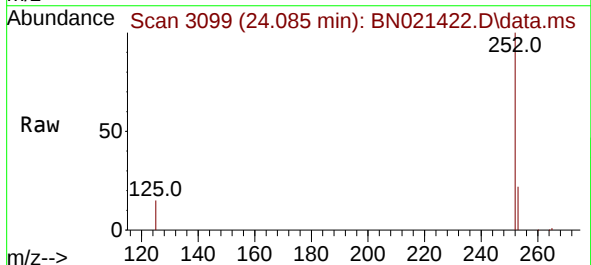




#40
Dibenzo(a,h)anthracene
Concen: 2.968 ng
RT: 26.881 min Scan# 4055
Delta R.T. 0.006 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:278 Resp: 109209
Ion Ratio Lower Upper
278 100
139 22.7 21.8 32.6
279 23.6 20.4 30.6



#41
Benzo(g,h,i)perylene
Concen: 2.883 ng
RT: 27.679 min Scan# 4328
Delta R.T. 0.009 min
Lab File: BN021422.D
Acq: 29 Aug 2022 14:20

Tgt Ion:276 Resp: 111636
Ion Ratio Lower Upper
276 100
277 23.8 19.7 29.5
138 28.9 23.7 35.5

