

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
 Data File : BN021431.D
 Acq On : 29 Aug 2022 20:43
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Aug 30 01:16:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 29 16:30:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.076	152	5626	0.400	ng	0.00
7) Naphthalene-d8	10.909	136	17479	0.400	ng	0.00
13) Acenaphthene-d10	14.728	164	9398	0.400	ng	0.00
19) Phenanthrene-d10	17.480	188	19312	0.400	ng	0.00
29) Chrysene-d12	21.664	240	13986	0.400	ng	# 0.00
35) Perylene-d12	24.185	264	9730	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.599	112	4034	0.366	ng	0.00
5) Phenol-d6	7.224	99	5009	0.357	ng	0.00
8) Nitrobenzene-d5	9.254	82	4139	0.351	ng	0.00
11) 2-Methylnaphthalene-d10	12.493	152	14350	0.364	ng	0.00
14) 2,4,6-Tribromophenol	16.218	330	954	0.309	ng	0.00
15) 2-Fluorobiphenyl	13.360	172	15284	0.372	ng	0.00
27) Fluoranthene-d10	19.506	212	17216	0.347	ng	0.00
31) Terphenyl-d14	20.097	244	11973	0.381	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.410	88	2623	0.373	ng	# 87
3) n-Nitrosodimethylamine	3.750	42	2396	0.378	ng	92
6) bis(2-Chloroethyl)ether	7.491	93	6614	0.375	ng	98
9) Naphthalene	10.962	128	19012	0.367	ng	99
10) Hexachlorobutadiene	11.240	225	3308	0.369	ng	# 99
12) 2-Methylnaphthalene	12.191	142	2155	0.377	ng	# 96
16) Acenaphthylene	14.451	152	15128	0.343	ng	100
17) Acenaphthene	14.793	154	11367	0.366	ng	100
18) Fluorene	15.776	166	13698	0.358	ng	100
21) 4-Bromophenyl-phenylether	16.670	248	4278	0.354	ng	99
22) Hexachlorobenzene	16.783	284	5355	0.362	ng	99
23) Atrazine	16.926	200	2251	0.319	ng	96
24) Pentachlorophenol	17.131	266	930	0.412	ng	99
25) Phenanthrene	17.521	178	23875	0.358	ng	100
26) Anthracene	17.613	178	18027	0.340	ng	99
28) Fluoranthene	19.535	202	24222	0.350	ng	100
30) Pyrene	19.898	202	26676	0.358	ng	95
32) Benzo(a)anthracene	21.646	228	16592	0.341	ng	100
33) Chrysene	21.700	228	21463	0.370	ng	99
34) Bis(2-ethylhexyl)phtha...	21.566	149	6846	0.349	ng	98
36) Indeno(1,2,3-cd)pyrene	26.843	276	15692	0.357	ng	100
37) Benzo(b)fluoranthene	23.410	252	16761	0.349	ng	97
38) Benzo(k)fluoranthene	23.460	252	16508	0.342	ng	98
39) Benzo(a)pyrene	24.074	252	11870	0.355	ng	98
40) Dibenzo(a,h)anthracene	26.869	278	12648	0.358	ng	96
41) Benzo(g,h,i)perylene	27.661	276	13096	0.338	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
Data File : BN021431.D
Acq On : 29 Aug 2022 20:43
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Quant Time: Aug 30 01:16:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 29 16:30:43 2022
Response via : Initial Calibration

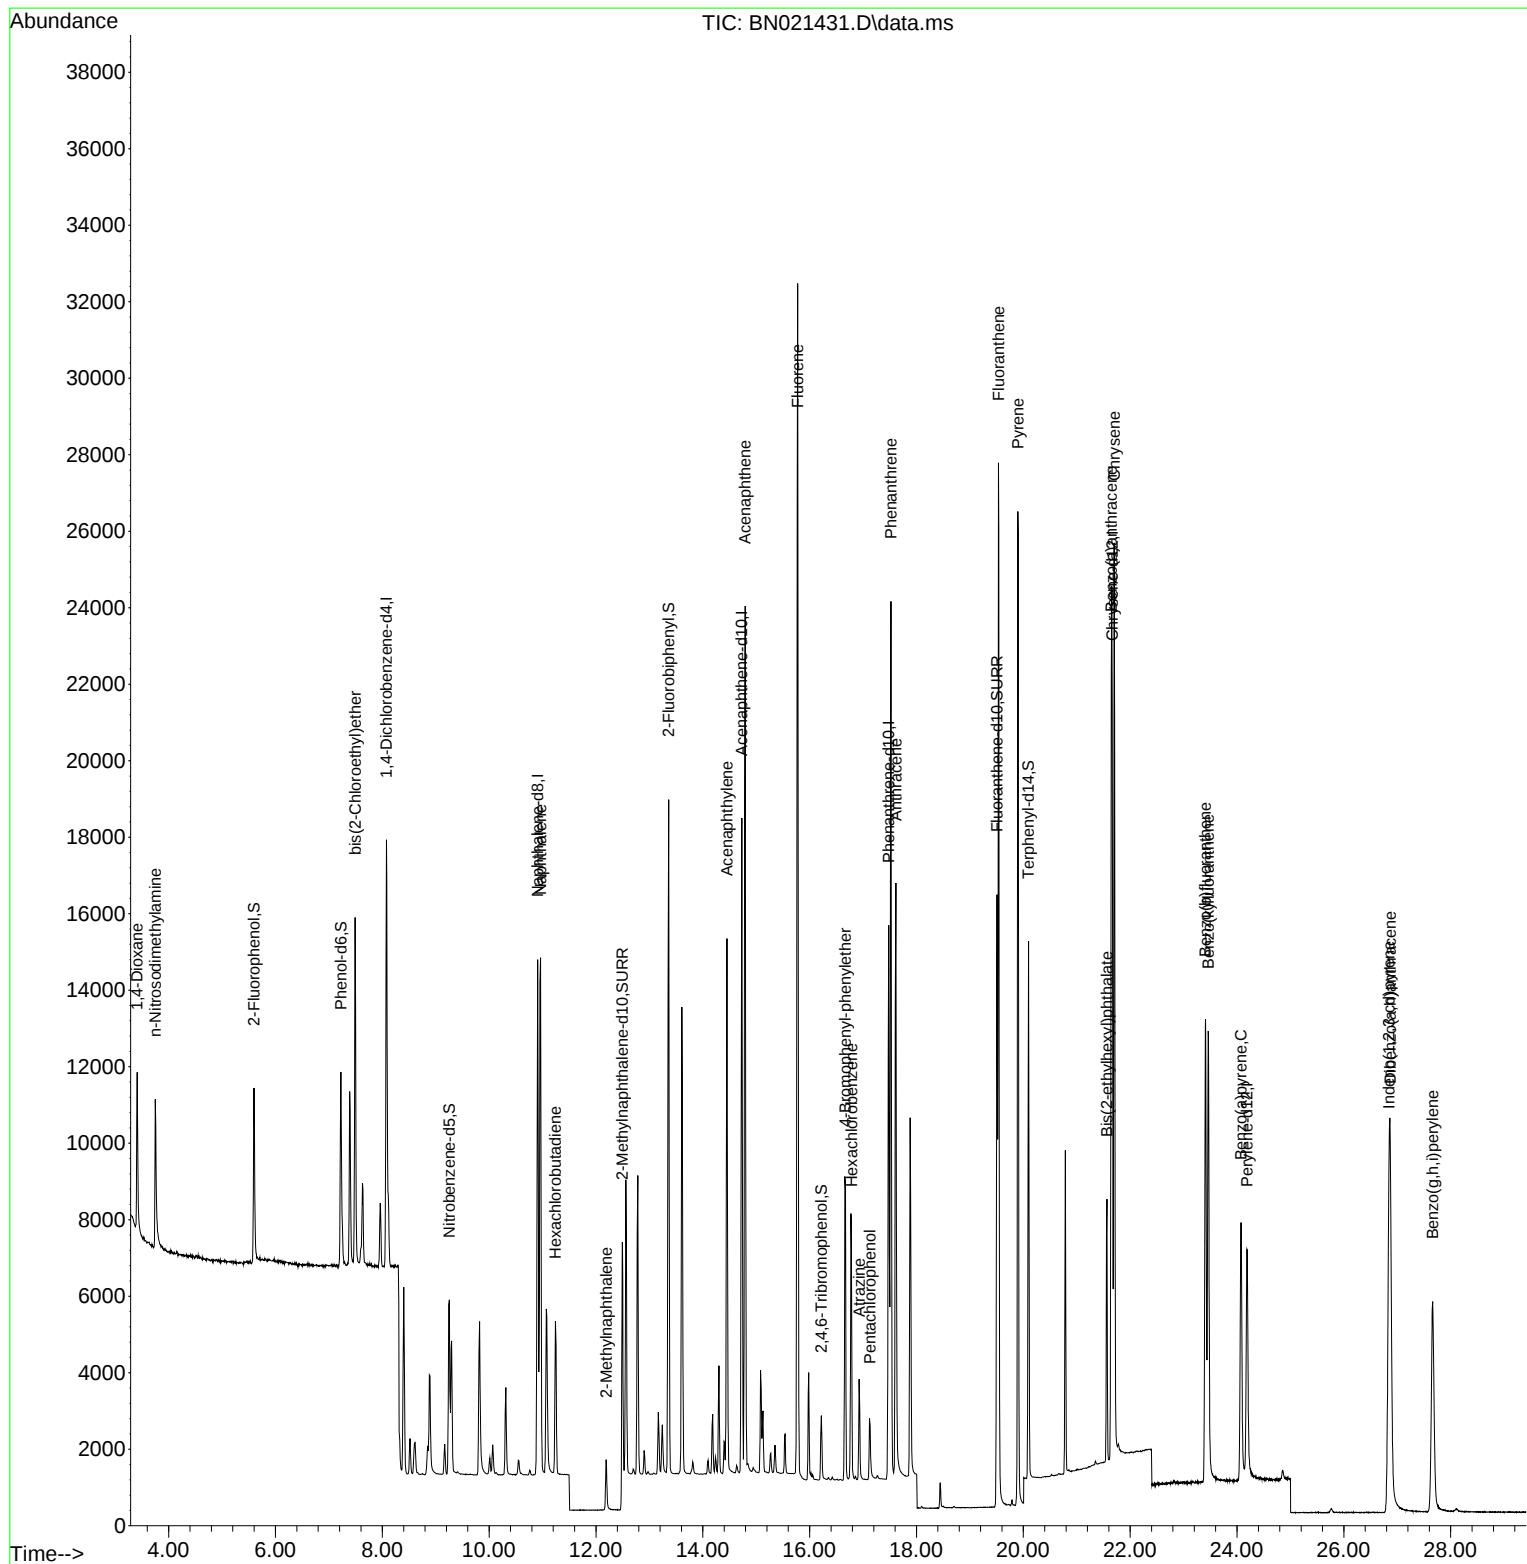





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.076 min Scan# 665
 Delta R.T. -0.007 min
 Lab File: BN021431.D
 Acq: 29 Aug 2022 20:43

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC



Tgt Ion:152 Resp: 5626




Ion	Ratio	Lower	Upper
152	100		
150	157.2	121.4	182.0
115	62.4	48.6	72.8

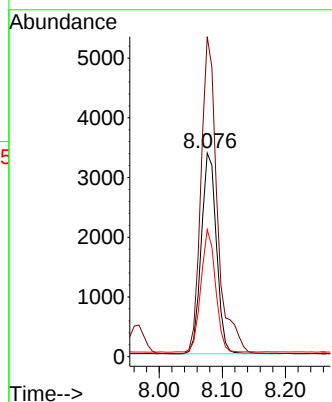

#2
 1,4-Dioxane
 Concen: 0.373 ng
 RT: 3.410 min Scan# 18
 Delta R.T. 0.000 min
 Lab File: BN021431.D
 Acq: 29 Aug 2022 20:43

Tgt Ion: 88 Resp: 2623

Ion	Ratio	Lower	Upper
88	100		
43	28.1	35.8	53.8#
58	75.0	57.1	85.7

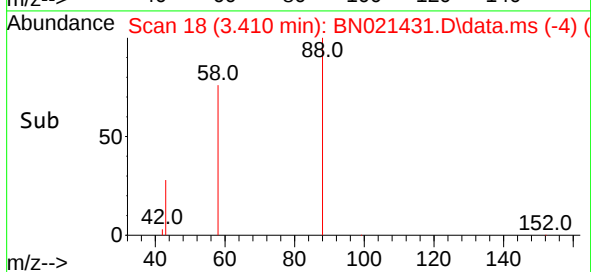
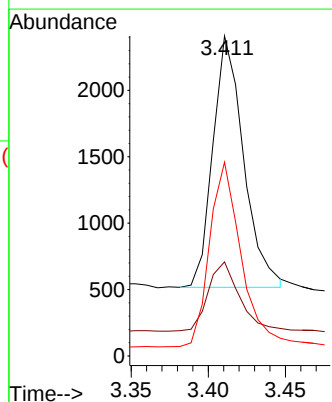





#3
n-Nitrosodimethylamine
Concen: 0.378 ng
RT: 3.750 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 42 Resp: 2396
Ion Ratio Lower Upper
42 100
74 131.3 113.0 169.6
44 11.6 10.5 15.7

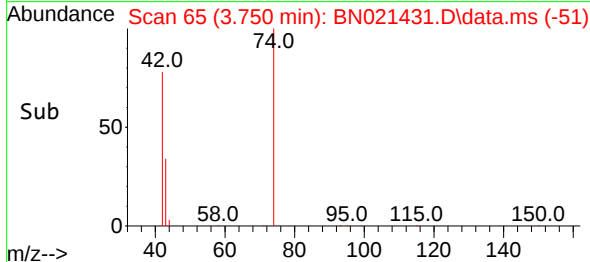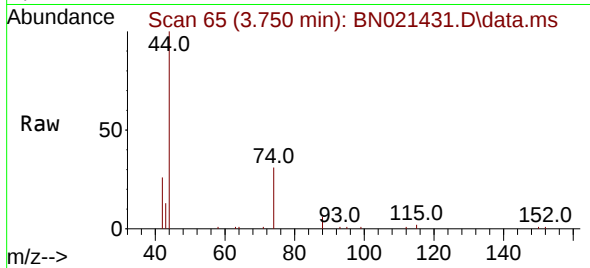

#4
2-Fluorophenol
Concen: 0.366 ng
RT: 5.599 min Scan# 321
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion: 112 Resp: 4034
Ion Ratio Lower Upper
112 100
64 56.0 43.5 65.3
63 29.3 22.6 34.0

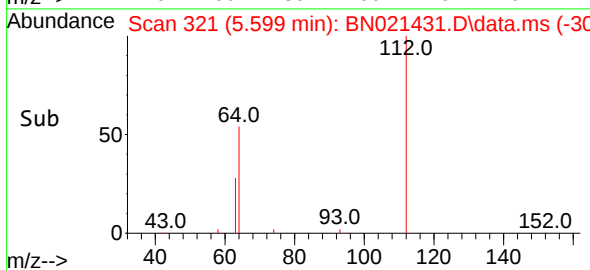

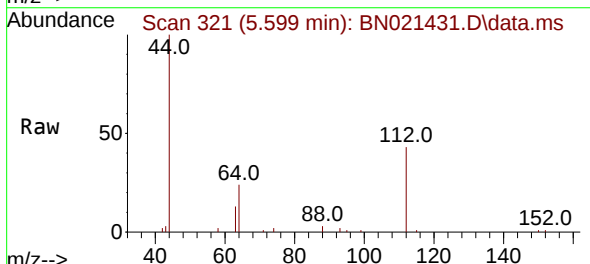




#5
Phenol-d6
Concen: 0.357 ng
RT: 7.224 min Scan# 546
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	99	Resp:	5009
Ion	Ratio	Lower	Upper
99	100		
42	18.7	15.5	23.3
71	31.4	24.2	36.2

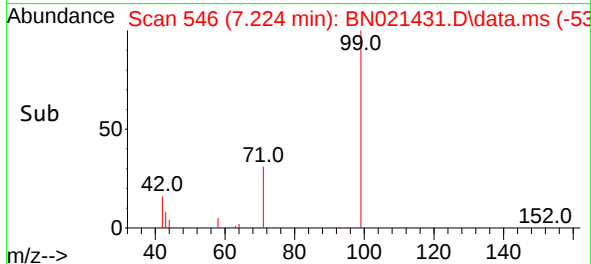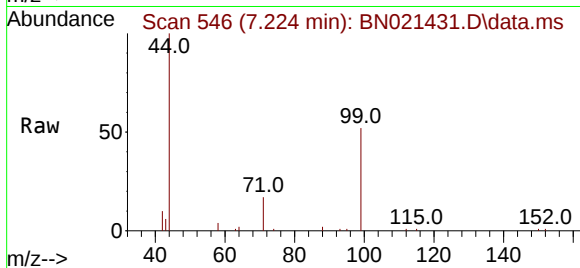

#6
bis(2-Chloroethyl)ether
Concen: 0.375 ng
RT: 7.491 min Scan# 583
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:	93	Resp:	6614
Ion	Ratio	Lower	Upper
93	100		
63	75.2	57.8	86.8
95	32.5	25.9	38.9


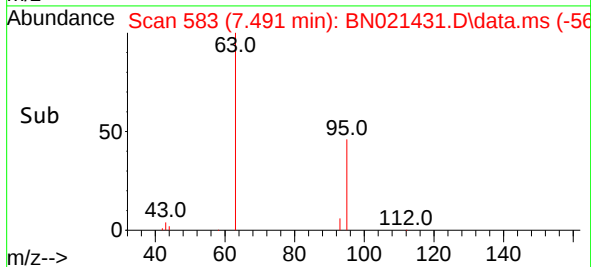

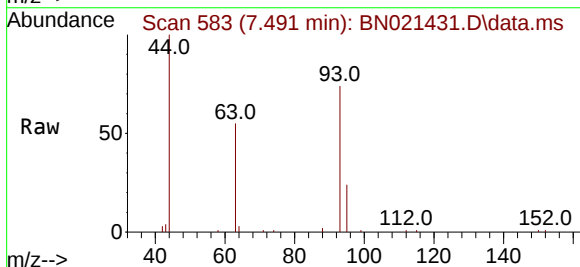




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.909 min Scan# 940
Delta R.T. -0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	17479
Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.3	13.9
54	7.3	6.9	10.3
68	6.5	6.1	9.1

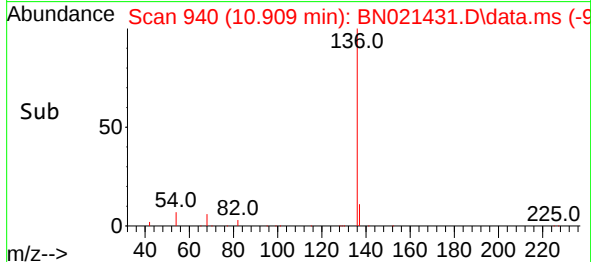

#8
Nitrobenzene-d5
Concen: 0.351 ng
RT: 9.254 min Scan# 785
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:	82	Resp:	4139
Ion	Ratio	Lower	Upper
82	100		
128	46.1	30.9	46.3
54	45.2	42.7	64.1

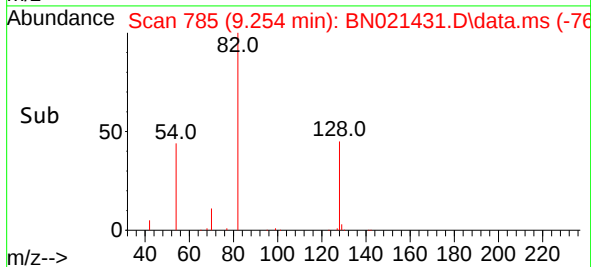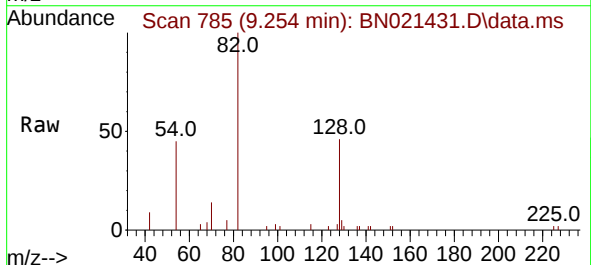

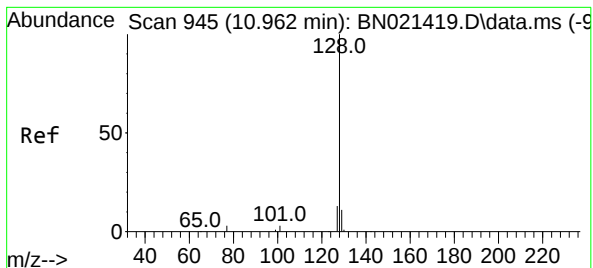

#9

Naphthalene

Concen: 0.367 ng

RT: 10.962 min Scan# 945

Delta R.T. 0.000 min

Lab File: BN021431.D

Acq: 29 Aug 2022 20:43





Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:128	Resp:	19012
Ion Ratio	Lower	Upper
128	100	
129	11.3	9.3 13.9
127	13.0	11.0 16.4

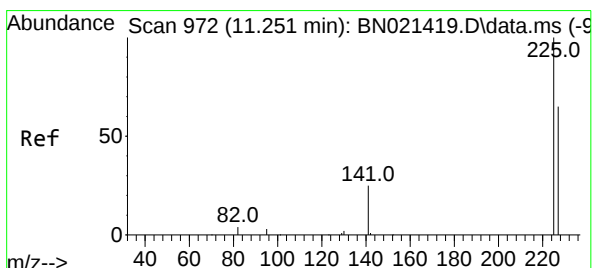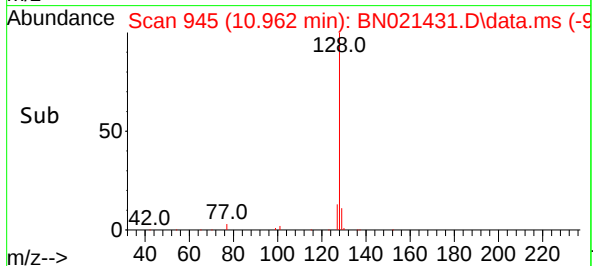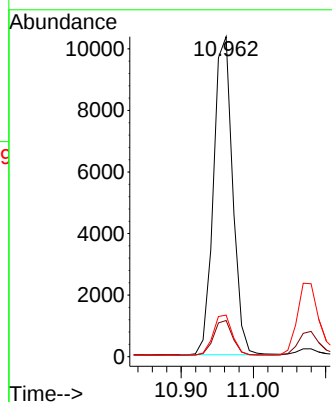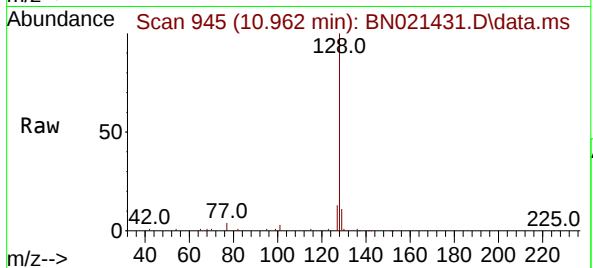

#10

Hexachlorobutadiene

Concen: 0.369 ng




RT: 11.240 min Scan# 971

Delta R.T. -0.011 min

Lab File: BN021431.D

Acq: 29 Aug 2022 20:43

Tgt Ion:225	Resp:	3308
Ion Ratio	Lower	Upper
225	100	
223	0.0	0.0 0.0
227	64.5	51.2 76.8

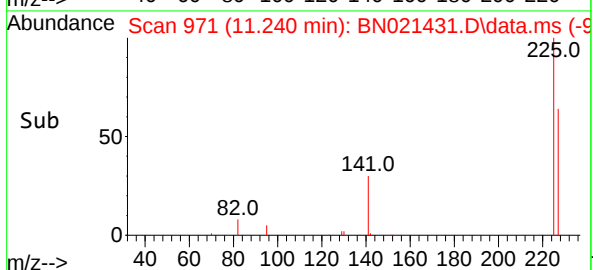

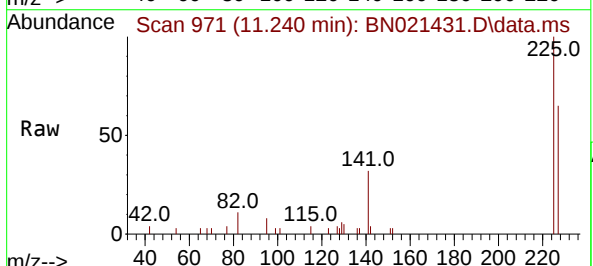




#11
2-Methylnaphthalene-d10
Concen: 0.364 ng
RT: 12.493 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 14350
Ion Ratio Lower Upper
152 100
151 19.2 14.5 21.7

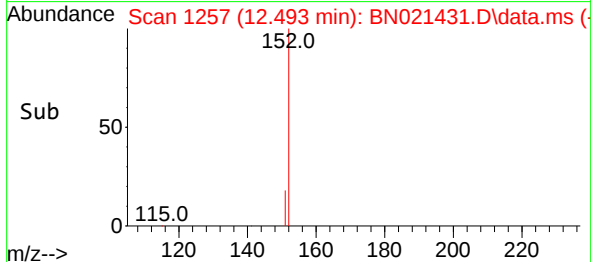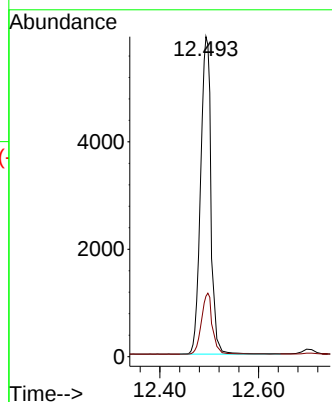

#12
2-Methylnaphthalene
Concen: 0.377 ng
RT: 12.191 min Scan# 1177
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:142 Resp: 2155
Ion Ratio Lower Upper
142 100
141 14.1 12.2 18.2
115 7.6 7.9 11.9#

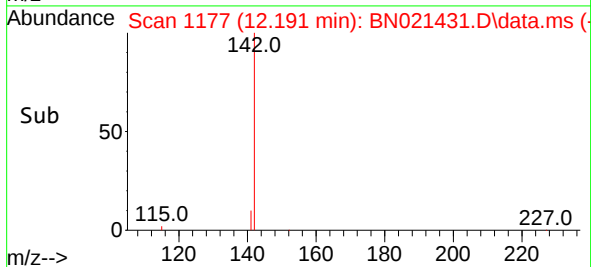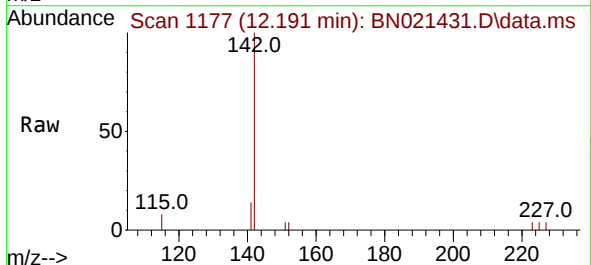



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.728 min Scan# 1468

Delta R.T. 0.000 min

Lab File: BN021431.D

Acq: 29 Aug 2022 20:43

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:164 Resp: 9398

Ion Ratio Lower Upper

164 100

162 102.5 82.2 123.4

160 50.6 39.5 59.3

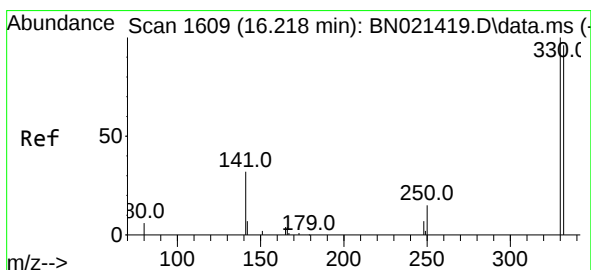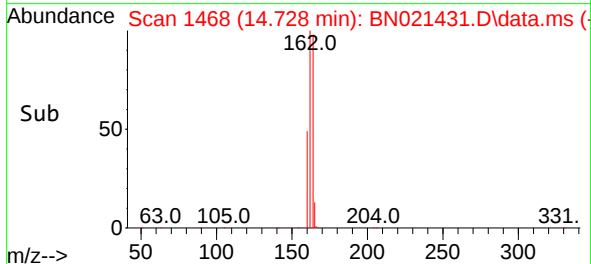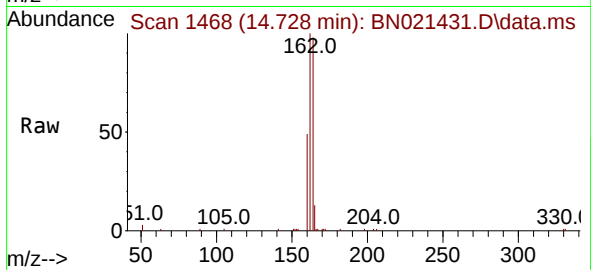

#14

2,4,6-Tribromophenol

Concen: 0.309 ng

RT: 16.218 min Scan# 1609

Delta R.T. 0.000 min

Lab File: BN021431.D

Acq: 29 Aug 2022 20:43




Tgt Ion:330 Resp: 954

Ion Ratio Lower Upper

330 100

332 96.6 79.3 118.9

141 44.5 37.1 55.7



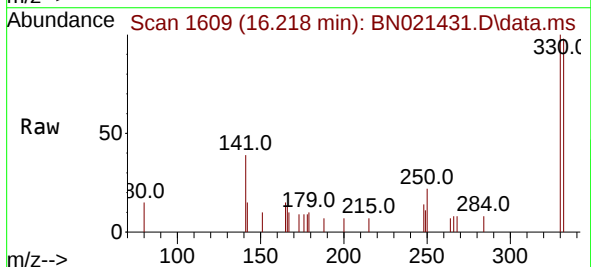




#15
2-Fluorobiphenyl
Concen: 0.372 ng
RT: 13.360 min Scan# 1340
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172 Resp: 15284
Ion Ratio Lower Upper
172 100
171 34.2 27.8 41.6
170 23.1 18.6 28.0

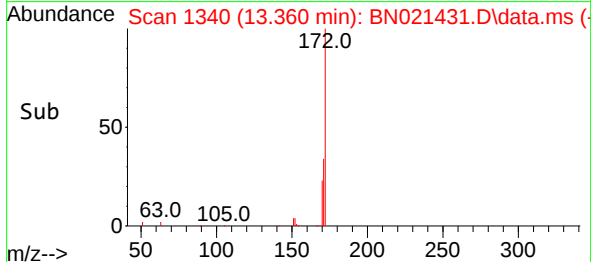

#16
Acenaphthylene
Concen: 0.343 ng
RT: 14.451 min Scan# 1442
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:152 Resp: 15128
Ion Ratio Lower Upper
152 100
151 19.3 15.4 23.2
153 13.0 10.3 15.5

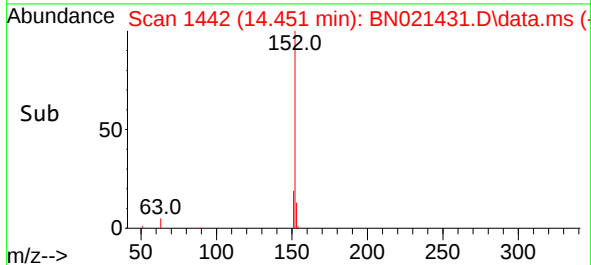

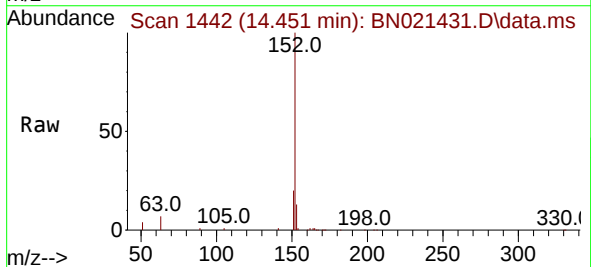




#17
Acenaphthene
Concen: 0.366 ng
RT: 14.793 min Scan# 1474
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 11367
Ion Ratio Lower Upper
154 100
153 112.0 89.5 134.3
152 57.9 45.5 68.3

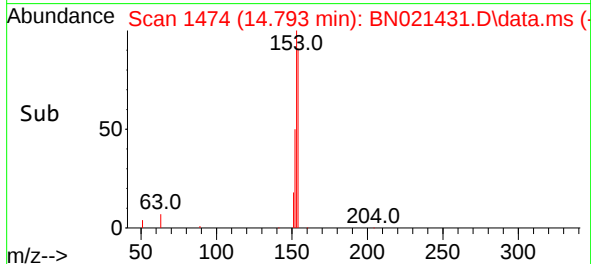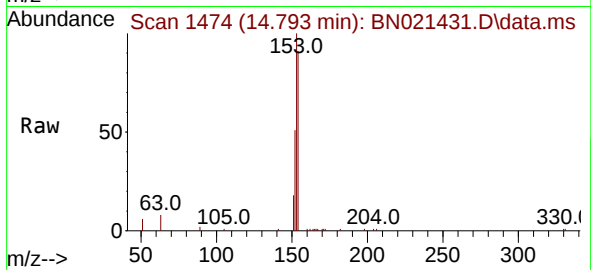

#18
Fluorene
Concen: 0.358 ng
RT: 15.776 min Scan# 1566
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:166 Resp: 13698
Ion Ratio Lower Upper
166 100
165 98.9 78.7 118.1
167 13.3 10.6 16.0


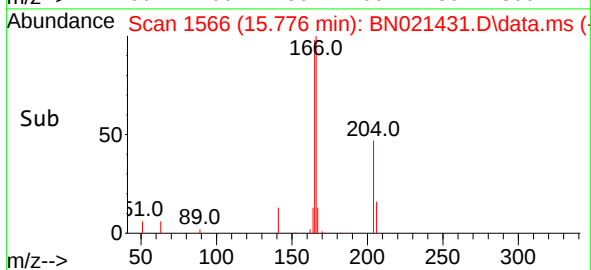

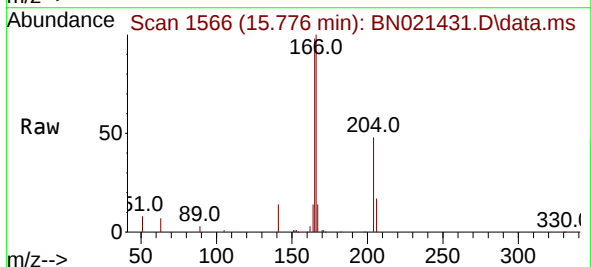




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.480 min Scan# 1732
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:188 Resp: 19312
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.9 9.5 14.3

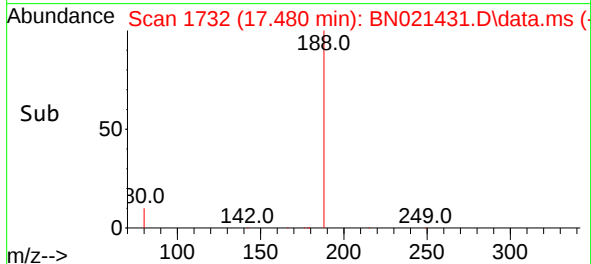

#21
4-Bromophenyl-phenylether
Concen: 0.354 ng
RT: 16.670 min Scan# 1653
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:248 Resp: 4278
Ion Ratio Lower Upper
248 100
250 102.6 81.8 122.6
141 47.2 38.5 57.7

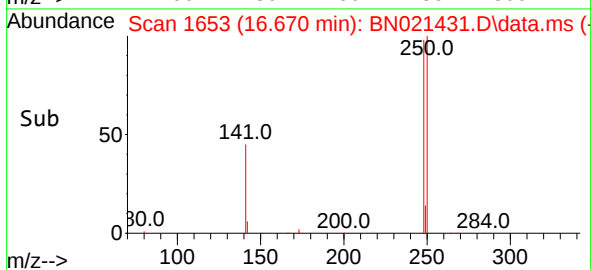

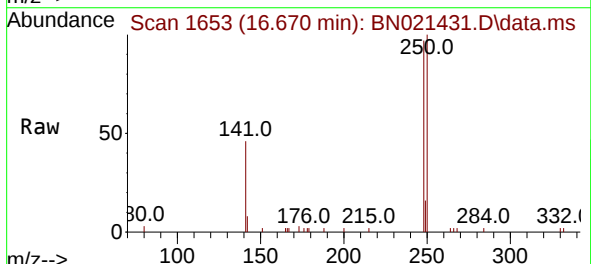




#22
Hexachlorobenzene
Concen: 0.362 ng
RT: 16.783 min Scan# 1664
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:284 Resp: 5355
Ion Ratio Lower Upper
284 100
142 41.5 32.3 48.5
249 31.5 25.4 38.2

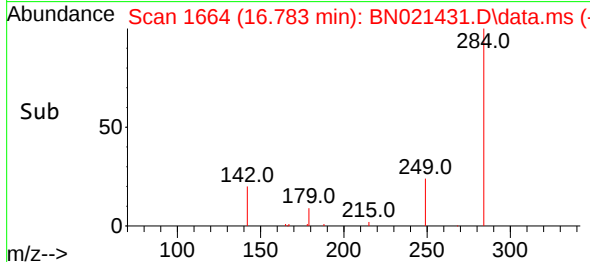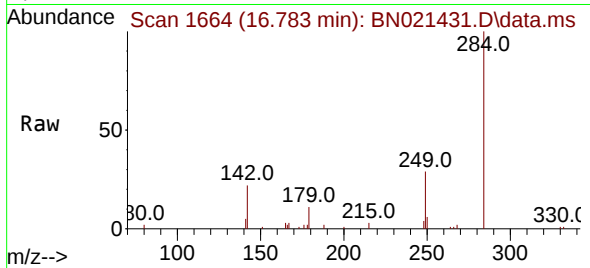

#23
Atrazine
Concen: 0.319 ng
RT: 16.926 min Scan# 1678
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:200 Resp: 2251
Ion Ratio Lower Upper
200 100
173 32.8 24.3 36.5
215 45.9 38.4 57.6

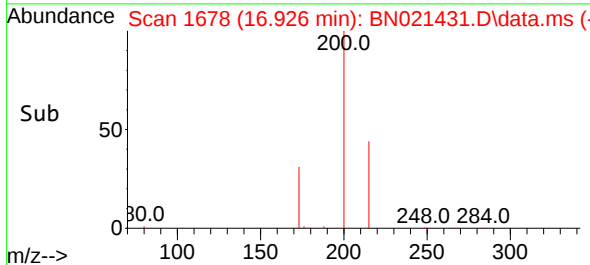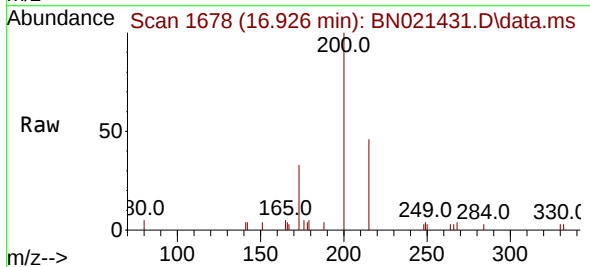

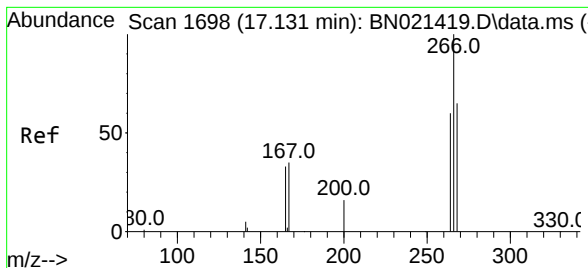

#24

Pentachlorophenol

Concen: 0.412 ng

RT: 17.131 min Scan# 1698

Delta R.T. 0.000 min

Lab File: BN021431.D

Acq: 29 Aug 2022 20:43

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:266 Resp: 930

Ion Ratio Lower Upper

266 100

264 60.5 49.0 73.6

268 64.5 50.9 76.3

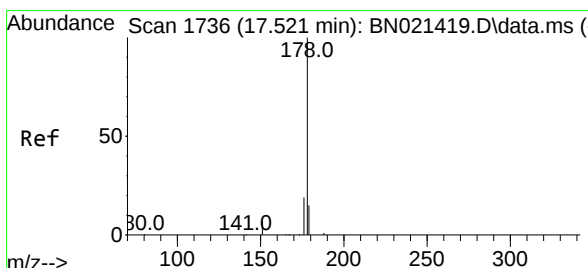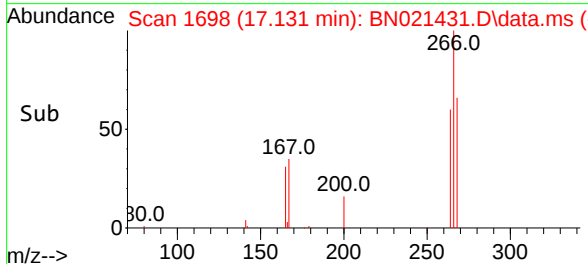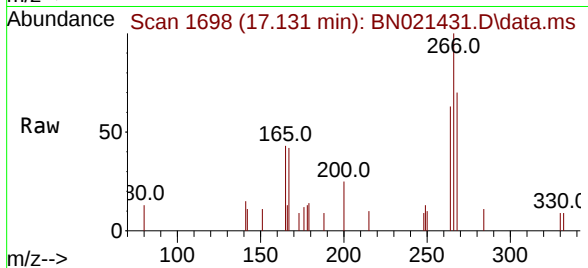

#25

Phenanthrene

Concen: 0.358 ng

RT: 17.521 min Scan# 1736

Delta R.T. 0.000 min

Lab File: BN021431.D

Acq: 29 Aug 2022 20:43




Tgt Ion:178 Resp: 23875

Ion Ratio Lower Upper

178 100

176 19.5 15.4 23.2

179 15.3 12.2 18.4

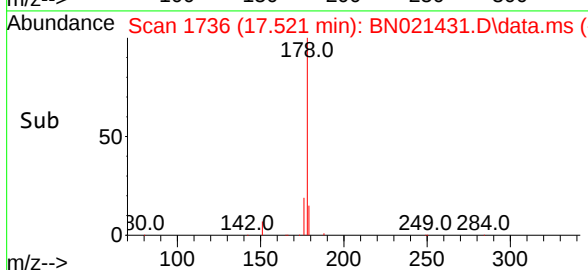

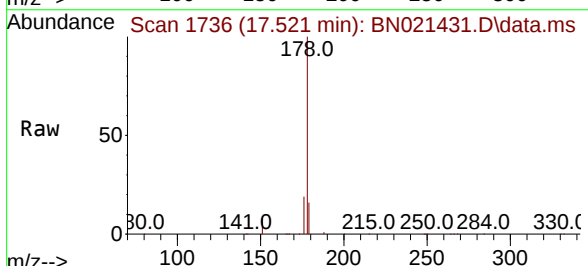




#26
 Anthracene
 Concen: 0.340 ng
 RT: 17.613 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN021431.D
 Acq: 29 Aug 2022 20:43




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:178 Resp: 18027
 Ion Ratio Lower Upper
 178 100
 176 18.5 14.6 22.0
 179 15.4 12.2 18.2

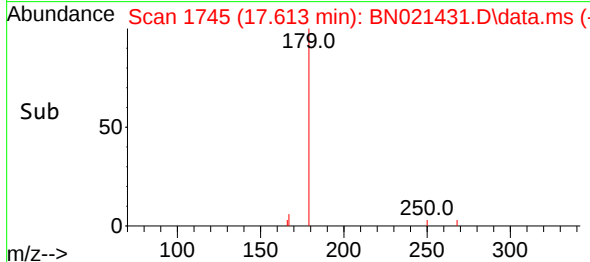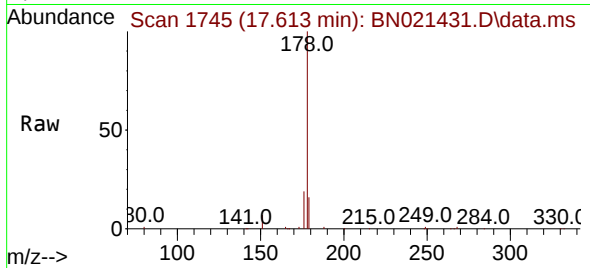

#27
 Fluoranthene-d10
 Concen: 0.347 ng
 RT: 19.506 min Scan# 2138
 Delta R.T. -0.004 min
 Lab File: BN021431.D
 Acq: 29 Aug 2022 20:43

Tgt Ion:212 Resp: 17216
 Ion Ratio Lower Upper
 212 100
 106 18.1 14.2 21.2
 104 10.1 7.8 11.6

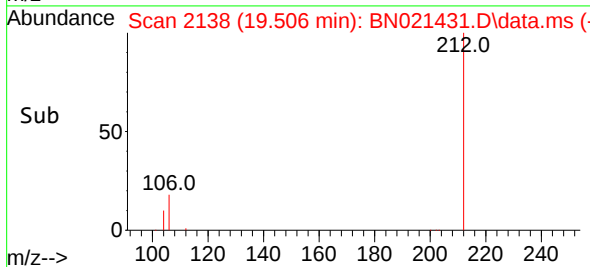

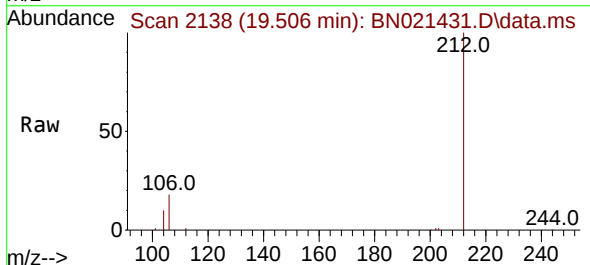




#28
Fluoranthene
Concen: 0.350 ng
RT: 19.535 min Scan# 2145
Delta R.T. -0.004 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:202 Resp: 24222
Ion Ratio Lower Upper
202 100
101 13.7 10.9 16.3
203 17.0 13.8 20.6

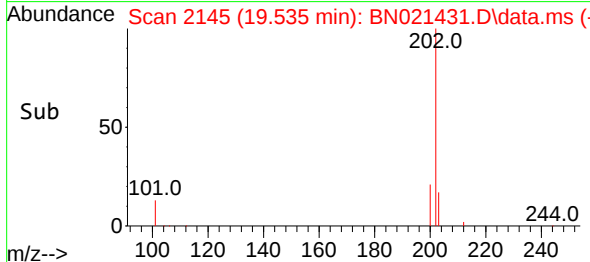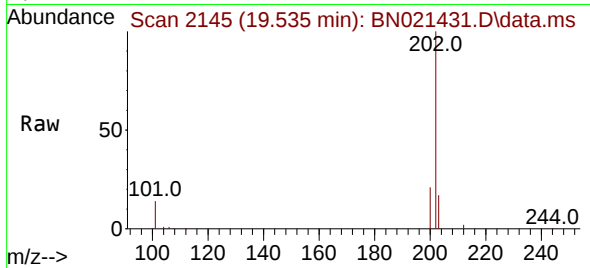

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.664 min Scan# 2442
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:240 Resp: 13986
Ion Ratio Lower Upper
240 100
120 16.2 10.2 15.4#
236 27.9 22.1 33.1


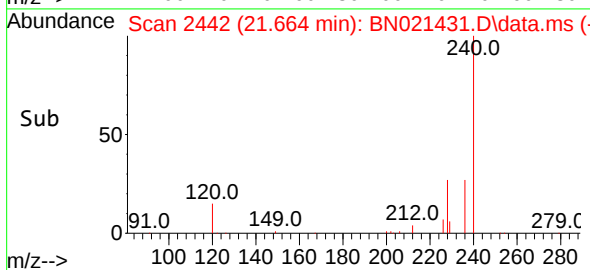

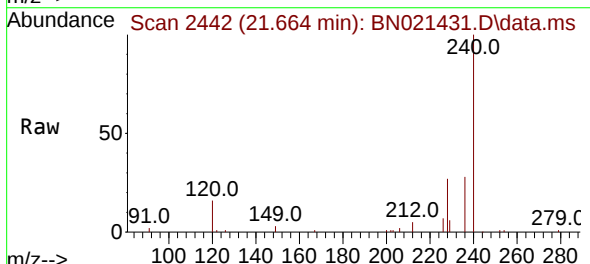


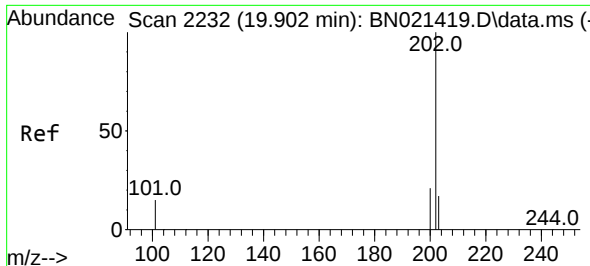

#30
Pyrene
Concen: 0.358 ng
RT: 19.898 min Scan# 21
Delta R.T. -0.004 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:202 Resp: 26676
Ion Ratio Lower Upper
202 100
200 20.6 13.9 20.9
203 15.7 11.9 17.9

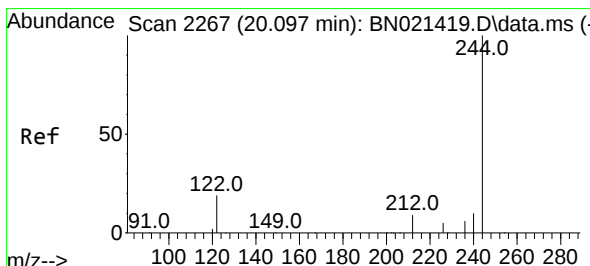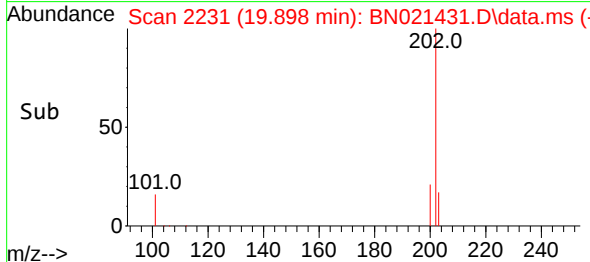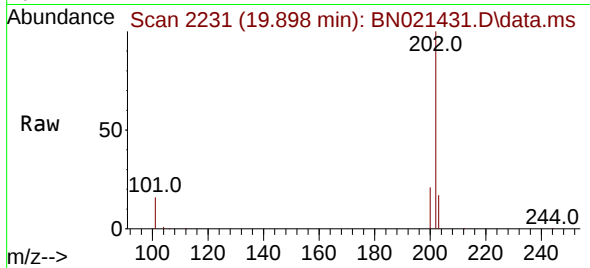

#31
Terphenyl-d14
Concen: 0.381 ng
RT: 20.097 min Scan# 2267
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:244 Resp: 11973
Ion Ratio Lower Upper
244 100
212 8.9 6.5 9.7
122 15.7 9.1 13.7#


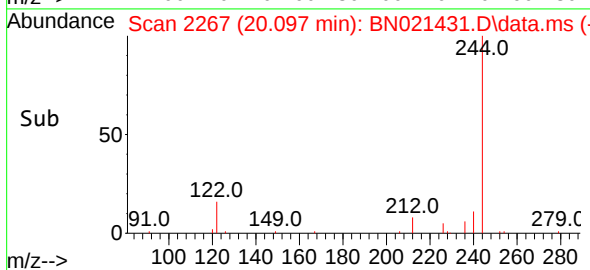

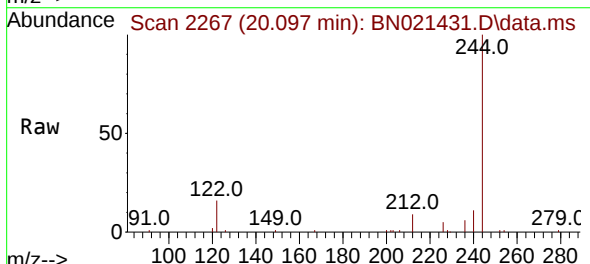




#32
Benzo(a)anthracene
Concen: 0.341 ng
RT: 21.646 min Scan# 2441
Delta R.T. -0.009 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:228 Resp: 16592
Ion Ratio Lower Upper
228 100
226 27.6 22.0 33.0
229 19.6 15.9 23.9

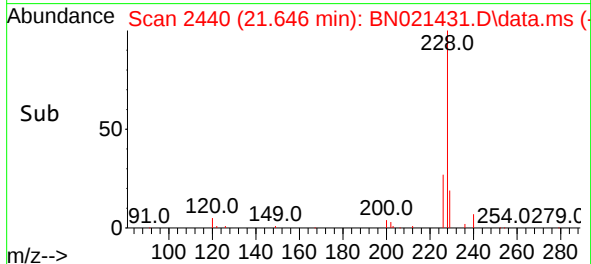

#33
Chrysene
Concen: 0.370 ng
RT: 21.700 min Scan# 2446
Delta R.T. -0.009 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:228 Resp: 21463
Ion Ratio Lower Upper
228 100
226 31.1 24.2 36.2
229 19.3 15.9 23.9

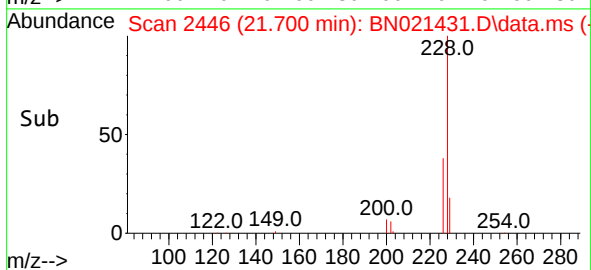

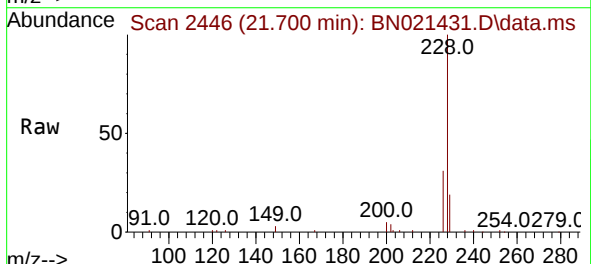




#34
Bis(2-ethylhexyl)phthalate
Concen: 0.349 ng
RT: 21.566 min Scan# 2431
Delta R.T. 0.000 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:149 Resp: 6846
Ion Ratio Lower Upper
149 100
167 25.6 21.4 32.0
279 2.4 2.2 3.2

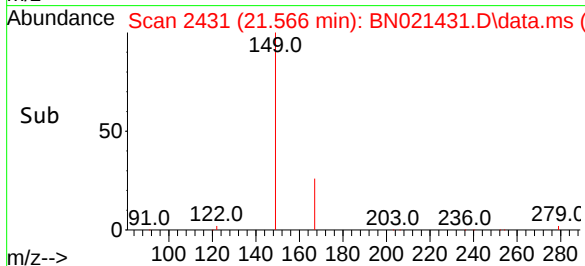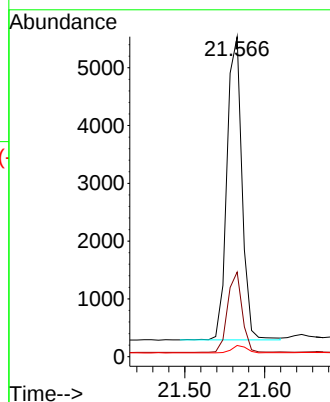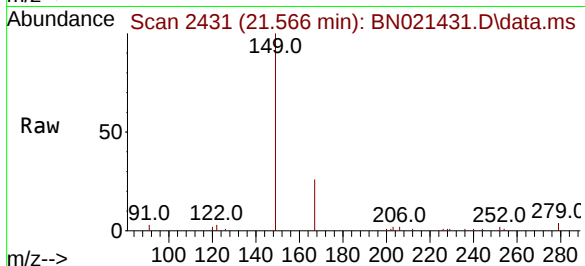

#35
Perylene-d12
Concen: 0.400 ng
RT: 24.185 min Scan# 3133
Delta R.T. -0.009 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:264 Resp: 9730
Ion Ratio Lower Upper
264 100
260 26.7 21.0 31.6
265 34.9 32.2 48.2

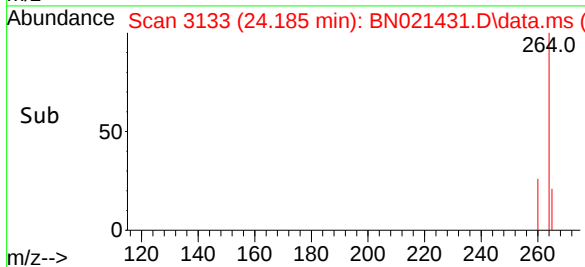
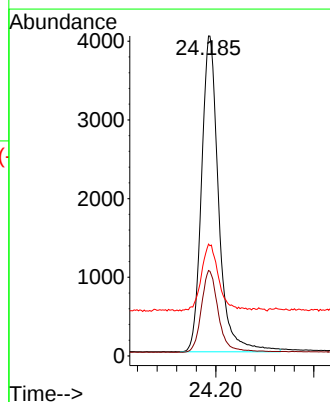
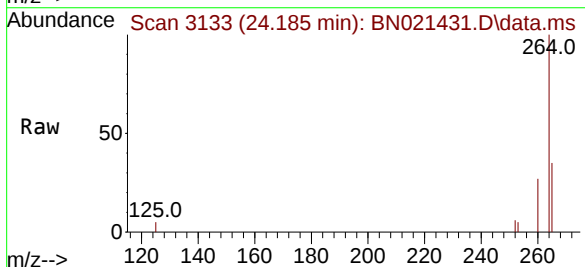




#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.357 ng
 RT: 26.843 min Scan# 4044
 Delta R.T. -0.006 min
 Lab File: BN021431.D
 Acq: 29 Aug 2022 20:43




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:276 Resp: 15692
 Ion Ratio Lower Upper
 276 100
 138 34.6 27.4 41.2
 277 24.7 19.9 29.9

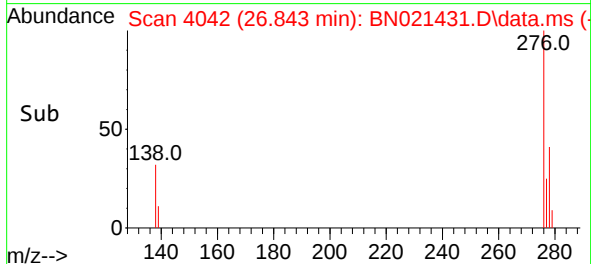

#37
 Benzo(b)fluoranthene
 Concen: 0.349 ng
 RT: 23.410 min Scan# 2868
 Delta R.T. -0.003 min
 Lab File: BN021431.D
 Acq: 29 Aug 2022 20:43

Tgt Ion:252 Resp: 16761
 Ion Ratio Lower Upper
 252 100
 253 23.4 19.8 29.6
 125 15.9 13.7 20.5

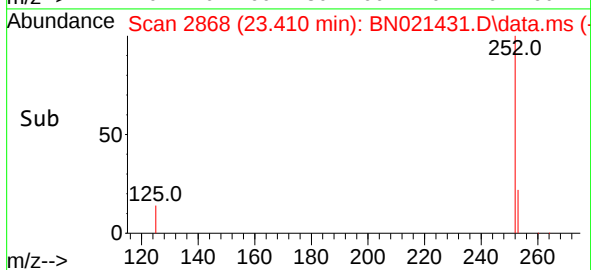

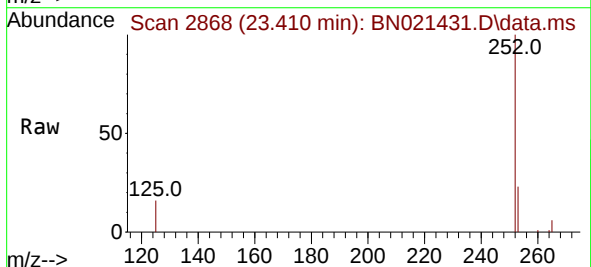




#38
Benzo(k)fluoranthene
Concen: 0.342 ng
RT: 23.460 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:252 Resp: 16508
Ion Ratio Lower Upper
252 100
253 23.1 19.5 29.3
125 15.1 12.3 18.5

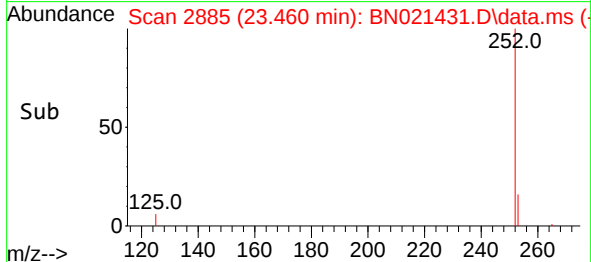

#39
Benzo(a)pyrene
Concen: 0.355 ng
RT: 24.074 min Scan# 3095
Delta R.T. -0.003 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:252 Resp: 11870
Ion Ratio Lower Upper
252 100
253 25.5 21.1 31.7
125 21.8 16.6 25.0


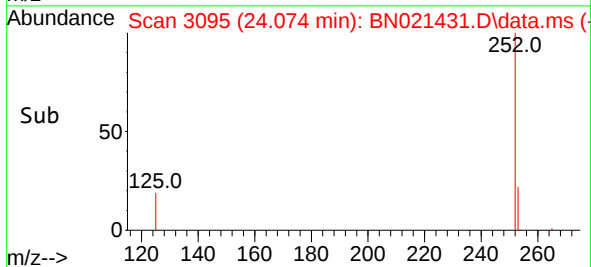

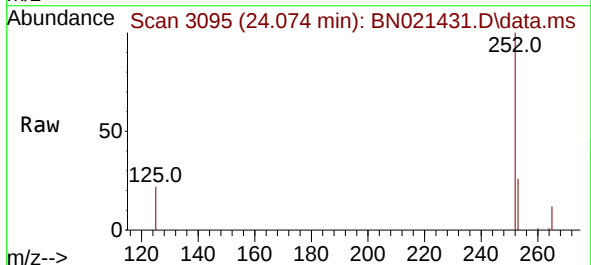




#40
Dibenzo(a,h)anthracene
Concen: 0.358 ng
RT: 26.869 min Scan# 4053
Delta R.T. -0.006 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:278 Resp: 12648
Ion Ratio Lower Upper
278 100
139 24.0 21.8 32.6
279 24.9 20.4 30.6

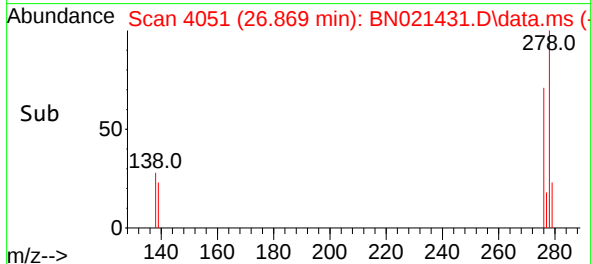

#41
Benzo(g,h,i)perylene
Concen: 0.338 ng
RT: 27.661 min Scan# 4322
Delta R.T. -0.009 min
Lab File: BN021431.D
Acq: 29 Aug 2022 20:43

Tgt Ion:276 Resp: 13096
Ion Ratio Lower Upper
276 100
277 24.8 19.7 29.5
138 30.5 23.7 35.5

