
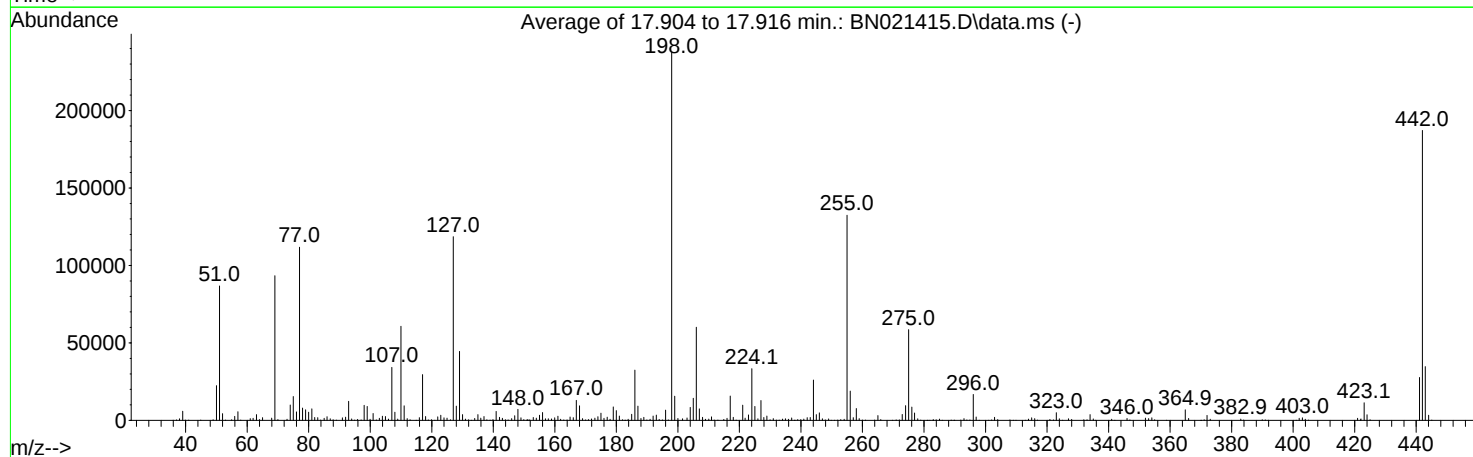


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
 Data File : BN021415.D
 Acq On : 29 Aug 2022 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 29 16:30:43 2022

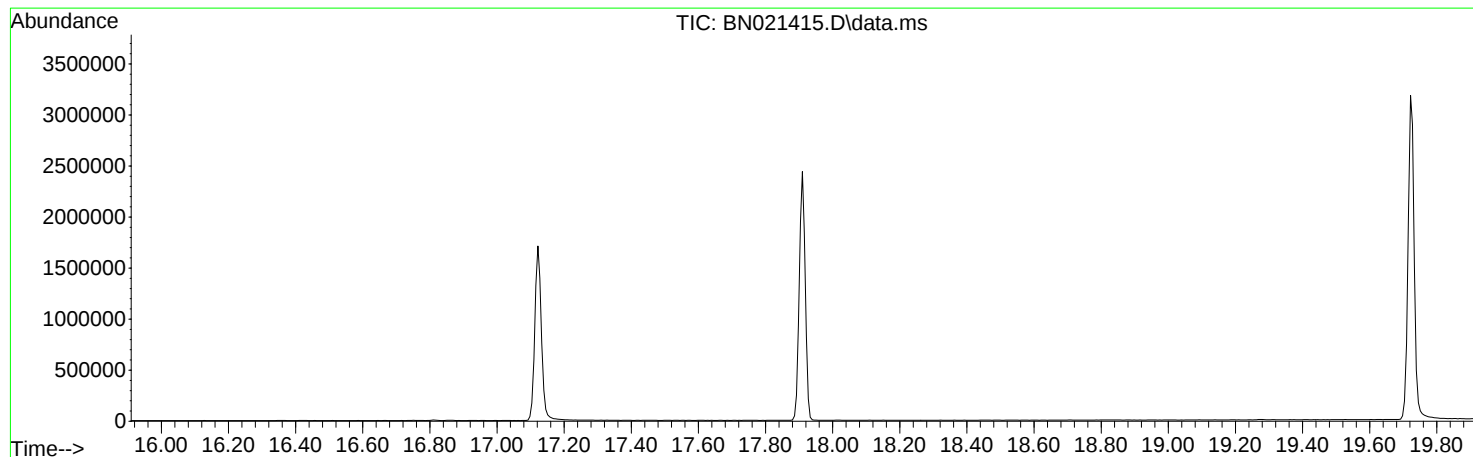

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	86733	PASS
68	69	0.00	2	1.6	1487	PASS
69	198	0.00	100	39.3	93339	PASS
70	69	0.00	2	0.6	527	PASS
127	198	10	80	49.9	118563	PASS
197	198	0.00	2	0.2	362	PASS
198	198	100	100	100.0	237461	PASS
199	198	5	9	6.6	15603	PASS
275	198	10	60	24.7	58563	PASS
365	198	1	100	2.9	6809	PASS
441	198	0.01	100	11.6	27656	PASS
442	442	50	100	100.0	187136	PASS
443	442	15	24	18.5	34691	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/29/2022	BNA_N	<u>BN021415.D</u>
Compound Name	Response	Retention Time
DDT	791919	20.95
DDD	7863	20.51
DDE	978	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8841	800760	1.10

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
 Data File : BN021415.D
 Acq On : 29 Aug 2022 09:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 29 14:49:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 20 17:56:56 2021
 Response via : Initial Calibration

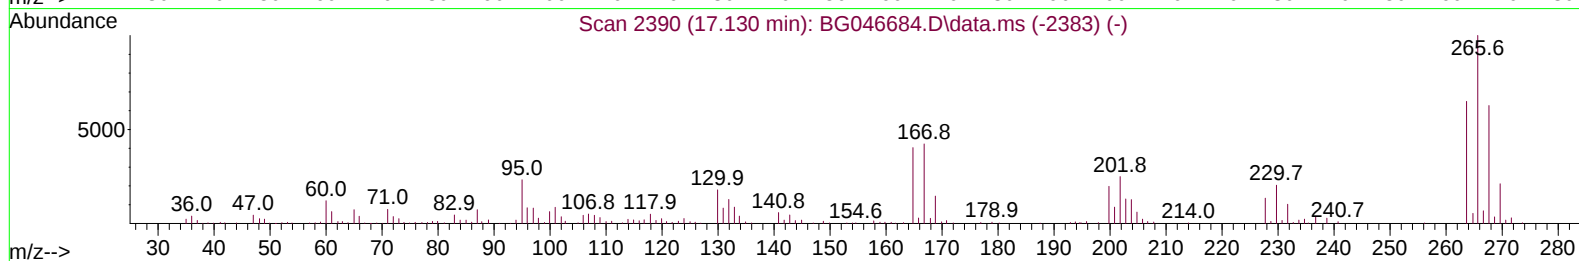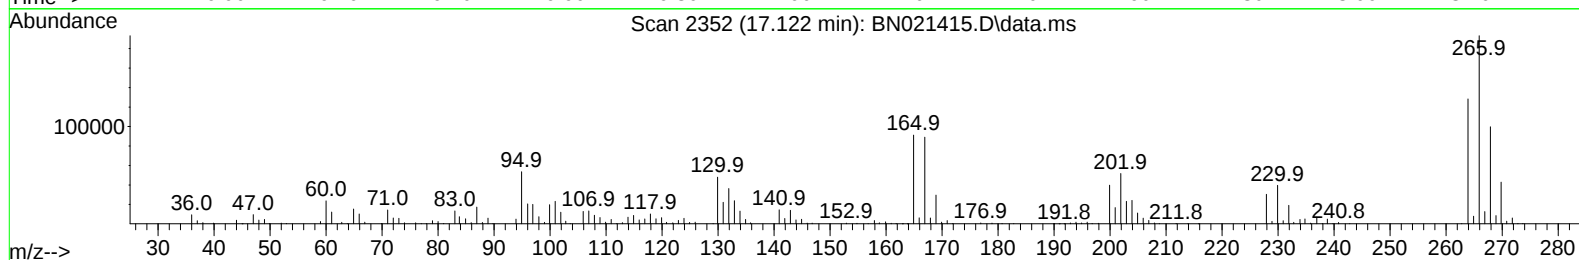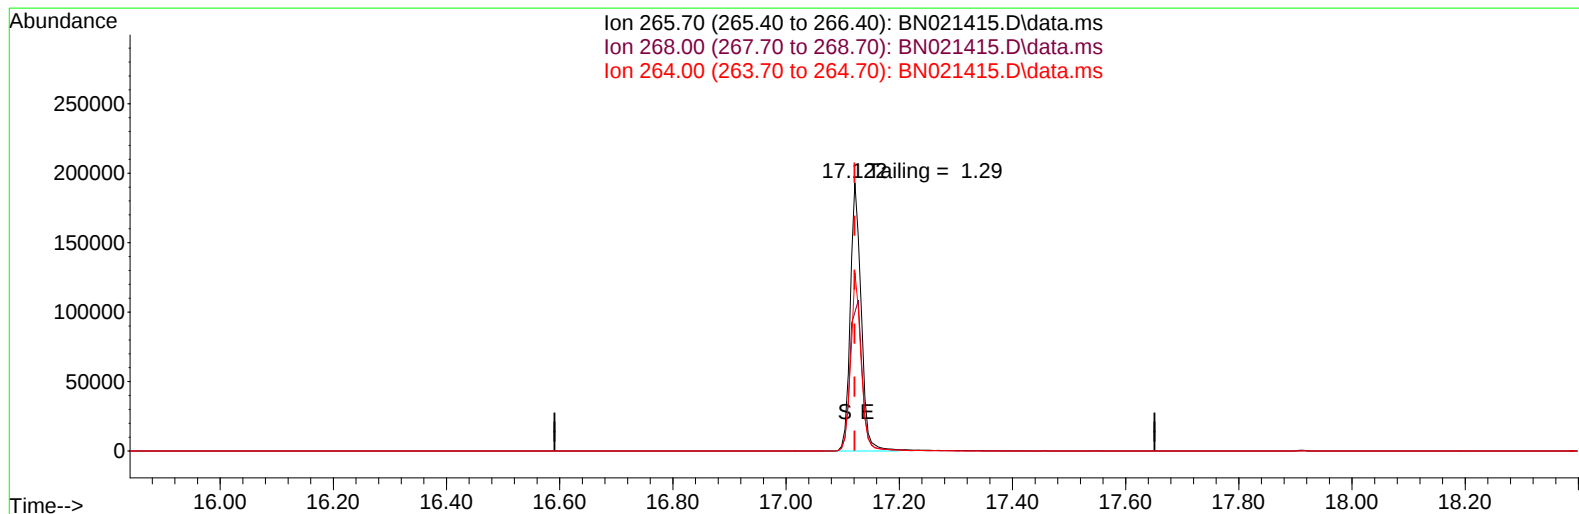

TIC: BN021415.D\data.ms

(70) Pentachlorophenol (C)

17.122min (+ 0.001) 19651.27 ng




response 262171

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	51.63
264.00	61.60	66.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
Data File : BN021415.D
Acq On : 29 Aug 2022 09:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 29 14:49:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

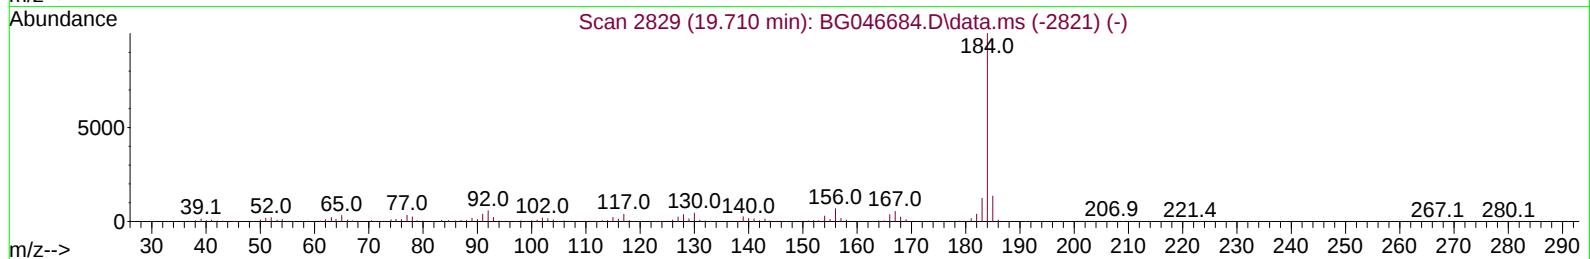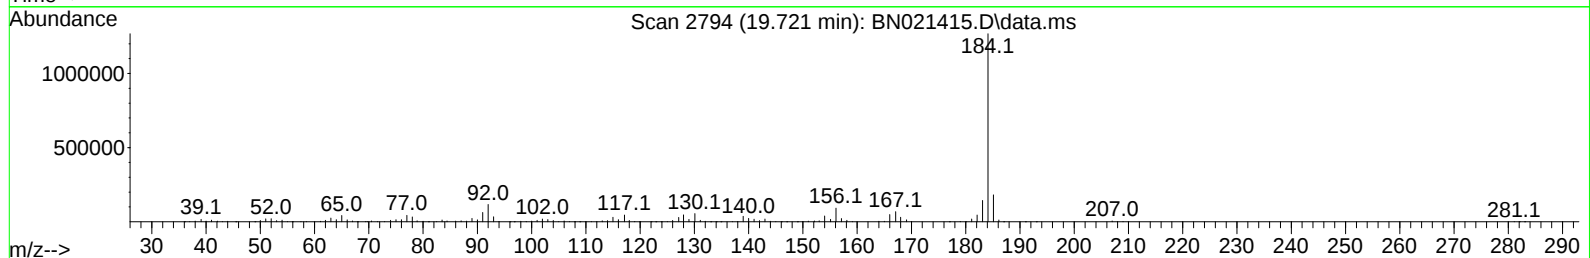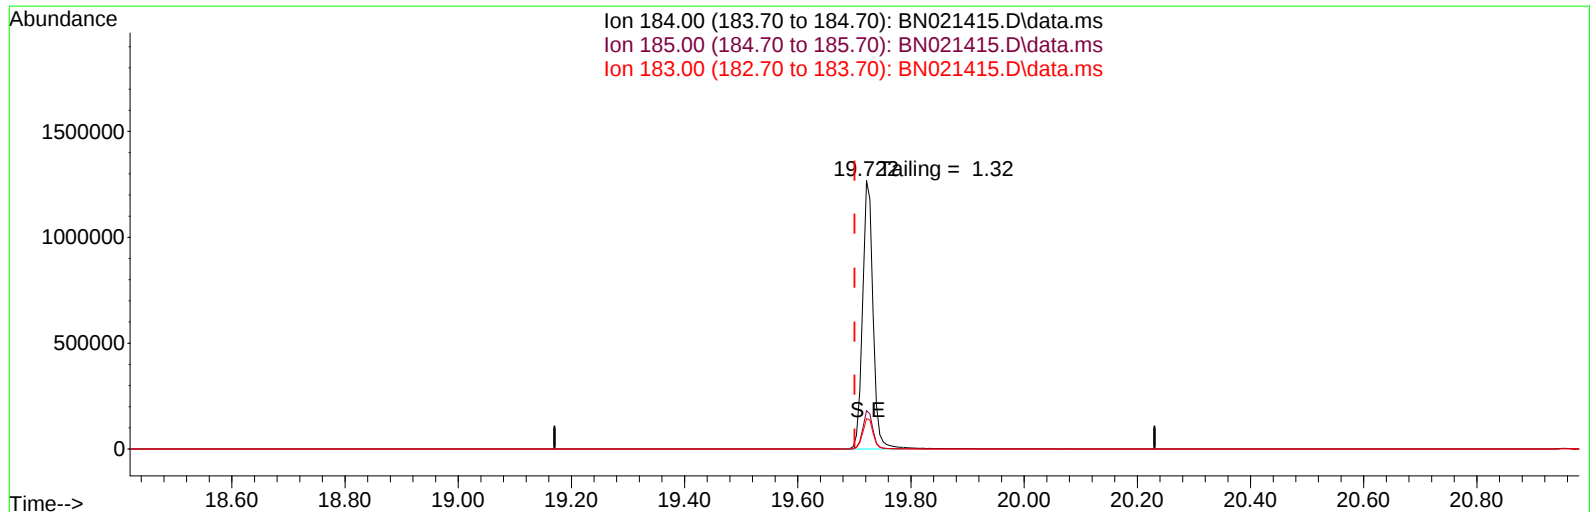

TIC: BN021415.D\data.ms

(77) Benzidine

19.721min (+ 0.021) 0.00 ng

response 1642830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.33
183.00	13.20	11.35
0.00	0.00	0.00