
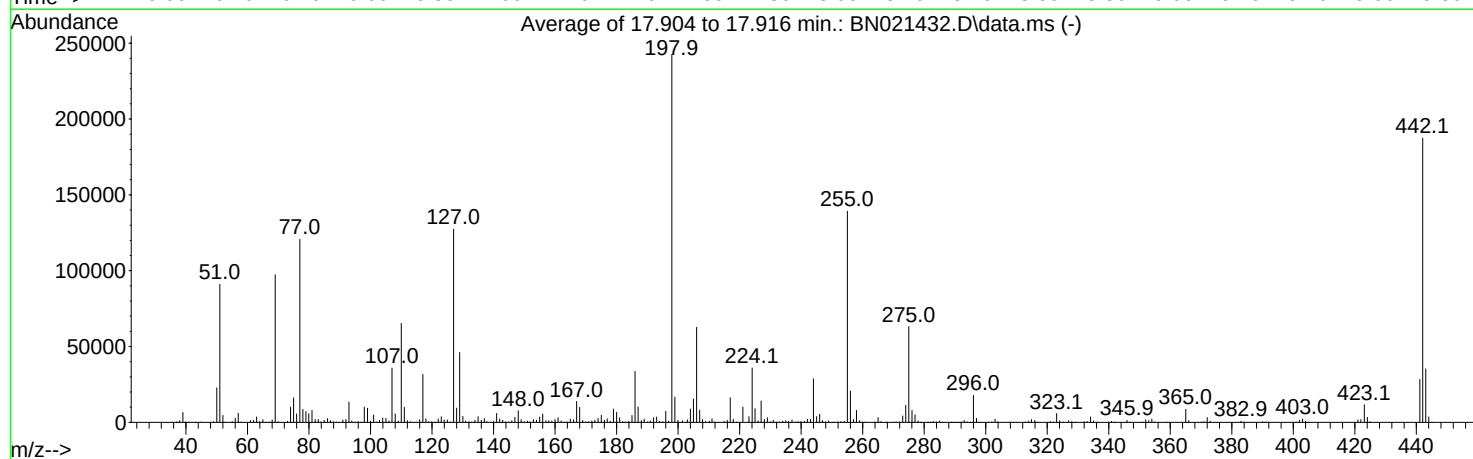


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
 Data File : BN021432.D
 Acq On : 29 Aug 2022 22:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 29 16:30:43 2022

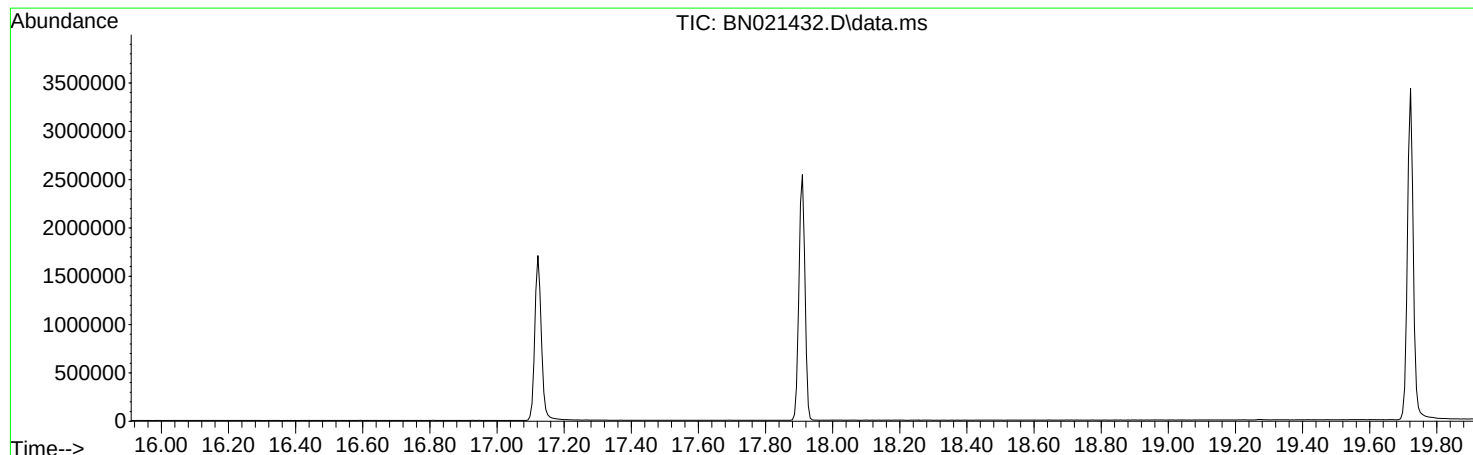

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	91080	PASS
68	69	0.00	2	1.7	1612	PASS
69	198	0.00	100	40.1	97352	PASS
70	69	0.00	2	0.5	474	PASS
127	198	10	80	52.5	127291	PASS
197	198	0.00	2	0.3	831	PASS
198	198	100	100	100.0	242539	PASS
199	198	5	9	6.9	16721	PASS
275	198	10	60	26.0	63144	PASS
365	198	1	100	3.5	8573	PASS
441	198	0.01	100	11.7	28360	PASS
442	442	50	100	100.0	187371	PASS
443	442	15	24	18.8	35216	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/29/2022	BNA_N	<u>BN021432.D</u>
Compound Name	Response	Retention Time
DDT	796416	20.951
DDD	7986	20.51
DDE	457	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8443	804859	1.05

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
 Data File : BN021432.D
 Acq On : 29 Aug 2022 22:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 30 05:08:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 30 05:08:28 2022
 Response via : Initial Calibration

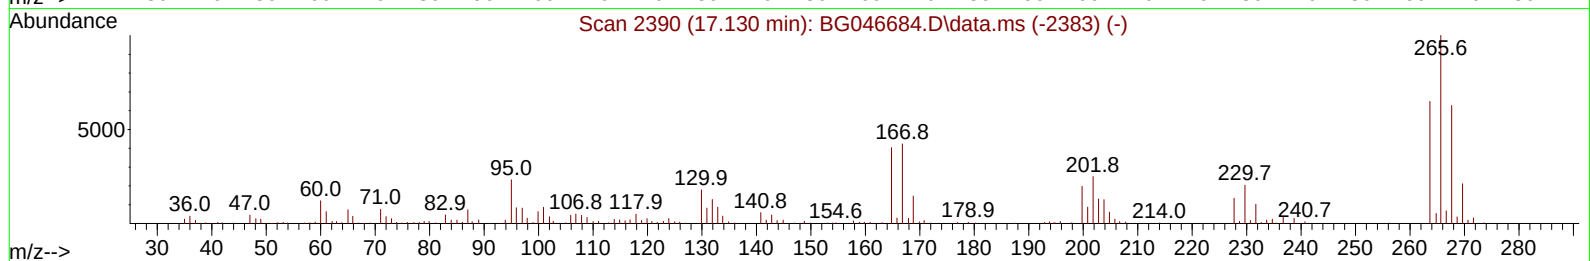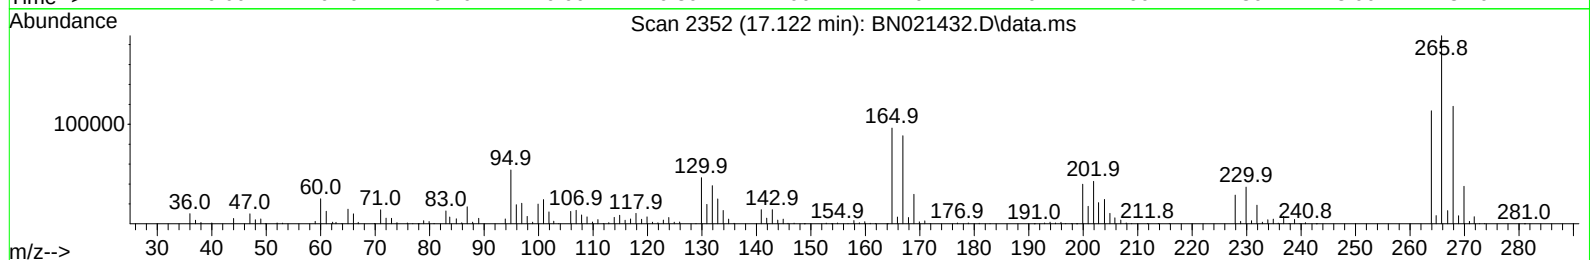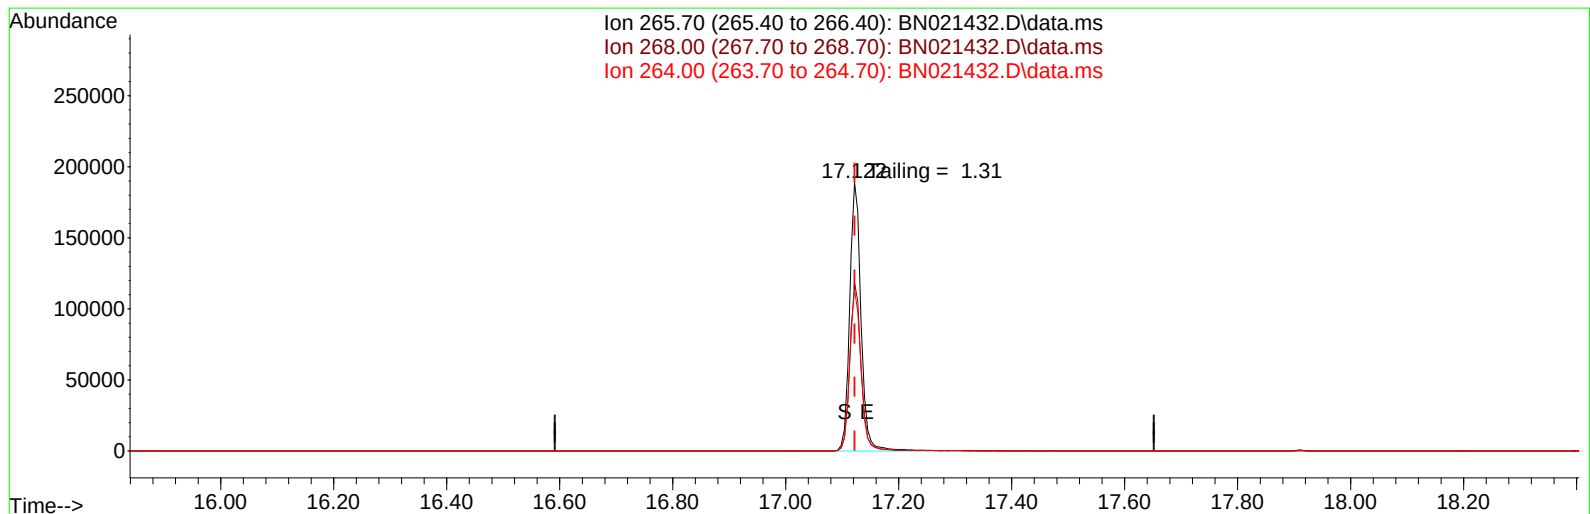

TIC: BN021432.D\data.ms

(70) Pentachlorophenol (C)

17.122min (0.000) 19618.43 ng




response 265120

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.51
264.00	61.60	60.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082922\
 Data File : BN021432.D
 Acq On : 29 Aug 2022 22:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 30 05:08:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 30 05:08:28 2022
 Response via : Initial Calibration

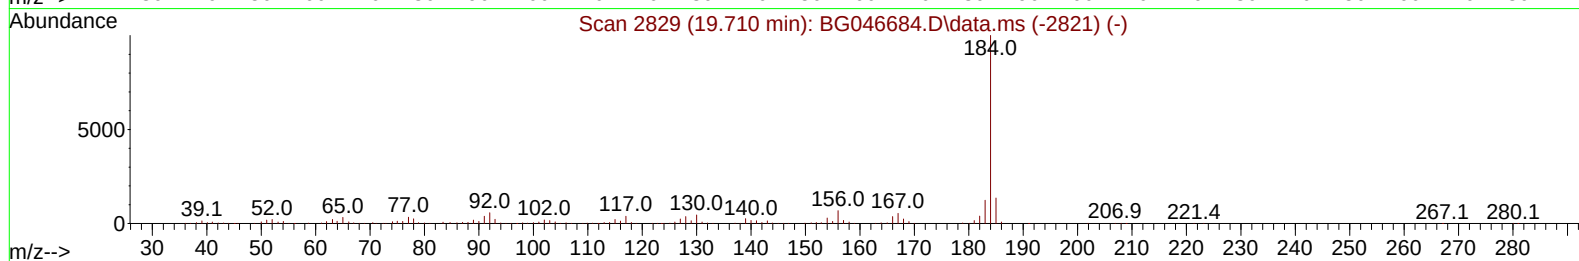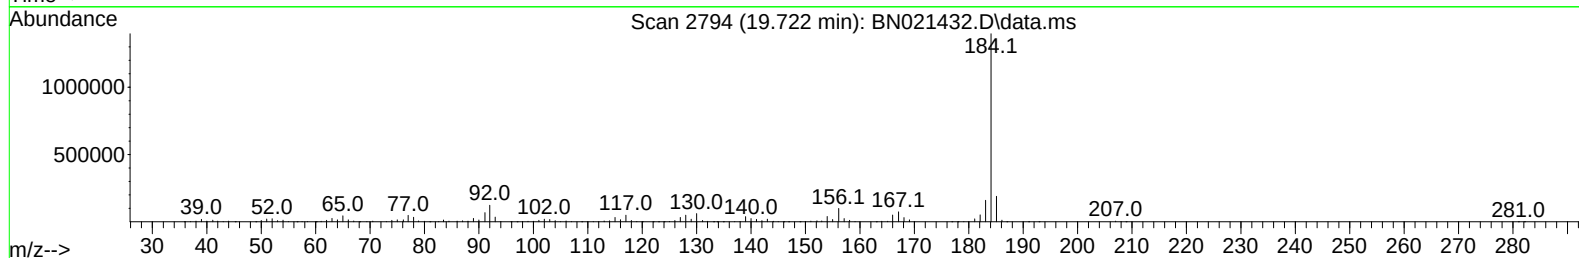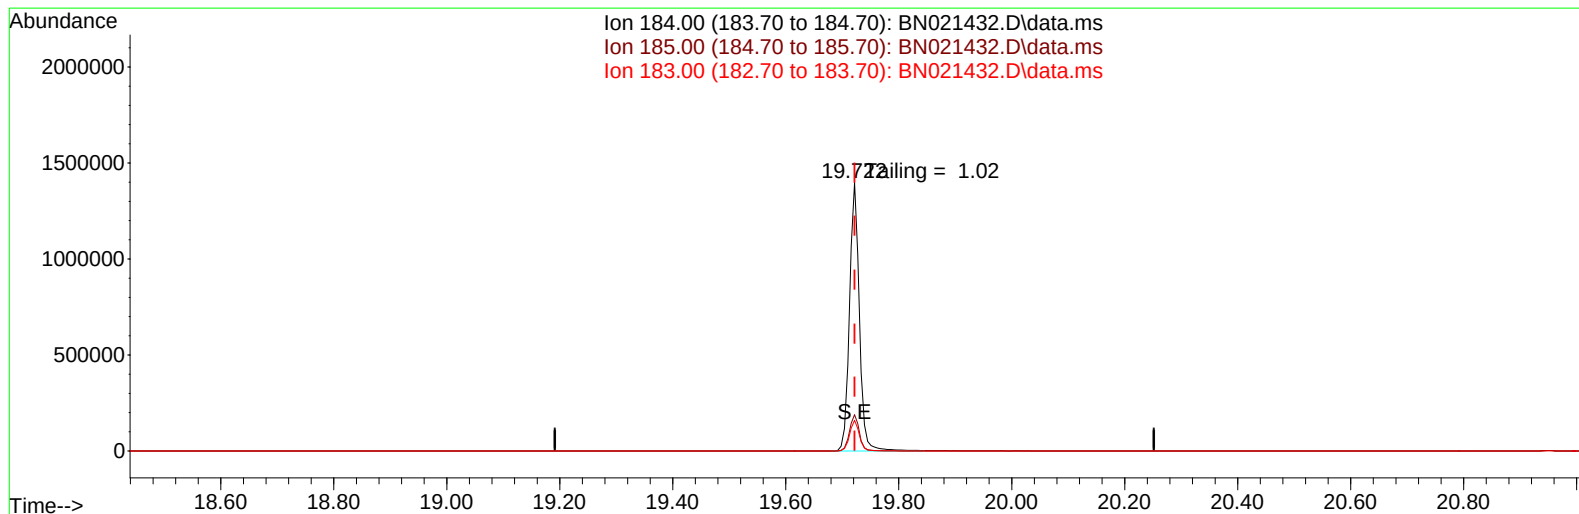

TIC: BN021432.D\data.ms

(77) Benzidine

19.722min (0.000) 0.00 ng

response 1708697

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.53
183.00	13.20	11.44
0.00	0.00	0.00