
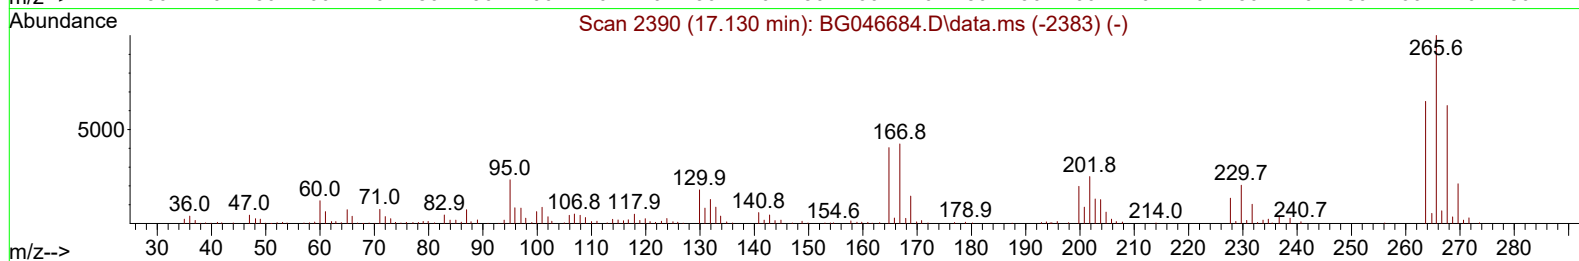
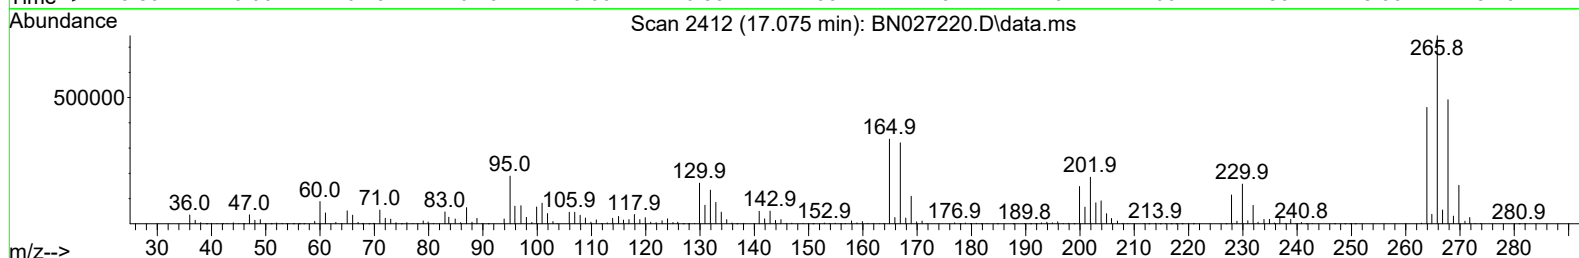


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
Data File : BN027220.D
Acq On : 28 Aug 2023 17:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 06:03:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 06:02:58 2023
Response via : Initial Calibration

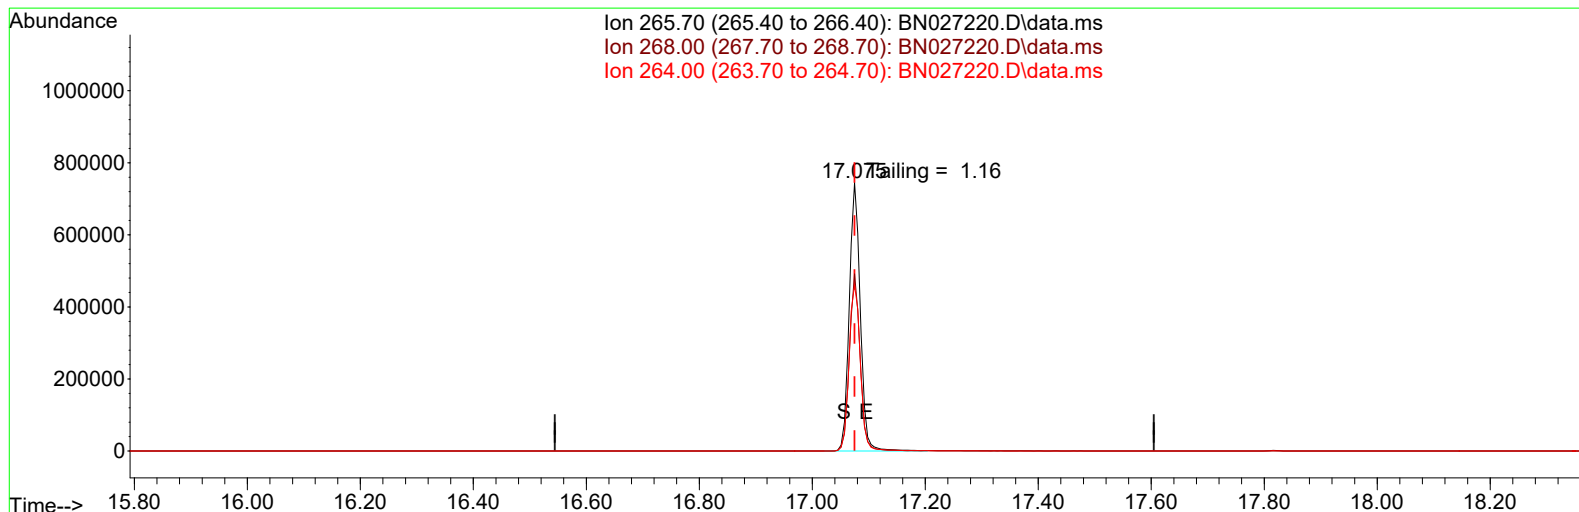

TIC: BN027220.D\data.ms

(70) Pentachlorophenol (C)




17.075min (0.000) 27232.29 ng

response 1015774

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.99
264.00	61.60	61.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
 Data File : BN027220.D
 Acq On : 28 Aug 2023 17:51
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 06:03:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 29 06:02:58 2023
 Response via : Initial Calibration

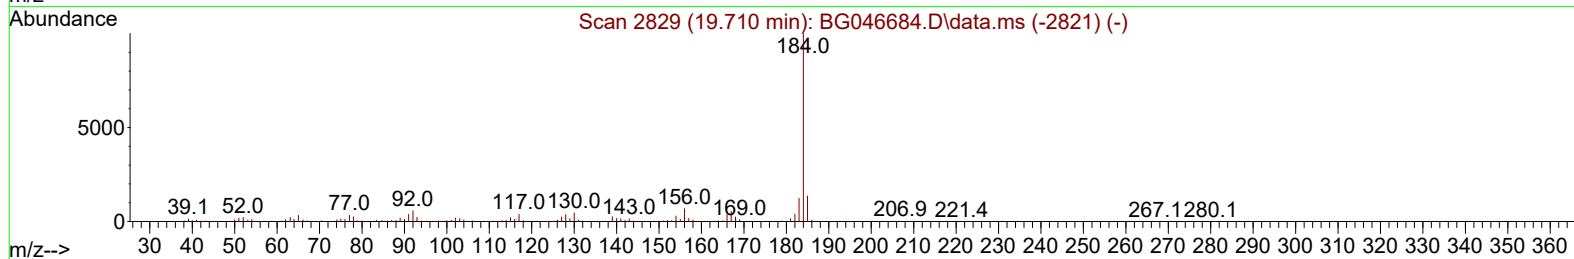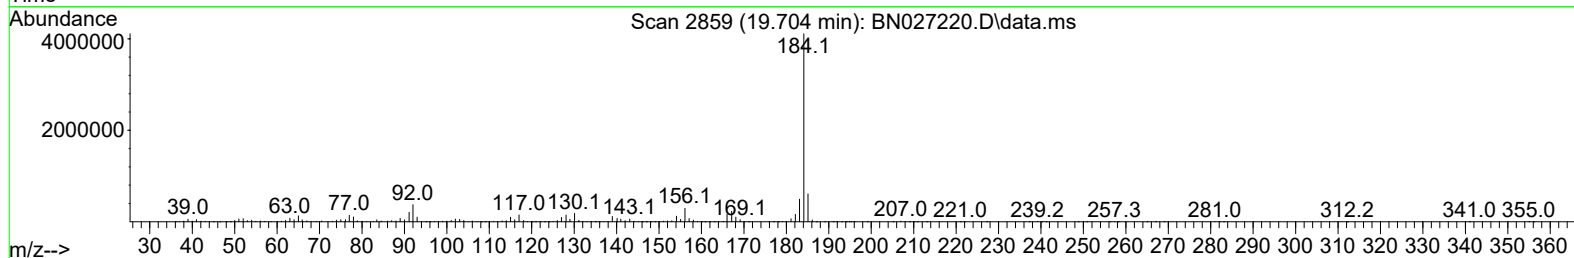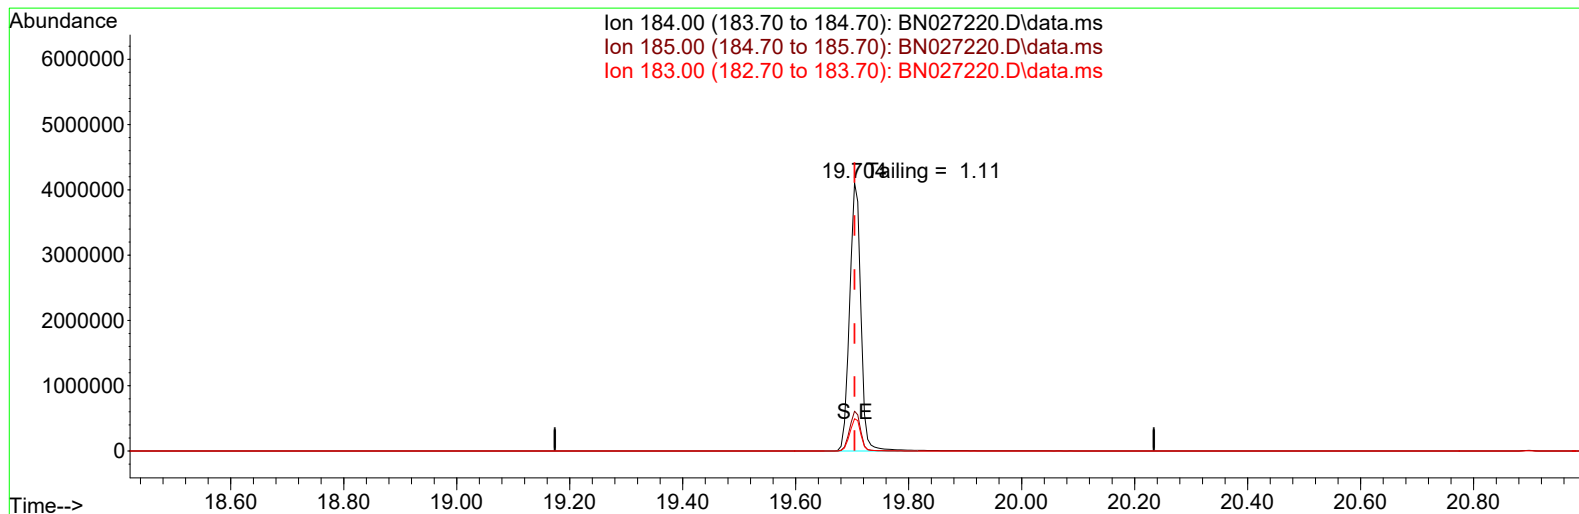

TIC: BN027220.D\data.ms

(77) Benzidine**19.704min (0.000) 235987.13 ng****response 5674025**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.84
183.00	13.20	12.05
0.00	0.00	0.00