
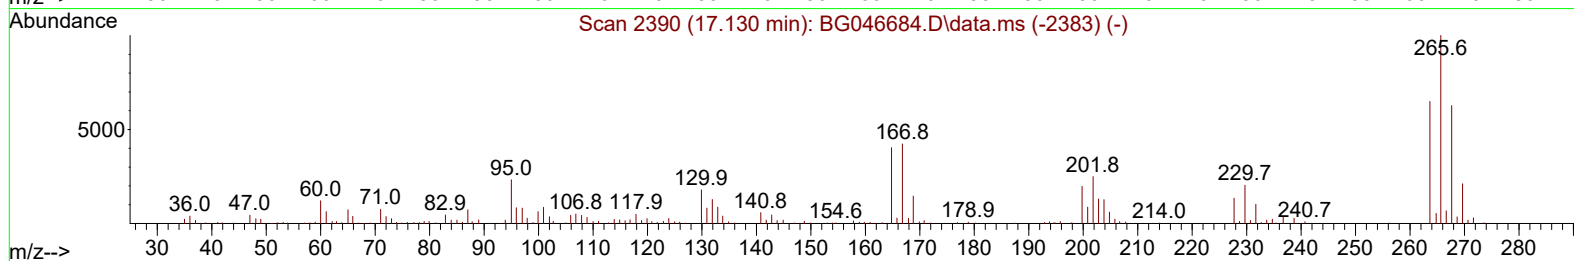
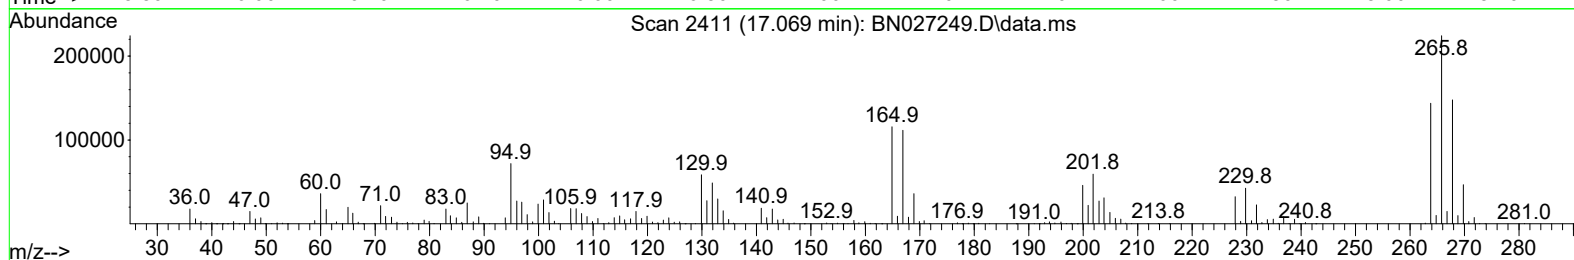


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
Data File : BN027249.D
Acq On : 29 Aug 2023 21:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 30 02:33:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 02:32:19 2023
Response via : Initial Calibration

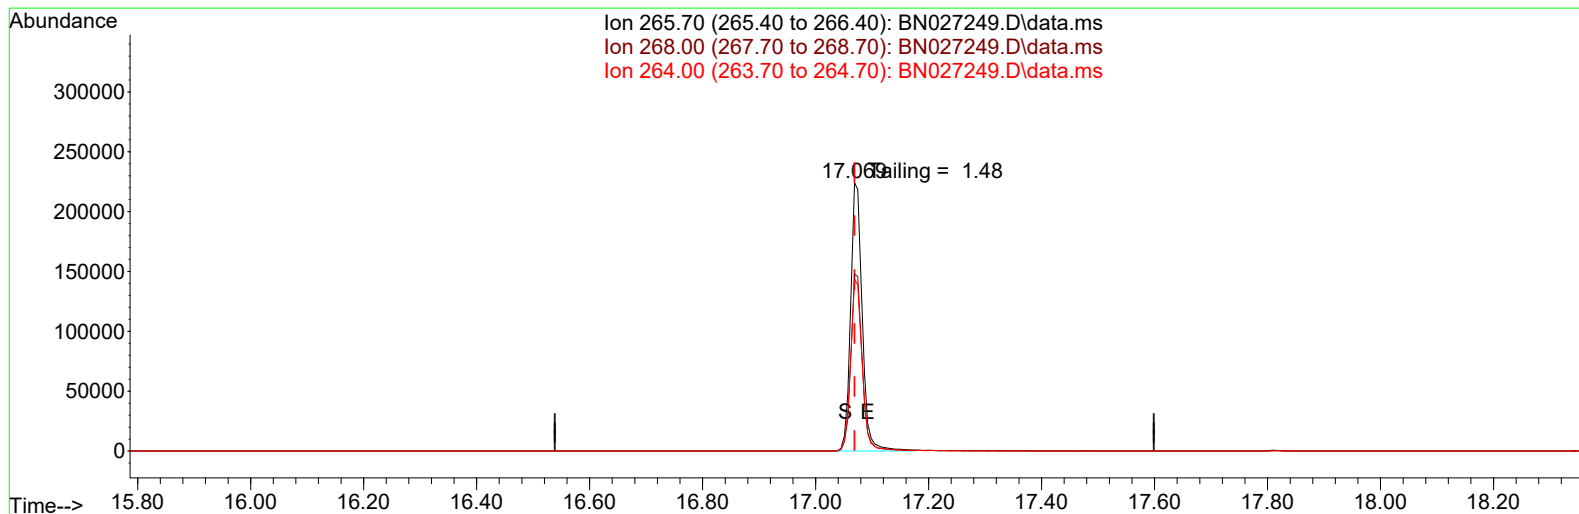

TIC: BN027249.D\data.ms

(70) Pentachlorophenol (C)




17.069min (-0.000) 20390.21 ng

response 325155

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.90
264.00	61.60	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
Data File : BN027249.D
Acq On : 29 Aug 2023 21:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 30 02:33:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 02:32:19 2023
Response via : Initial Calibration

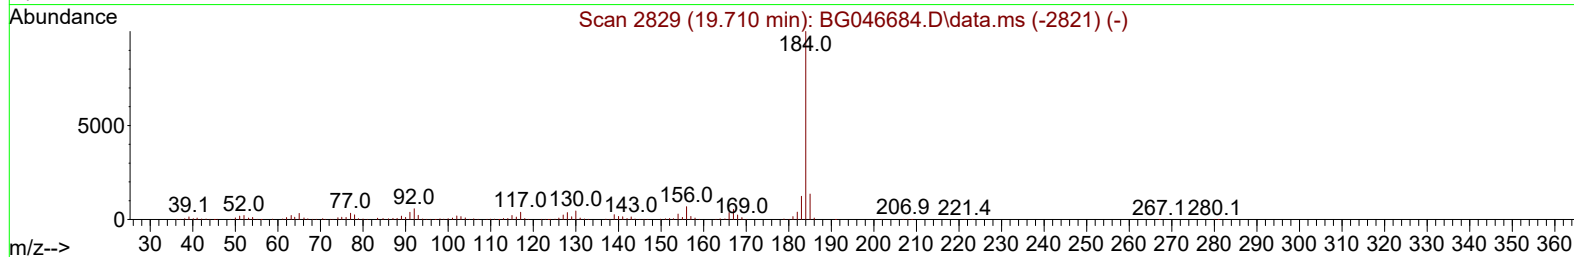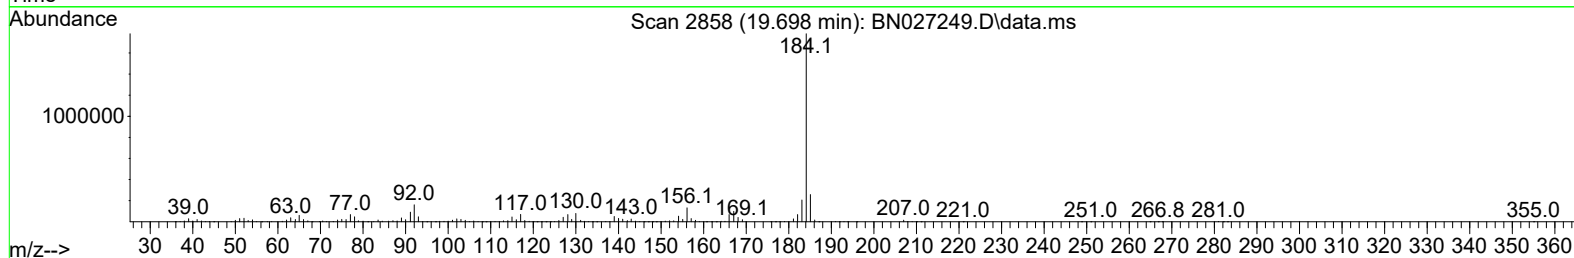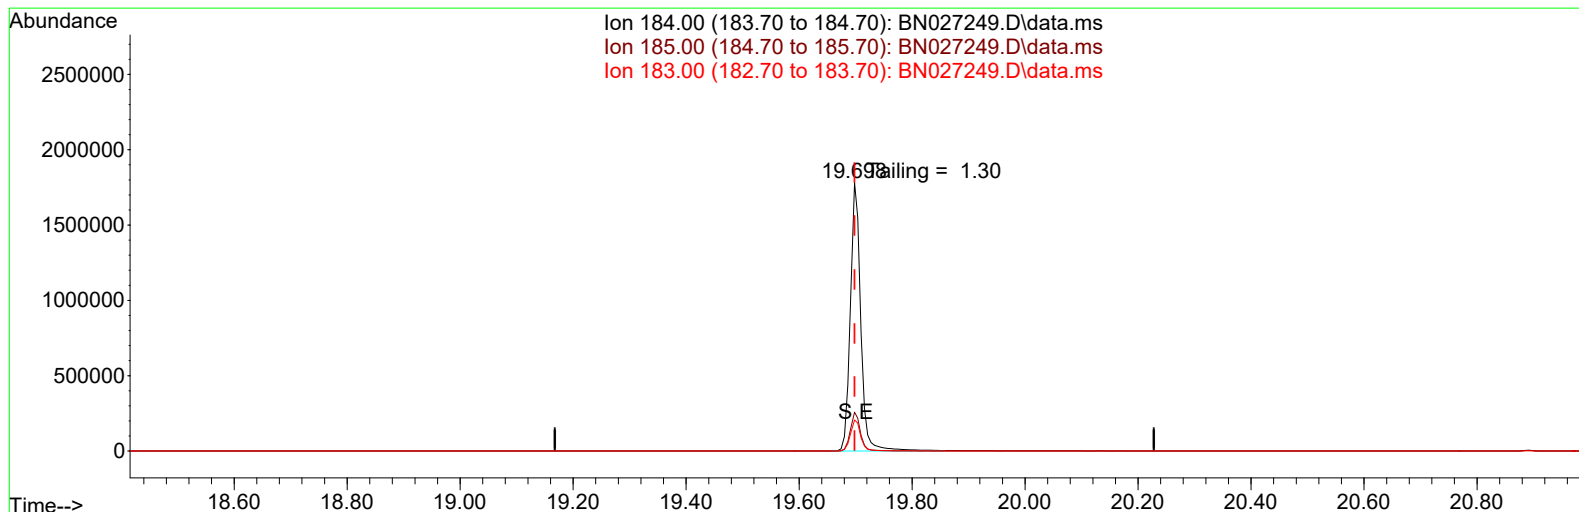

TIC: BN027249.D\data.ms

(77) Benzidine

19.698min (-0.000) 0.00 ng

response 2304744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.50
183.00	13.20	11.56
0.00	0.00	0.00