
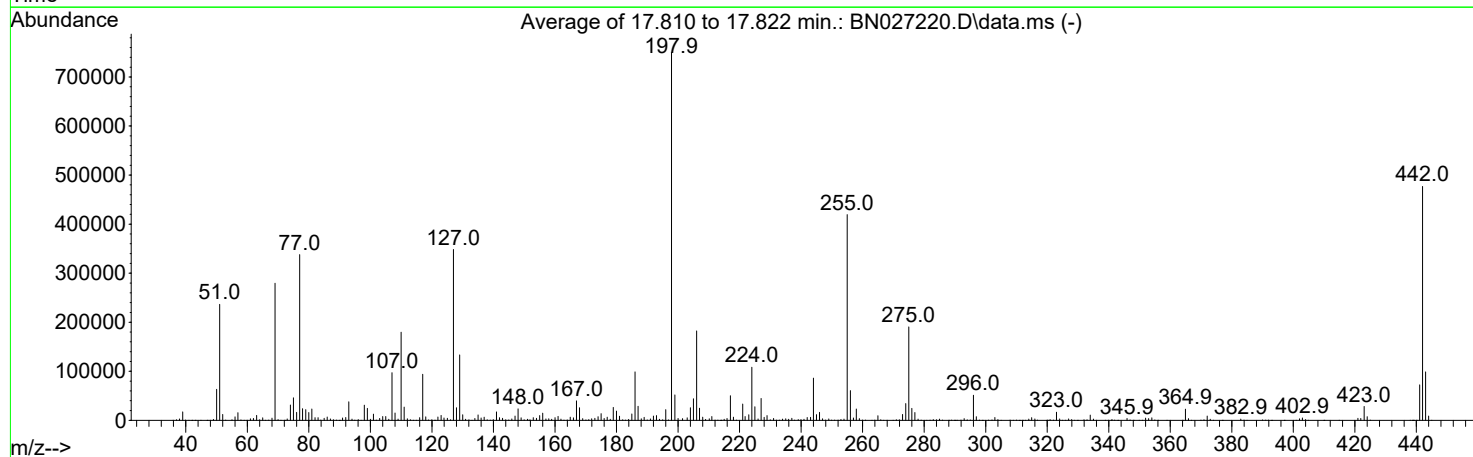


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
 Data File : BN027220.D
 Acq On : 28 Aug 2023 17:51
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 29 05:37:30 2023

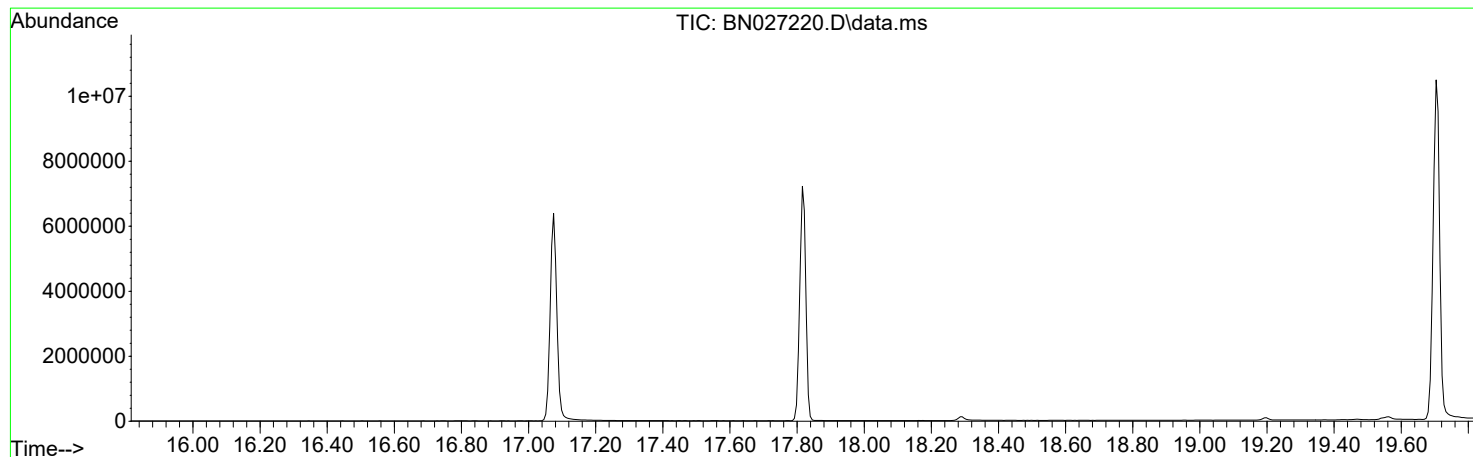




AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	236633	PASS
68	69	0.00	2	1.7	4711	PASS
69	198	0.00	100	37.3	279688	PASS
70	69	0.00	2	0.5	1522	PASS
127	198	10	80	46.4	348224	PASS
197	198	0.00	2	0.1	891	PASS
198	198	100	100	100.0	749867	PASS
199	198	5	9	6.9	52040	PASS
275	198	10	60	25.4	190443	PASS
365	198	1	100	3.0	22811	PASS
441	198	0.01	100	9.7	72533	PASS
442	442	50	100	100.0	476928	PASS
443	442	15	24	20.7	98893	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
Data File : BN027220.D
Acq On : 28 Aug 2023 17:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 29 06:03:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 06:02:58 2023
Response via : Initial Calibration

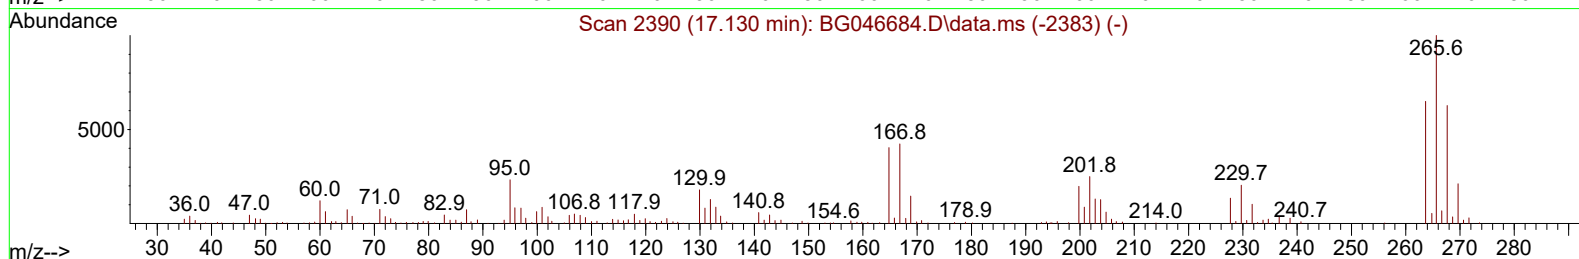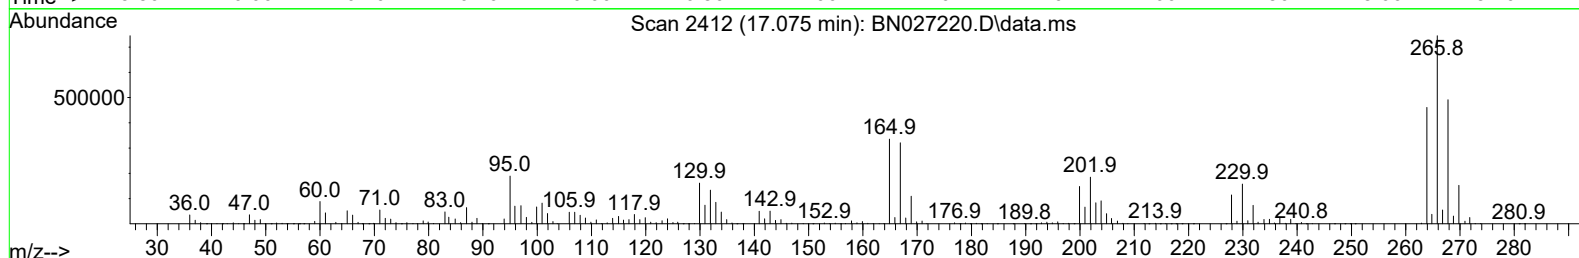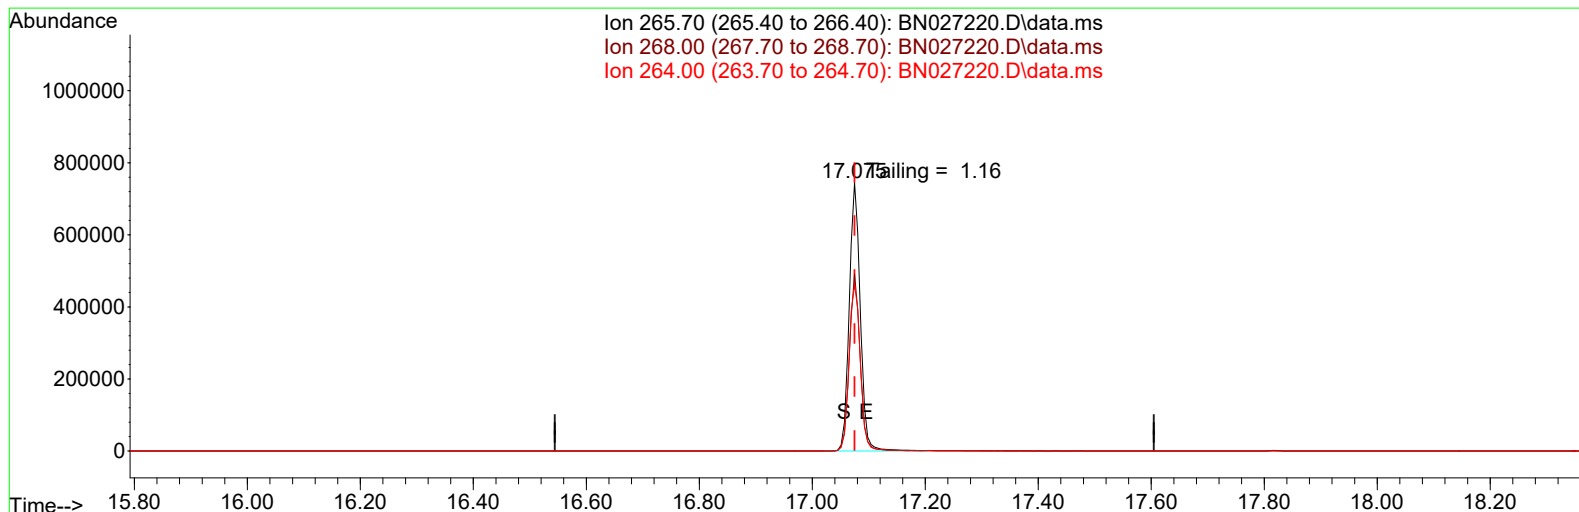

TIC: BN027220.D\data.ms

(70) Pentachlorophenol (C)

17.075min (0.000) 27232.29 ng




response 1015774

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.99
264.00	61.60	61.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
Data File : BN027220.D
Acq On : 28 Aug 2023 17:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 29 06:03:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 29 06:02:58 2023
Response via : Initial Calibration

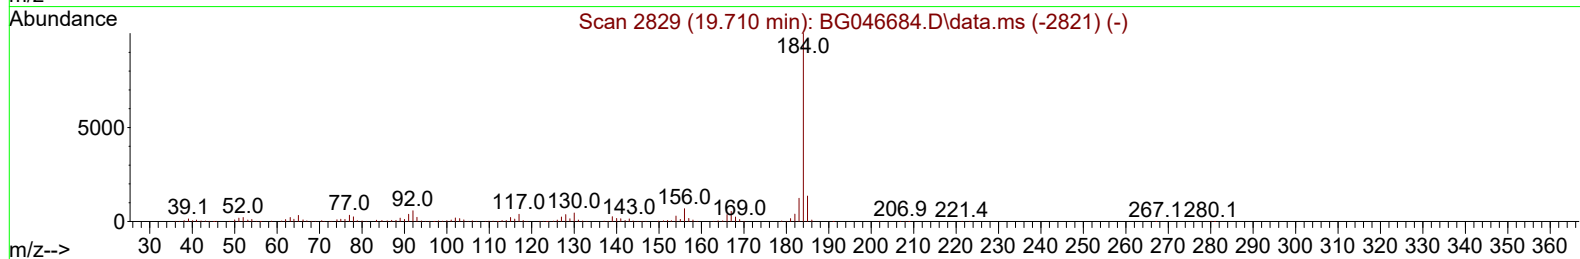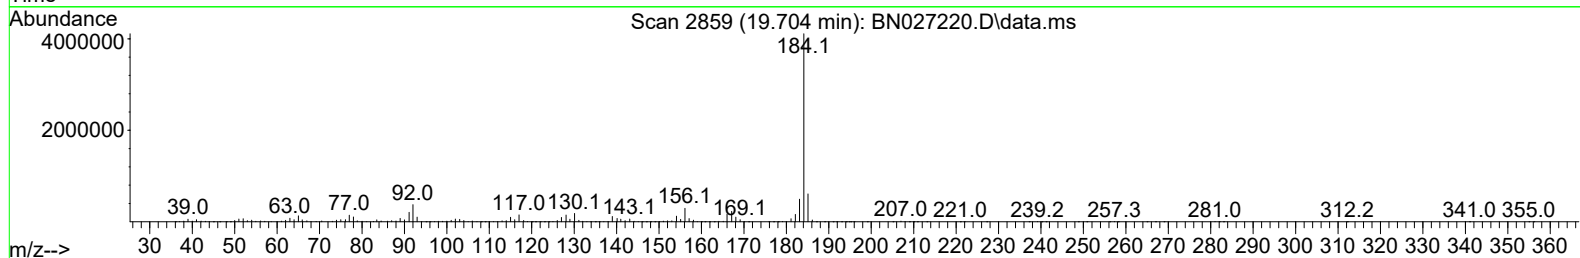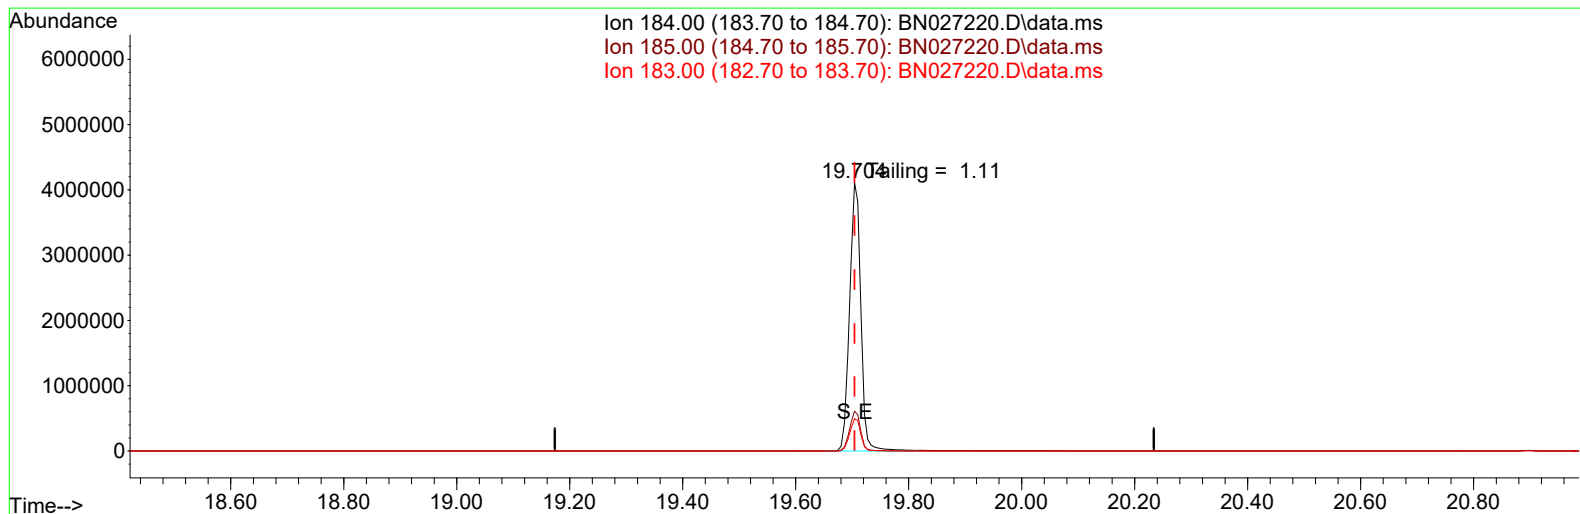

TIC: BN027220.D\data.ms

(77) Benzidine

19.704min (0.000) 235987.13 ng

response 5674025

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.84
183.00	13.20	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/29/2023	BNA_N	<u>BN027220.D</u>
Compound Name	Response	Retention Time
DDT	2457124	20.898
DDD	31758	20.457
DDE	1113	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32871	2489995	1.32

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP