


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
Data File : BN027249.D
Acq On : 29 Aug 2023 21:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 29 05:37:30 2023

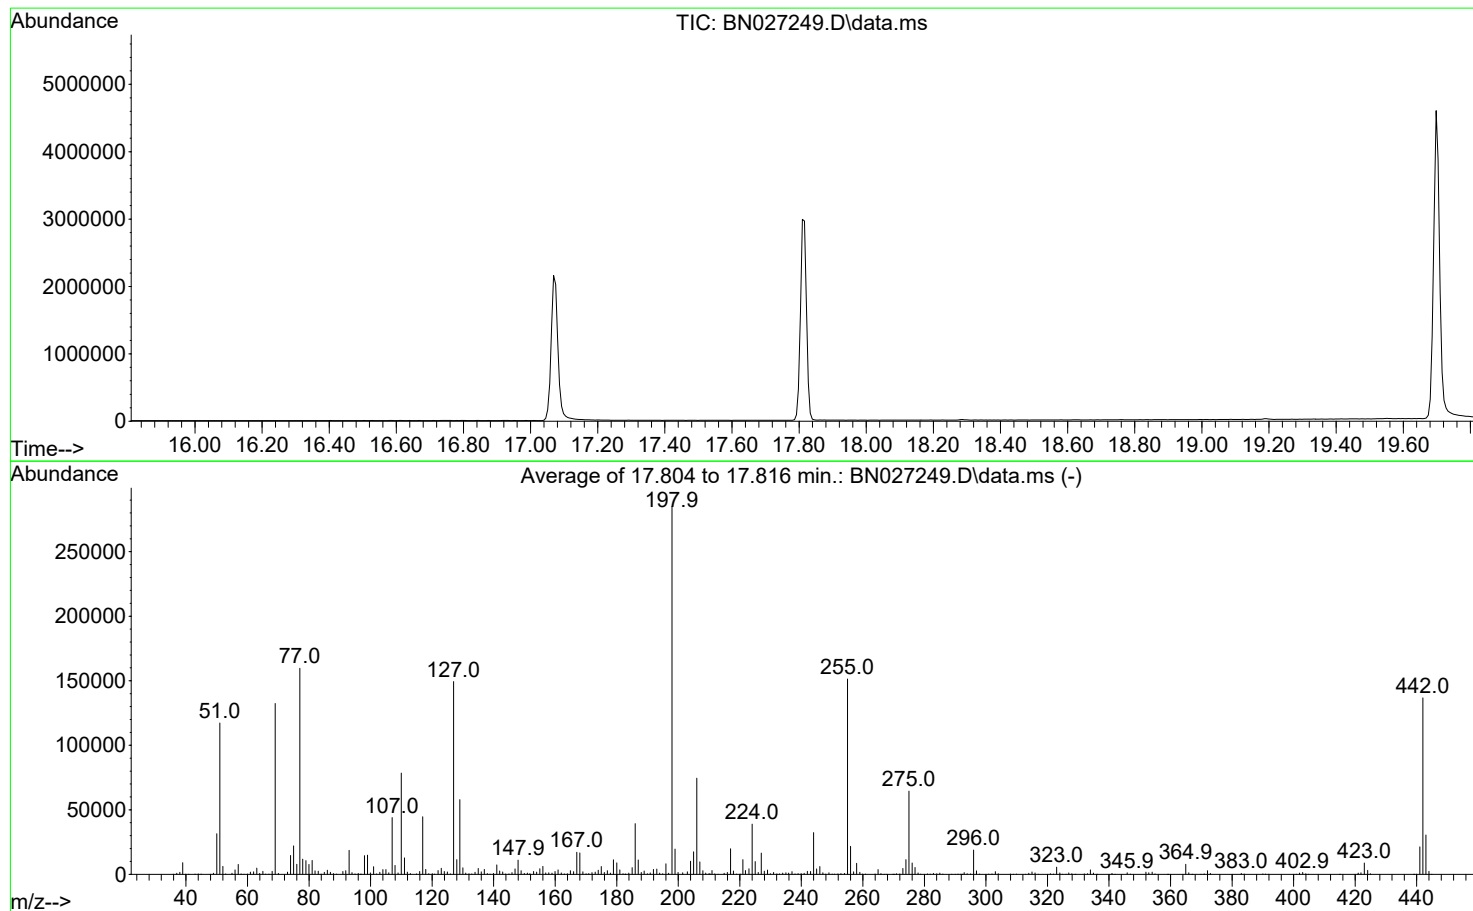




AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	117234	PASS
68	69	0.00	2	1.8	2362	PASS
69	198	0.00	100	46.5	132467	PASS
70	69	0.00	2	0.5	694	PASS
127	198	10	80	52.4	149381	PASS
197	198	0.00	2	0.3	936	PASS
198	198	100	100	100.0	285013	PASS
199	198	5	9	6.9	19545	PASS
275	198	10	60	22.6	64424	PASS
365	198	1	100	2.7	7775	PASS
441	198	0.01	100	7.5	21358	PASS
442	442	50	100	100.0	136744	PASS
443	442	15	24	22.3	30503	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
 Data File : BN027249.D
 Acq On : 29 Aug 2023 21:06
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 30 02:33:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 02:32:19 2023
 Response via : Initial Calibration

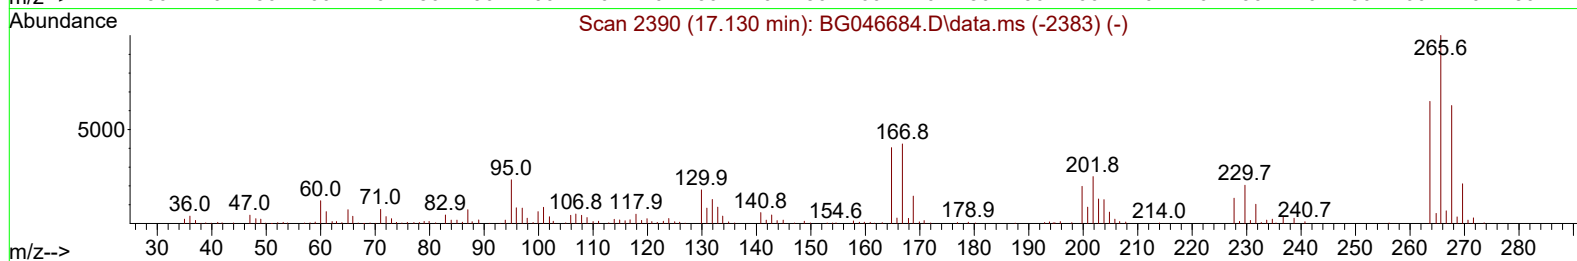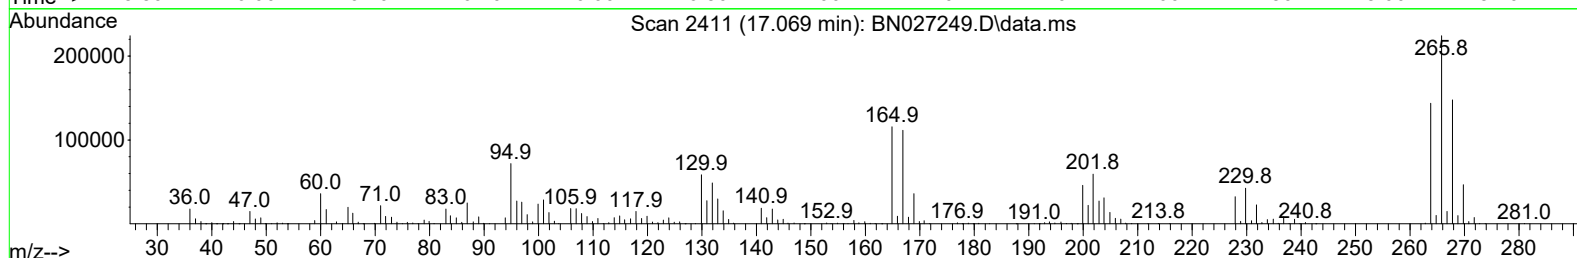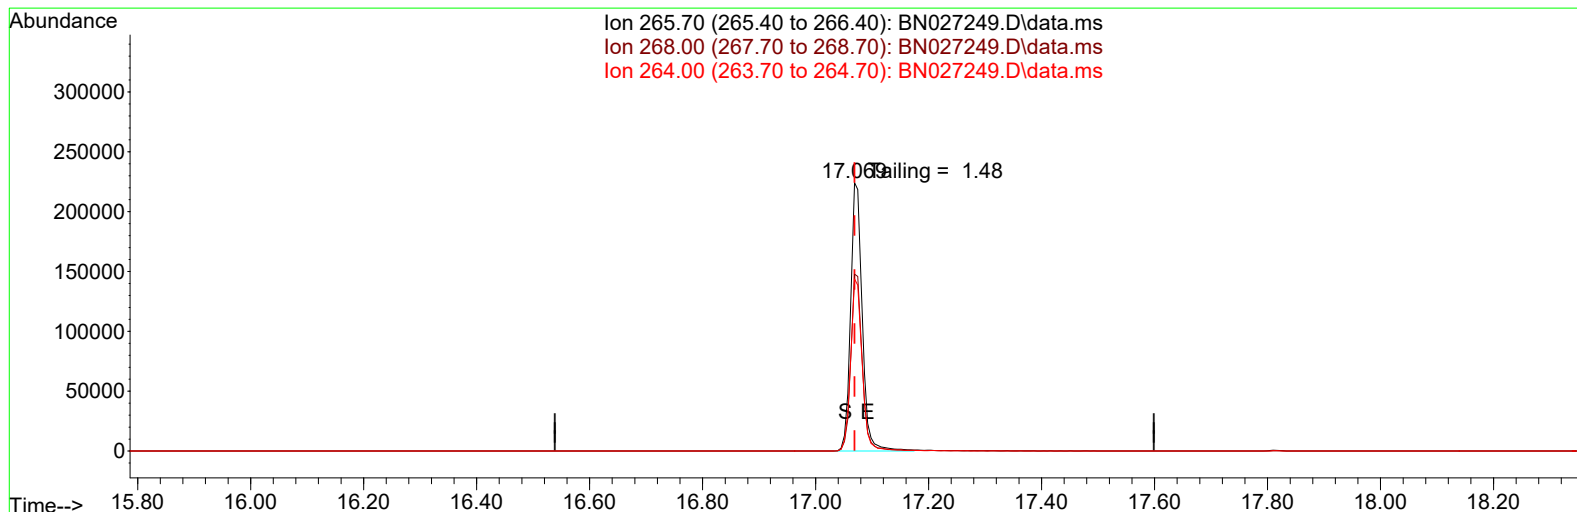

TIC: BN027249.D\data.ms

(70) Pentachlorophenol (C)

17.069min (-0.000) 20390.21 ng




response 325155

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.90
264.00	61.60	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082923\
Data File : BN027249.D
Acq On : 29 Aug 2023 21:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 30 02:33:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 02:32:19 2023
Response via : Initial Calibration

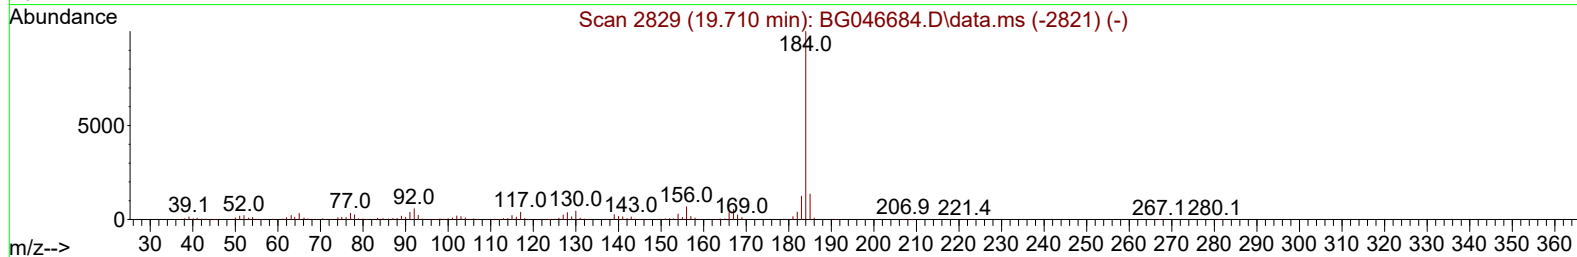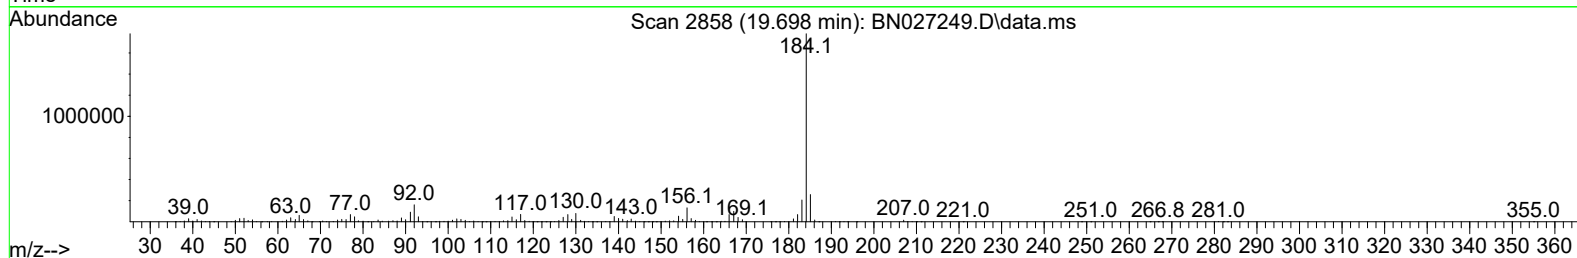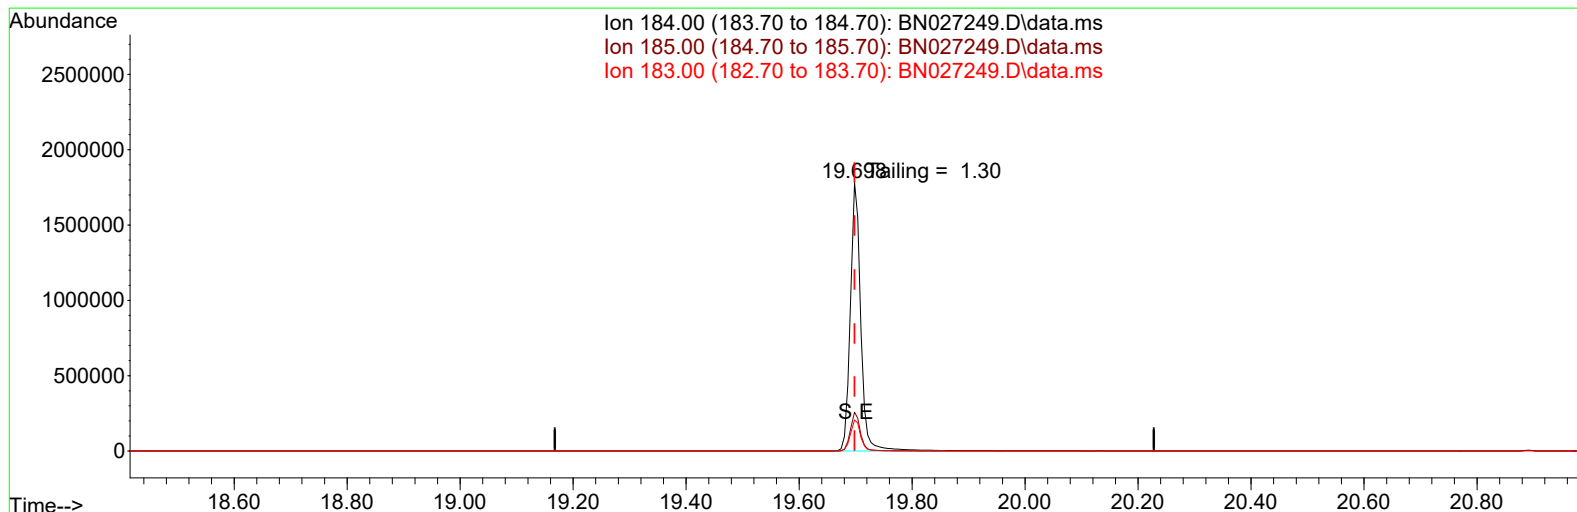

TIC: BN027249.D\data.ms

(77) Benzidine

19.698min (-0.000) 0.00 ng

response 2304744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.50
183.00	13.20	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/29/2023	BNA_N	<u>BN027249.D</u>
Compound Name	Response	Retention Time
DDT	1051193	20.892
DDD	19027	20.457
DDE	741	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19768	1070961	1.85

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP