

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
 Data File : BN033677.D
 Acq On : 29 Aug 2024 19:45
 Operator : MA/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Aug 29 23:25:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 29 23:20:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.530	152	5921	0.400	ng	0.00
7) Naphthalene-d8	10.293	136	14709	0.400	ng	0.00
13) Acenaphthene-d10	14.167	164	7002	0.400	ng	0.00
19) Phenanthrene-d10	16.917	188	13601	0.400	ng	0.00
29) Chrysene-d12	21.121	240	11201	0.400	ng	0.00
35) Perylene-d12	23.282	264	11292	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.169	112	84608	4.496	ng	0.00
5) Phenol-d6	6.722	99	103969	4.644	ng	0.00
8) Nitrobenzene-d5	8.659	82	62085	5.090	ng	0.00
11) 2-Methylnaphthalene-d10	11.884	152	104495	4.966	ng	0.00
14) 2,4,6-Tribromophenol	15.663	330	18641	4.952	ng	0.00
15) 2-Fluorobiphenyl	12.777	172	145128	5.074	ng	0.00
27) Fluoranthene-d10	18.956	212	172261	5.269	ng	0.00
31) Terphenyl-d14	19.569	244	117029	4.597	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.175	88	31490	4.622	ng	99
3) n-Nitrosodimethylamine	3.457	42	38688	4.883	ng	98
6) bis(2-Chloroethyl)ether	6.967	93	76446	4.816	ng	100
9) Naphthalene	10.336	128	194289	4.943	ng	98
10) Hexachlorobutadiene	10.635	225	39436	5.030	ng	# 99
12) 2-Methylnaphthalene	11.960	142	121558	4.886	ng	98
16) Acenaphthylene	13.879	152	161908	5.272	ng	100
17) Acenaphthene	14.231	154	106054	4.910	ng	98
18) Fluorene	15.226	166	132733	4.875	ng	100
20) 4,6-Dinitro-2-methylph...	15.300	198	12809	6.031	ng	# 60
21) 4-Bromophenyl-phenylether	16.122	248	40395	4.890	ng	94
22) Hexachlorobenzene	16.222	284	44785	4.911	ng	99
23) Atrazine	16.396	200	33204	5.035	ng	99
24) Pentachlorophenol	16.569	266	21479	5.435	ng	98
25) Phenanthrene	16.954	178	190525	5.035	ng	100
26) Anthracene	17.041	178	175045	5.228	ng	100
28) Fluoranthene	18.989	202	220041	5.262	ng	100
30) Pyrene	19.351	202	224678	4.494	ng	99
32) Benzo(a)anthracene	21.103	228	201028	4.964	ng	99
33) Chrysene	21.157	228	198885	4.941	ng	99
34) Bis(2-ethylhexyl)phtha...	21.068	149	110430	4.308	ng	# 86
36) Indeno(1,2,3-cd)pyrene	25.422	276	242688	5.177	ng	100
37) Benzo(b)fluoranthene	22.642	252	206618	4.900	ng	# 88
38) Benzo(k)fluoranthene	22.683	252	208139	5.015	ng	# 87
39) Benzo(a)pyrene	23.189	252	179174	5.135	ng	# 83
40) Dibenzo(a,h)anthracene	25.440	278	194015	5.176	ng	94
41) Benzo(g,h,i)perylene	26.071	276	207672	5.181	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033677.D
Acq On : 29 Aug 2024 19:45
Operator : MA/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Quant Time: Aug 29 23:25:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 29 23:20:50 2024
Response via : Initial Calibration

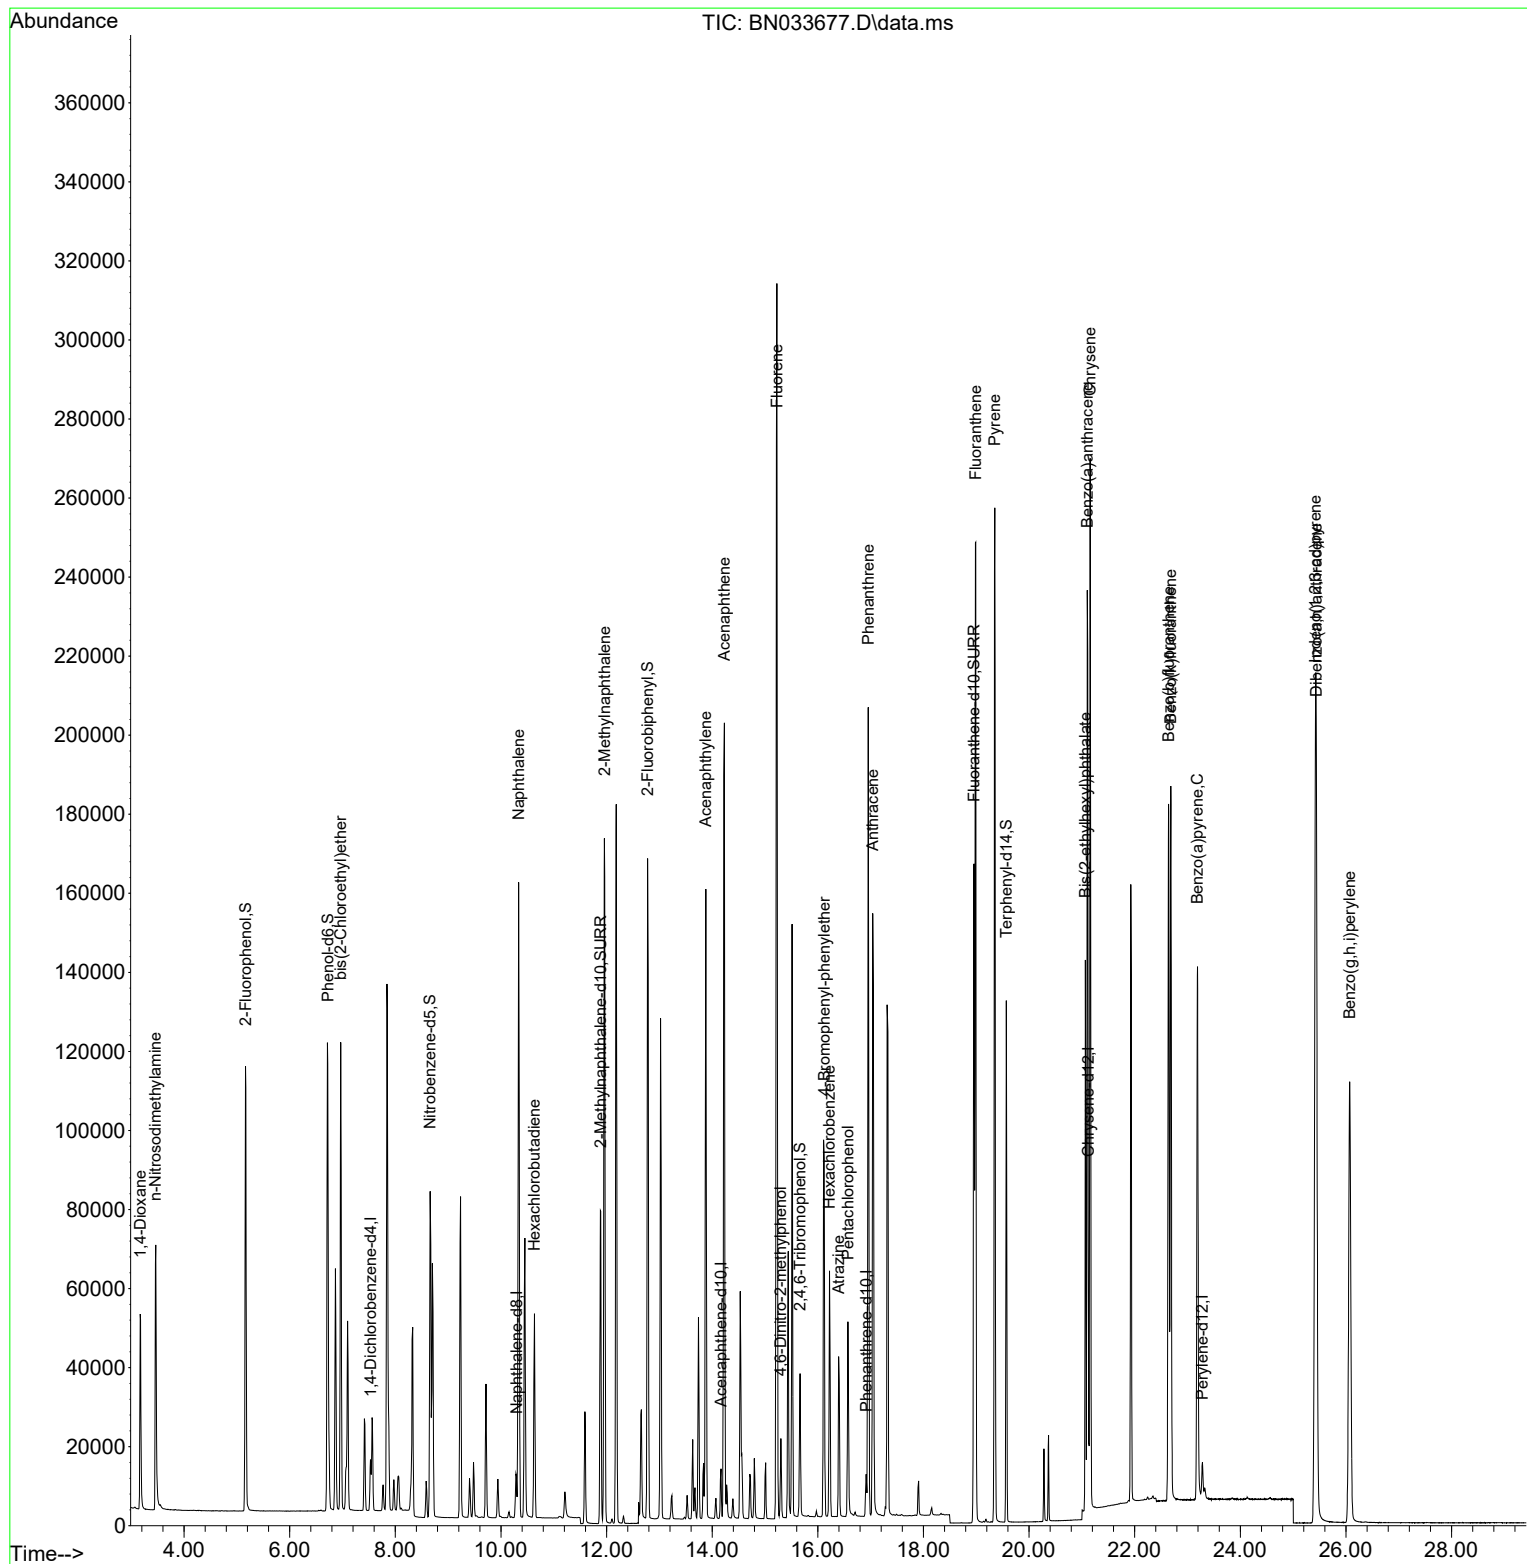






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.530 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN033677.D
 Acq: 29 Aug 2024 19:45


Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0





Tgt Ion:152 Resp: 5921
 Ion Ratio Lower Upper
 152 100
 150 154.9 123.4 185.0
 115 62.4 51.3 76.9




#2
 1,4-Dioxane
 Concen: 4.622 ng
 RT: 3.175 min Scan# 27
 Delta R.T. 0.000 min
 Lab File: BN033677.D
 Acq: 29 Aug 2024 19:45

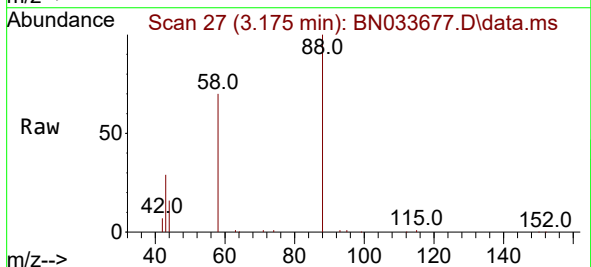

Tgt Ion: 88 Resp: 31490
 Ion Ratio Lower Upper
 88 100
 43 32.1 26.8 40.2
 58 79.0 63.4 95.0

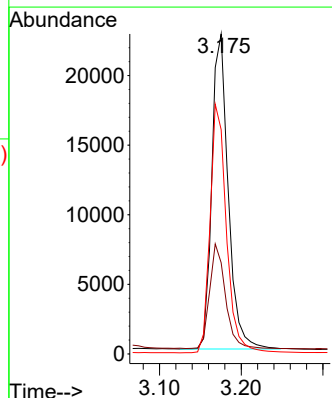



#3

n-Nitrosodimethylamine

Concen: 4.883 ng

RT: 3.457 min Scan# 6

Delta R.T. -0.007 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion: 42 Resp: 38688

Ion Ratio Lower Upper

42 100

74 116.4 91.8 137.6

44 6.5 6.2 9.4

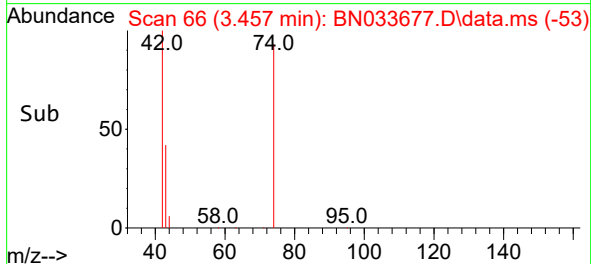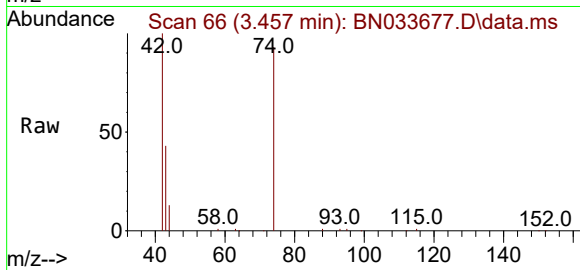

#4

2-Fluorophenol

Concen: 4.496 ng

RT: 5.169 min Scan# 303

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45




Tgt Ion: 112 Resp: 84608


Ion Ratio Lower Upper

112 100

64 59.7 48.6 72.8

63 31.9 26.6 39.8


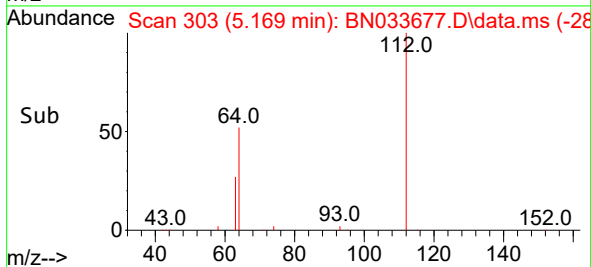

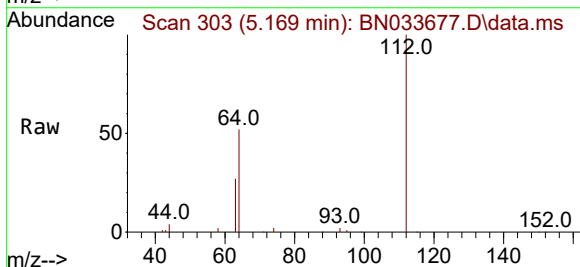




#5
Phenol-d6
Concen: 4.644 ng
RT: 6.722 min Scan# 518
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 103969
Ion Ratio Lower Upper
99 100
42 21.4 17.8 26.8
71 34.7 28.0 42.0

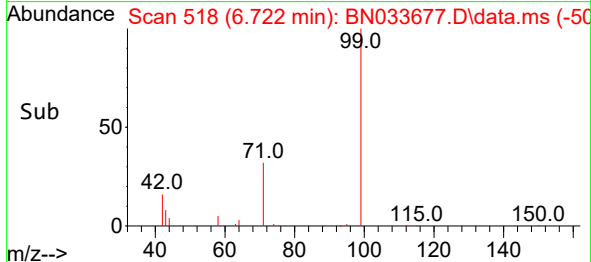

#6
bis(2-Chloroethyl)ether
Concen: 4.816 ng
RT: 6.967 min Scan# 552
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45

Tgt Ion: 93 Resp: 76446
Ion Ratio Lower Upper
93 100
63 79.9 63.9 95.9
95 32.7 26.4 39.6


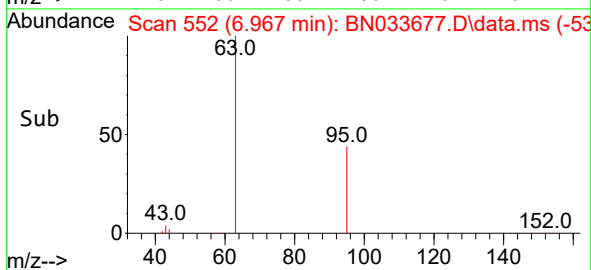

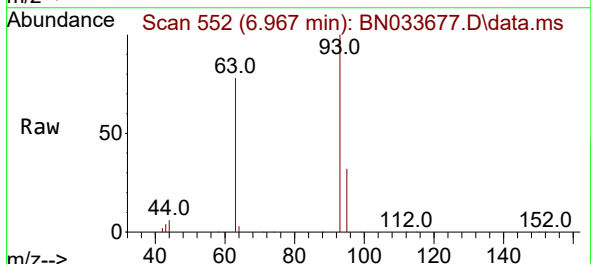




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.293 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	14709
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.1	13.7
54	6.9	5.8	8.6
68	5.2	4.2	6.2

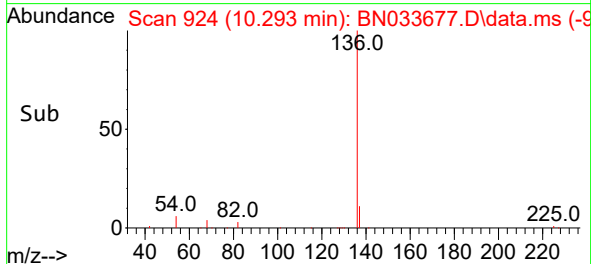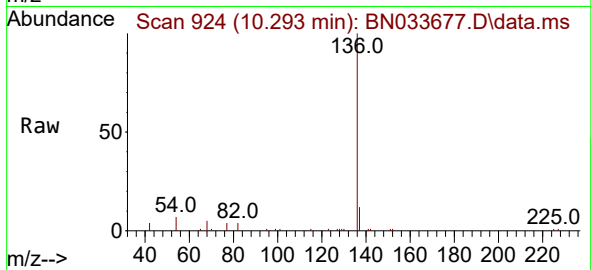

#8
Nitrobenzene-d5
Concen: 5.090 ng
RT: 8.659 min Scan# 771
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45

Tgt Ion:	82	Resp:	62085
Ion	Ratio	Lower	Upper
82	100		
128	36.8	29.3	43.9
54	58.1	49.4	74.0

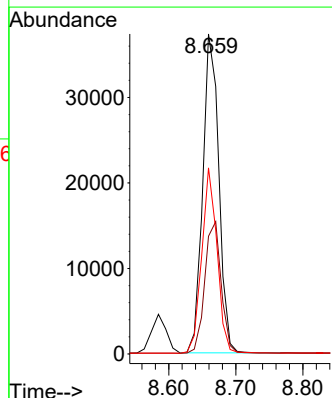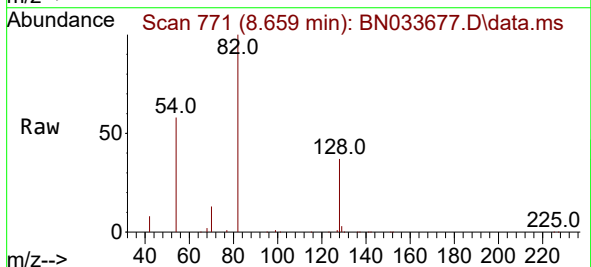



#9

Naphthalene

Concen: 4.943 ng

RT: 10.336 min Scan# 91

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:128 Resp: 194289

Ion Ratio Lower Upper

128 100

129 10.9 9.4 14.0

127 13.1 11.0 16.4



#10

Hexachlorobutadiene

Concen: 5.030 ng

RT: 10.635 min Scan# 956

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45




Tgt Ion:225 Resp: 39436


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.6 51.4 77.0

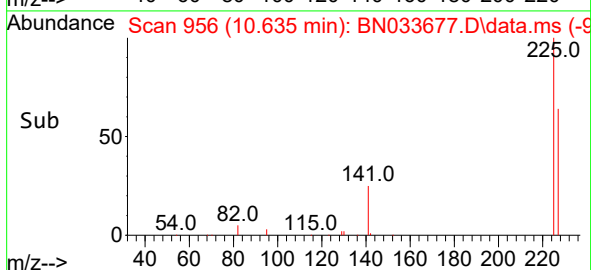



#11

2-Methylnaphthalene-d10

Concen: 4.966 ng

RT: 11.884 min Scan# 1138

Delta R.T. -0.003 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45

Instrument :

BNA_N

ClientSampleId :





SSTDICC5.0

Tgt Ion:152 Resp: 104495

Ion Ratio Lower Upper

152 100

151 20.6 16.7 25.1

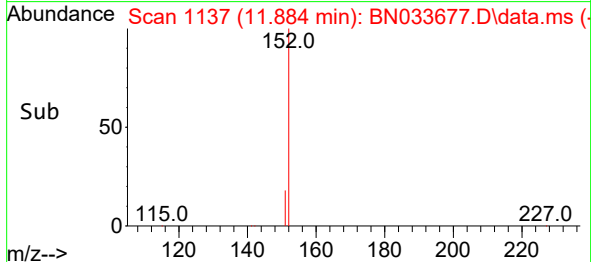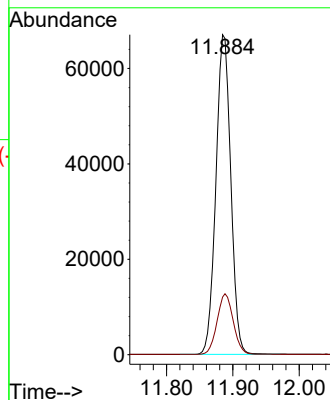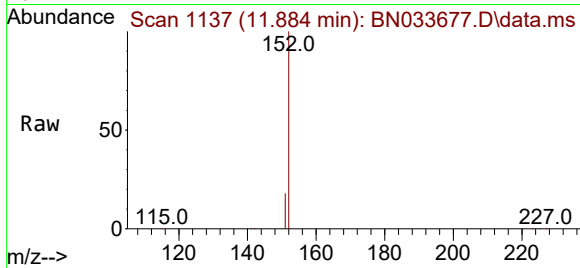

#12

2-Methylnaphthalene

Concen: 4.886 ng

RT: 11.960 min Scan# 1157

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45




Tgt Ion:142 Resp: 121558


Ion Ratio Lower Upper

142 100

141 88.5 71.8 107.8

115 36.8 31.4 47.0


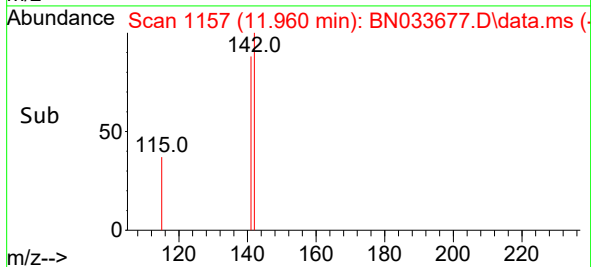
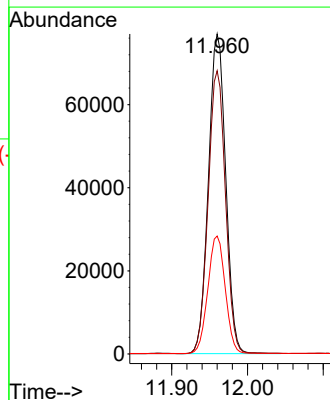
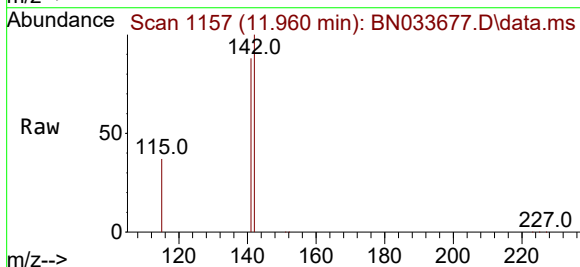


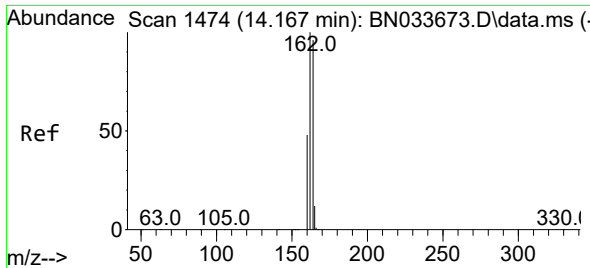

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.167 min Scan# 1474
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 7002
Ion Ratio Lower Upper
164 100
162 103.9 83.4 125.2
160 49.3 40.2 60.2

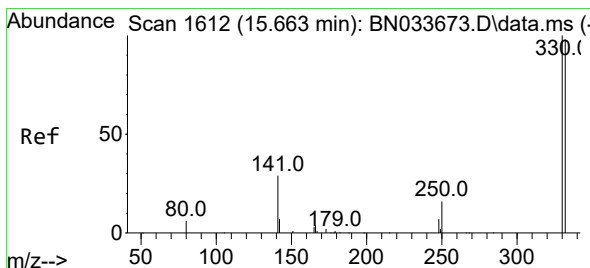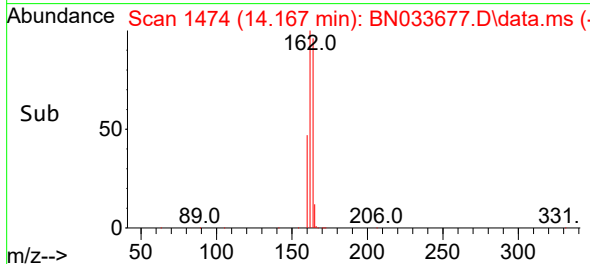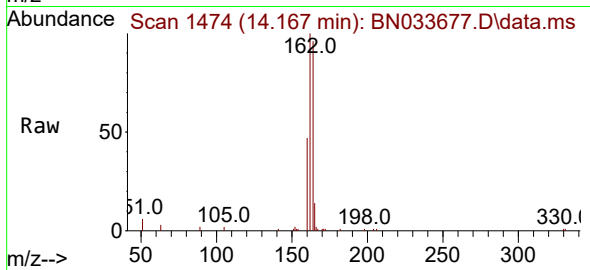

#14
2,4,6-Tribromophenol
Concen: 4.952 ng
RT: 15.663 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45

Tgt Ion:330 Resp: 18641
Ion Ratio Lower Upper
330 100
332 97.3 78.6 118.0
141 43.7 35.0 52.6

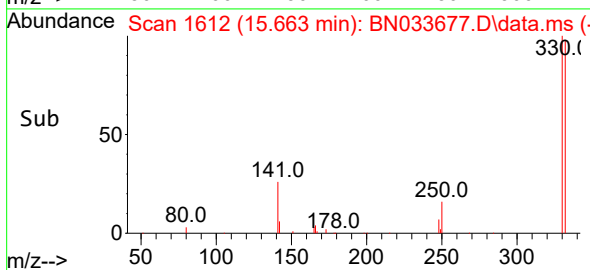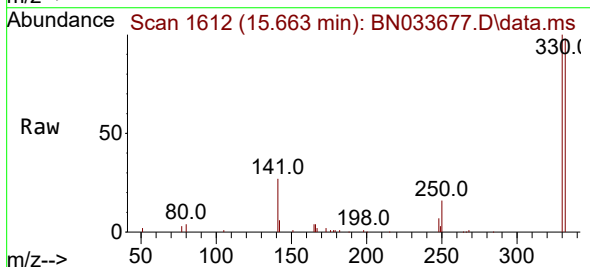



#15

2-Fluorobiphenyl

Concen: 5.074 ng

RT: 12.777 min Scan# 1344

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:172 Resp: 145128

Ion Ratio Lower Upper

172 100

171 35.8 29.2 43.8

170 24.2 19.7 29.5

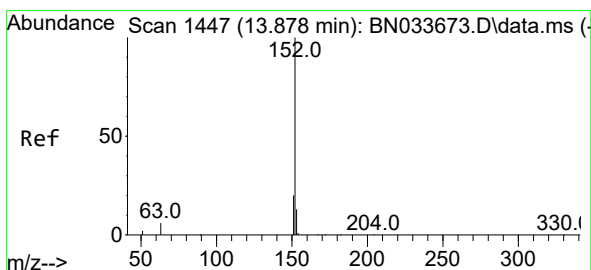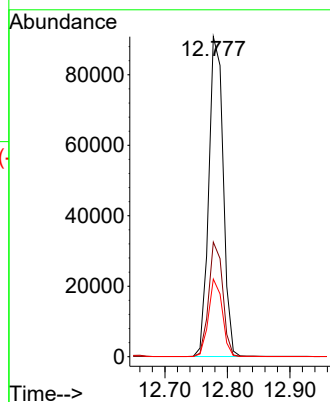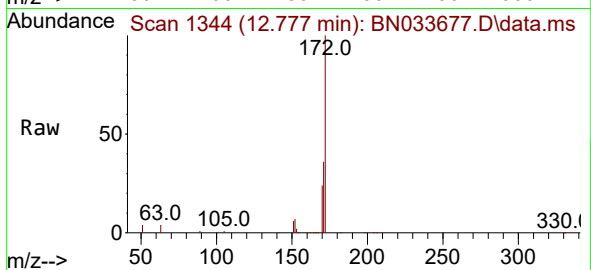

#16

Acenaphthylene

Concen: 5.272 ng

RT: 13.879 min Scan# 1447

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45




Tgt Ion:152 Resp: 161908


Ion Ratio Lower Upper

152 100

151 19.5 15.6 23.4

153 13.0 10.3 15.5

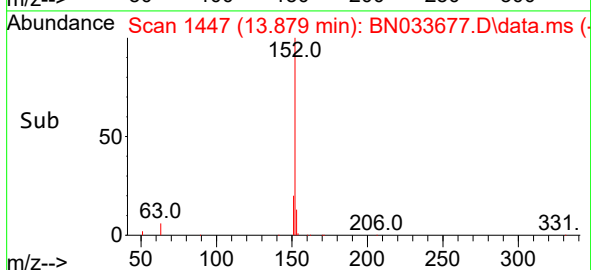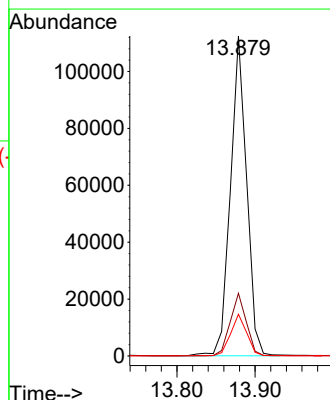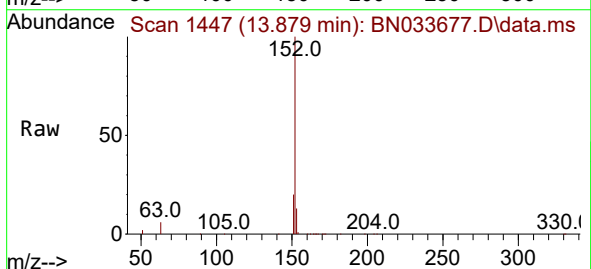



#17

Acenaphthene

Concen: 4.910 ng

RT: 14.231 min Scan# 1480

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:154 Resp: 106054

Ion Ratio Lower Upper

154 100

153 113.0 91.8 137.8

152 55.9 45.4 68.2

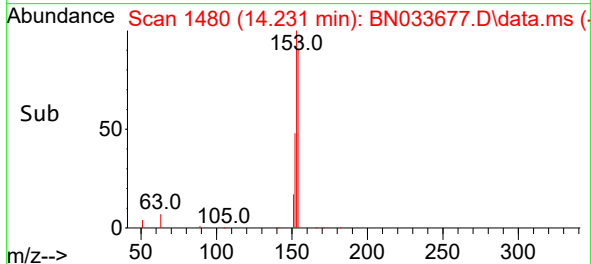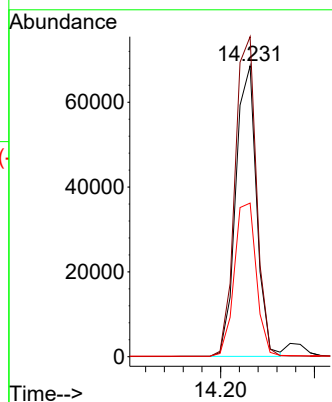

#18

Fluorene

Concen: 4.875 ng

RT: 15.226 min Scan# 1573

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45




Tgt Ion:166 Resp: 132733


Ion Ratio Lower Upper

166 100

165 98.4 78.6 118.0

167 13.3 10.7 16.1


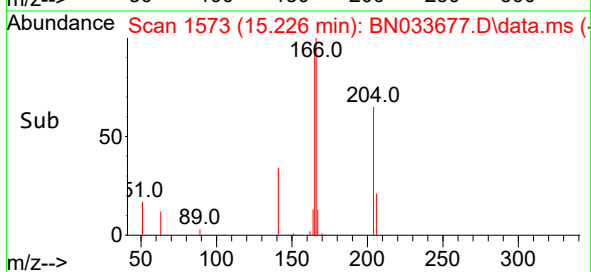
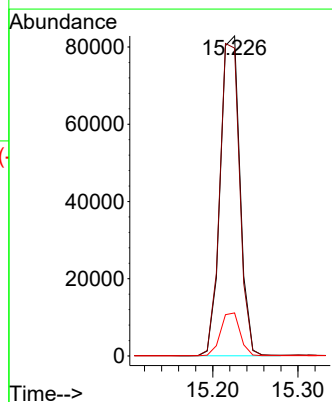



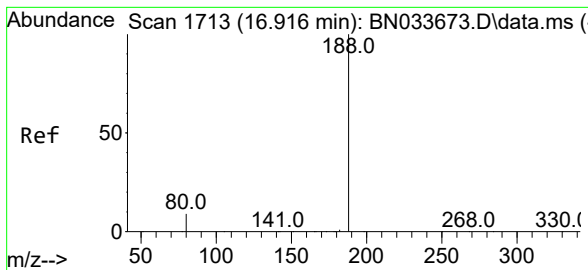

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.917 min Scan# 1713
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 13601
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.7 7.4 11.0

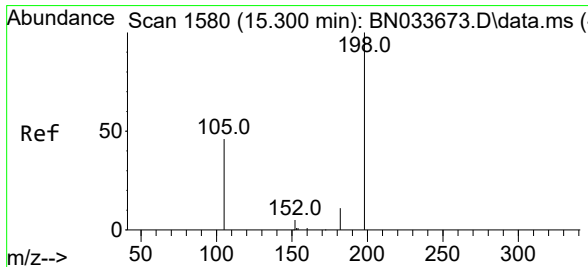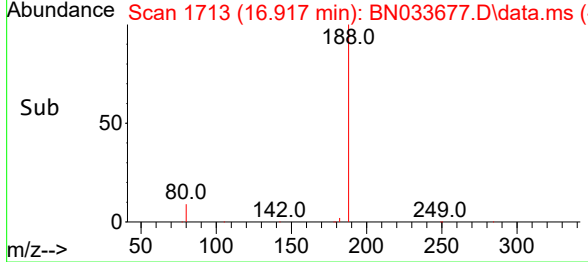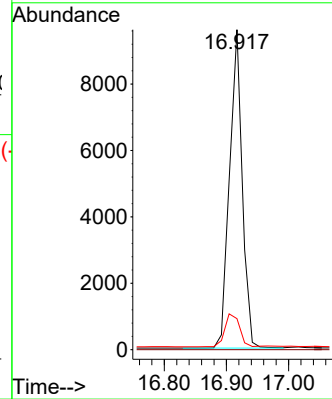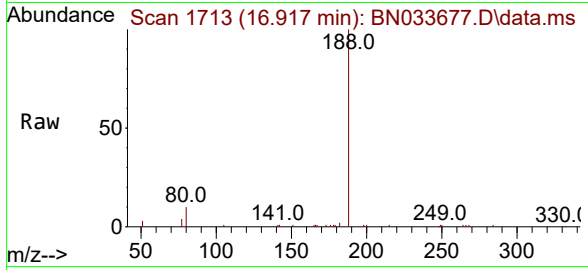

#20
4,6-Dinitro-2-methylphenol
Concen: 6.031 ng
RT: 15.300 min Scan# 1580
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45

Tgt Ion:198 Resp: 12809
Ion Ratio Lower Upper
198 100
51 50.8 82.9 124.3#
105 48.9 53.4 80.0#


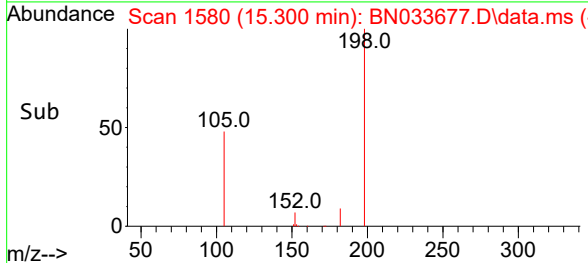
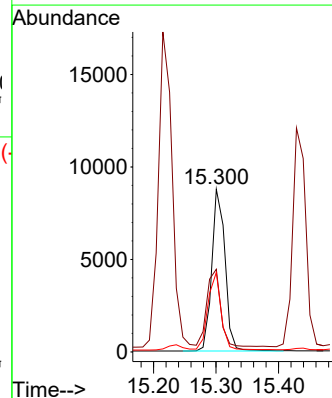
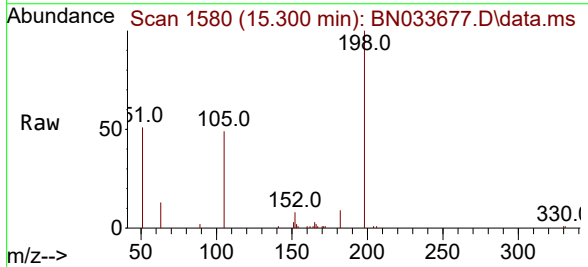




#21
4-Bromophenyl-phenylether
Concen: 4.890 ng
RT: 16.122 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 40395
Ion Ratio Lower Upper
248 100
250 102.0 79.0 118.4
141 41.3 38.5 57.7

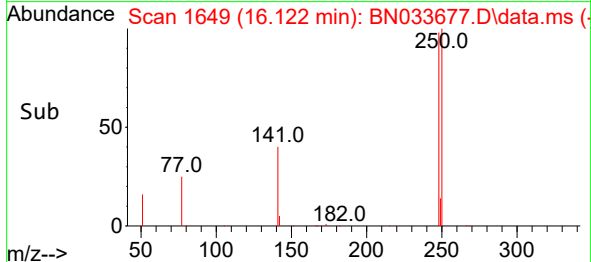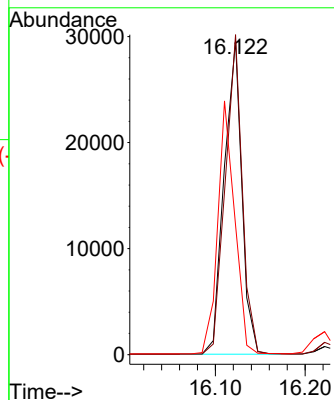

#22
Hexachlorobenzene
Concen: 4.911 ng
RT: 16.222 min Scan# 1657
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45

Tgt Ion:284 Resp: 44785
Ion Ratio Lower Upper
284 100
142 41.7 34.0 51.0
249 32.3 26.2 39.2

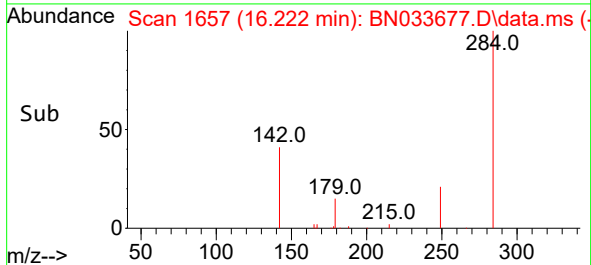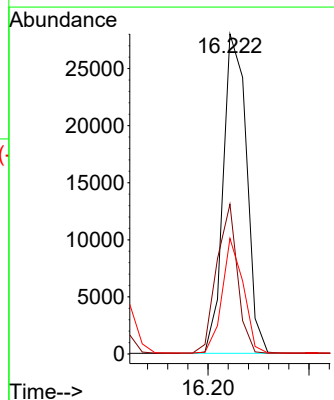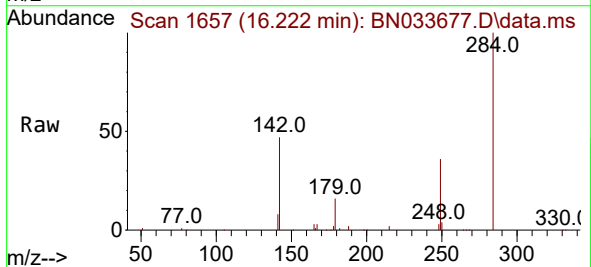



#23

Atrazine

Concen: 5.035 ng

RT: 16.396 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:200 Resp: 33204

Ion Ratio Lower Upper

200 100

173 34.1 27.0 40.4

215 43.3 35.5 53.3

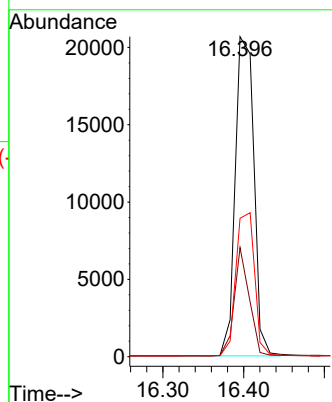

#24

Pentachlorophenol

Concen: 5.435 ng

RT: 16.569 min Scan# 1685

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45




Tgt Ion:266 Resp: 21479


Ion Ratio Lower Upper

266 100

264 62.8 51.4 77.2

268 63.9 51.9 77.9


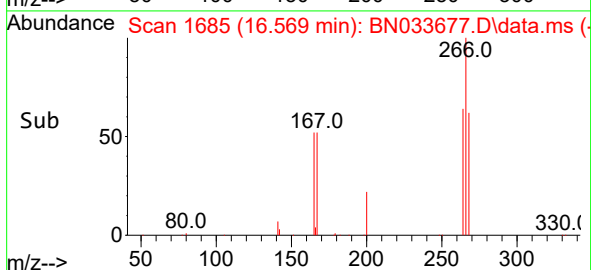




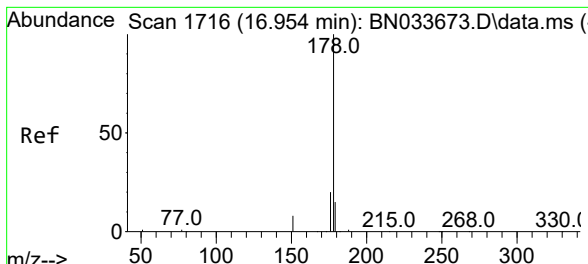

#25
Phenanthrene
Concen: 5.035 ng
RT: 16.954 min Scan# 1716
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 190525
Ion Ratio Lower Upper
178 100
176 19.2 15.4 23.2
179 15.2 12.2 18.2

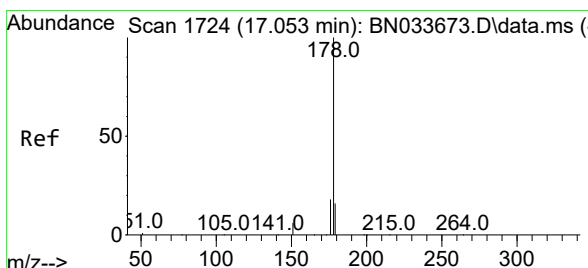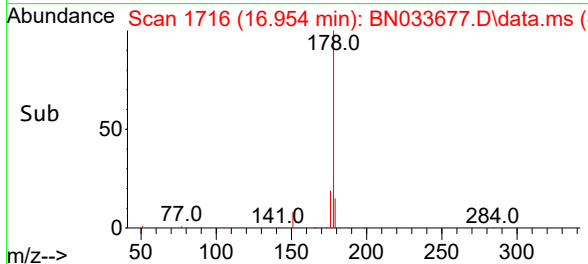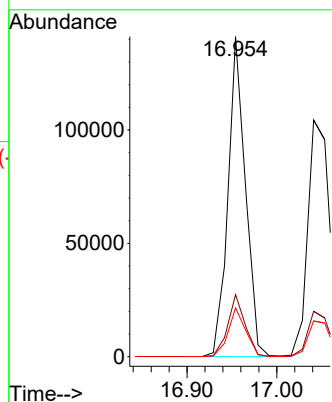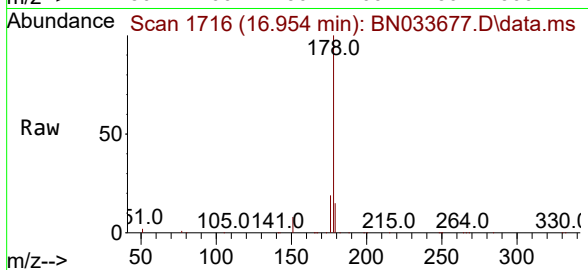

#26
Anthracene
Concen: 5.228 ng
RT: 17.041 min Scan# 1723
Delta R.T. -0.012 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45

Tgt Ion:178 Resp: 175045
Ion Ratio Lower Upper
178 100
176 18.6 14.9 22.3
179 15.2 12.2 18.4

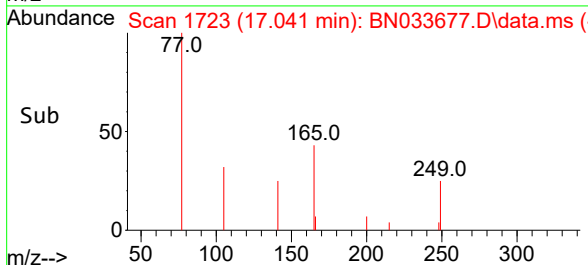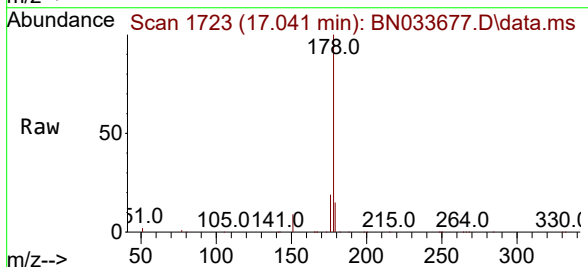



#27

Fluoranthene-d10

Concen: 5.269 ng

RT: 18.956 min Scan# 1938

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:212 Resp: 172261

Ion Ratio Lower Upper

212 100

106 14.7 11.8 17.6

104 8.4 6.9 10.3

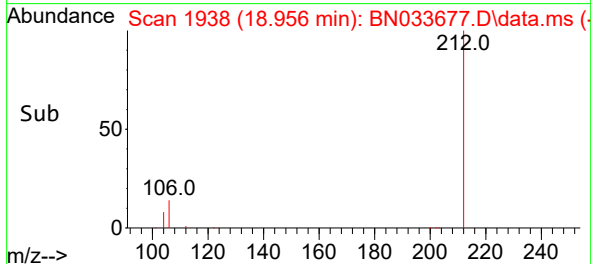

#28

Fluoranthene

Concen: 5.262 ng

RT: 18.989 min Scan# 1945

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45




Tgt Ion:202 Resp: 220041


Ion Ratio Lower Upper

202 100

101 11.6 9.2 13.8

203 17.4 13.8 20.8

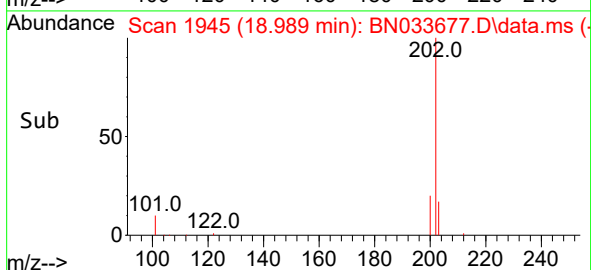

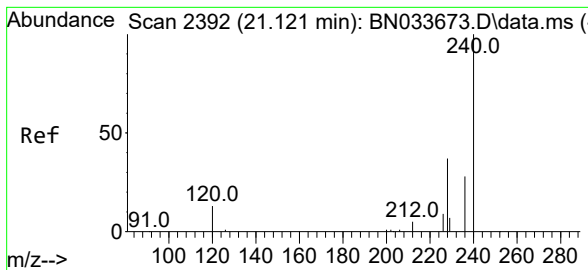

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.121 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:240 Resp: 11201

Ion Ratio Lower Upper

240 100

120 18.0 13.3 19.9

236 29.3 23.4 35.2

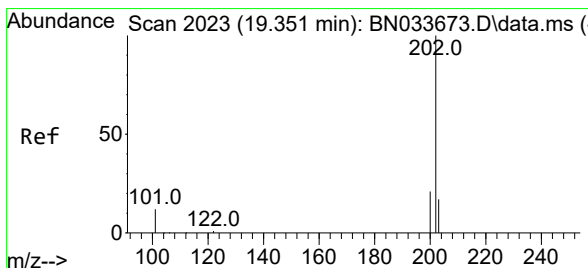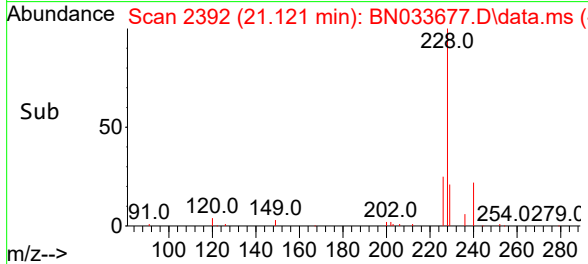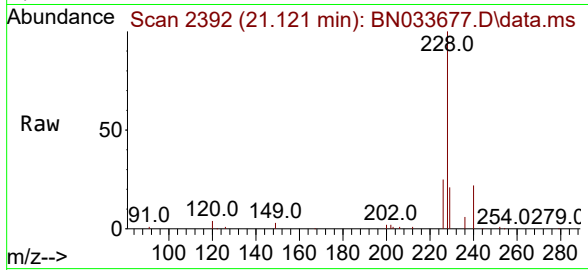

#30

Pyrene

Concen: 4.494 ng

RT: 19.351 min Scan# 2023

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45




Tgt Ion:202 Resp: 224678


Ion Ratio Lower Upper

202 100

200 20.9 16.8 25.2

203 17.7 14.5 21.7


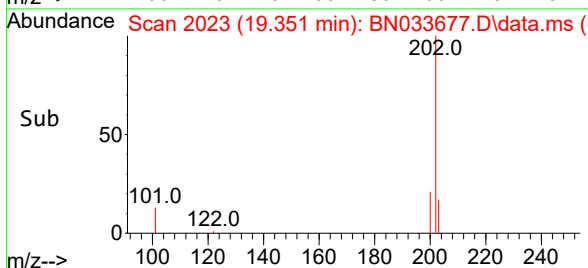
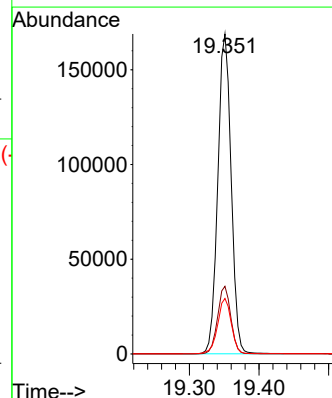
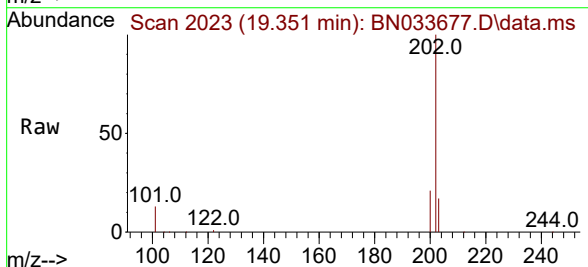




#31
 Terphenyl-d14
 Concen: 4.597 ng
 RT: 19.569 min Scan# 2070
 Delta R.T. 0.000 min
 Lab File: BN033677.D
 Acq: 29 Aug 2024 19:45




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:244 Resp: 117029
 Ion Ratio Lower Upper
 244 100
 212 9.2 8.2 12.4
 122 16.5 13.6 20.4

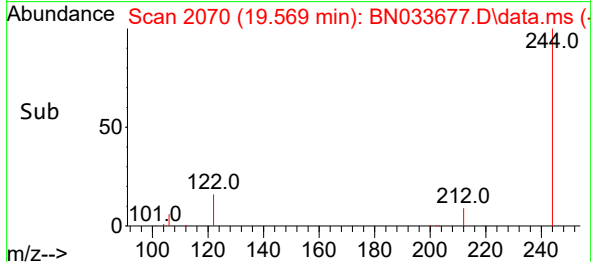

#32
 Benzo(a)anthracene
 Concen: 4.964 ng
 RT: 21.103 min Scan# 2390
 Delta R.T. 0.000 min
 Lab File: BN033677.D
 Acq: 29 Aug 2024 19:45

Tgt Ion:228 Resp: 201028
 Ion Ratio Lower Upper
 228 100
 226 28.2 22.6 34.0
 229 19.1 15.8 23.6

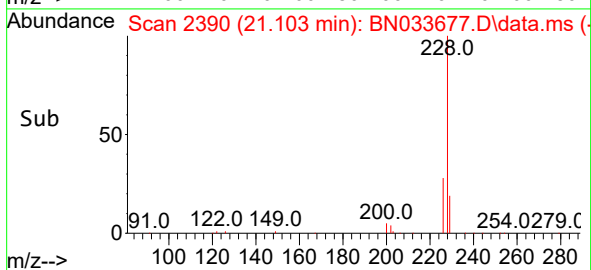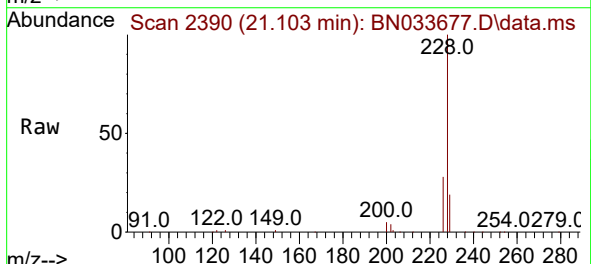

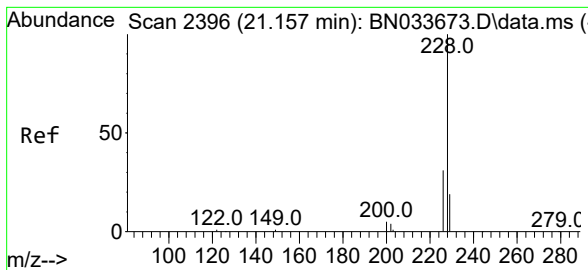

#33

Chrysene

Concen: 4.941 ng

RT: 21.157 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:228 Resp: 198885

Ion Ratio Lower Upper

228 100

226 30.2 24.7 37.1

229 19.3 15.6 23.4

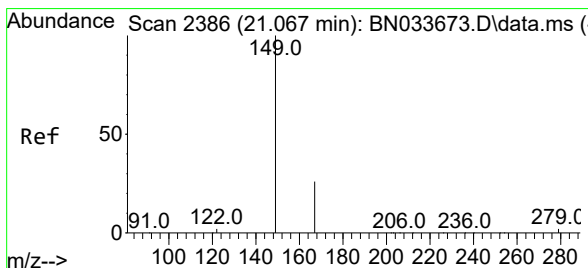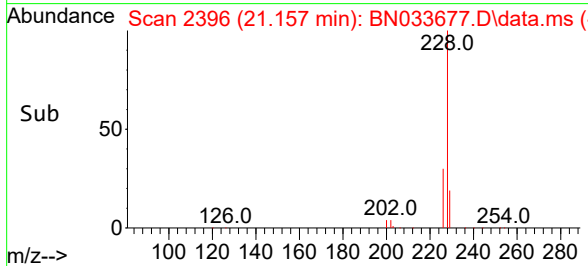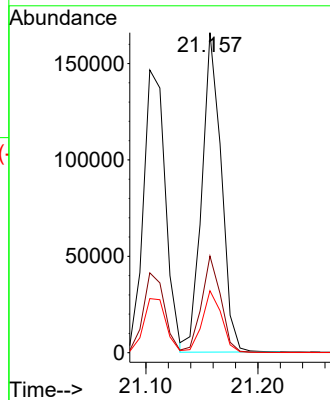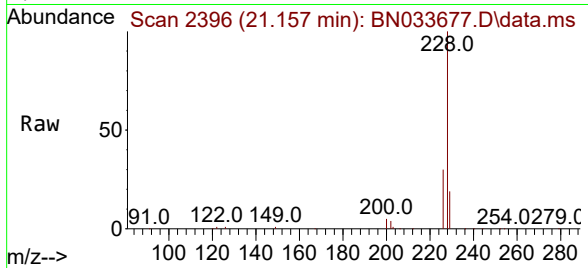

#34

Bis(2-ethylhexyl)phthalate

Concen: 4.308 ng

RT: 21.068 min Scan# 2386

Delta R.T. 0.000 min

Lab File: BN033677.D

Acq: 29 Aug 2024 19:45




Tgt Ion:149 Resp: 110430


Ion Ratio Lower Upper

149 100

167 26.6 28.3 42.5#

279 3.5 4.2 6.2#


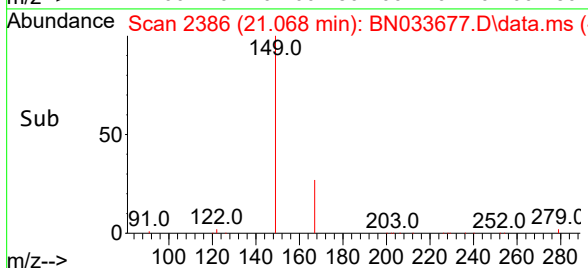
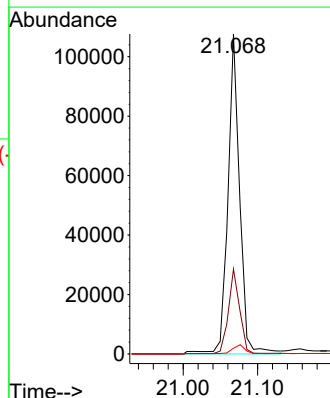
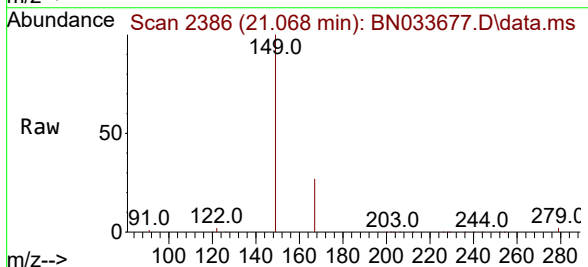




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.282 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:264 Resp: 11292
Ion Ratio Lower Upper
264 100
260 26.3 20.7 31.1
265 88.2 69.9 104.9

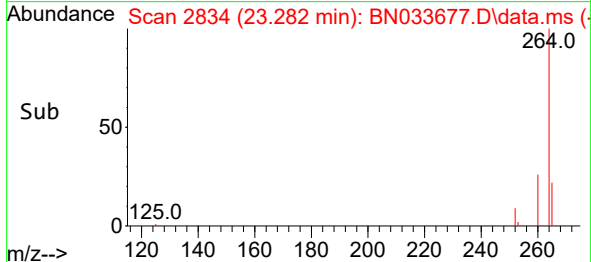

#36
Indeno(1,2,3-cd)pyrene
Concen: 5.177 ng
RT: 25.422 min Scan# 3566
Delta R.T. -0.002 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45

Tgt Ion:276 Resp: 242688
Ion Ratio Lower Upper
276 100
138 29.3 23.3 34.9
277 24.8 19.8 29.6


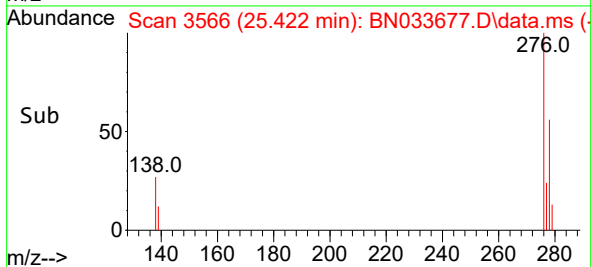

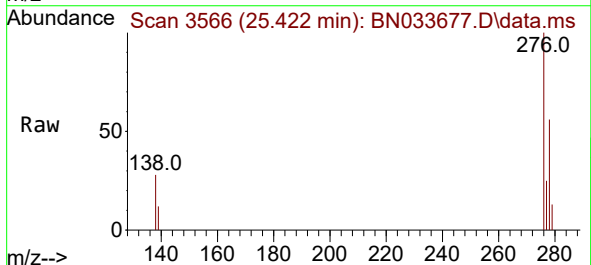




#37
Benzo(b)fluoranthene
Concen: 4.900 ng
RT: 22.642 min Scan# 2615
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 206618
Ion Ratio Lower Upper
252 100
253 22.0 21.6 32.4
125 12.1 15.2 22.8#

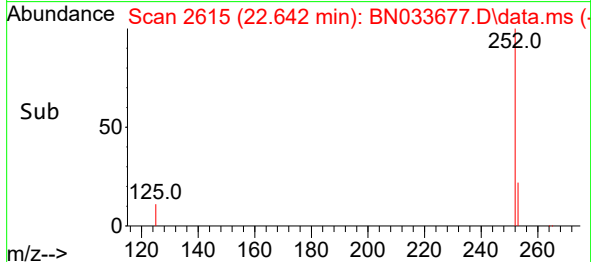

#38
Benzo(k)fluoranthene
Concen: 5.015 ng
RT: 22.683 min Scan# 2629
Delta R.T. -0.002 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45


Tgt Ion:252 Resp: 208139
Ion Ratio Lower Upper
252 100
253 21.8 21.4 32.2
125 11.9 15.8 23.6#

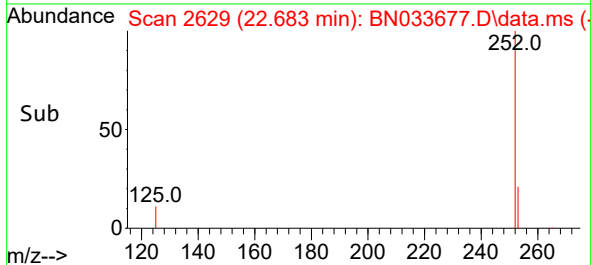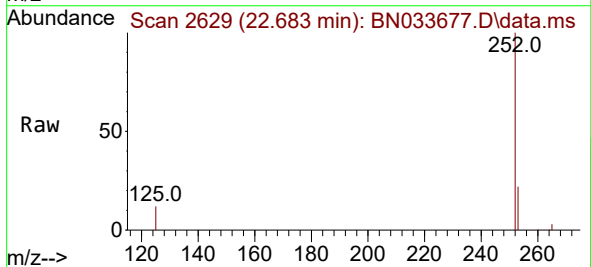






#39
Benzo(a)pyrene
Concen: 5.135 ng
RT: 23.189 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:252 Resp: 179174
Ion Ratio Lower Upper
252 100
253 22.0 23.6 35.4#
125 13.2 18.7 28.1#



#40
Dibenzo(a,h)anthracene
Concen: 5.176 ng
RT: 25.440 min Scan# 3572
Delta R.T. 0.003 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45


Tgt Ion:278 Resp: 194015
Ion Ratio Lower Upper
278 100
139 19.5 17.2 25.8
279 23.7 22.2 33.4

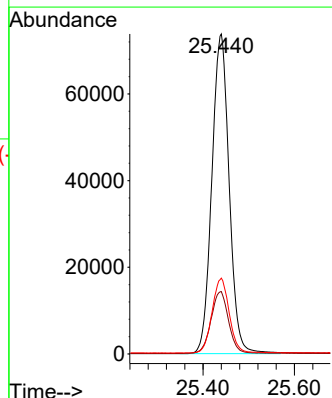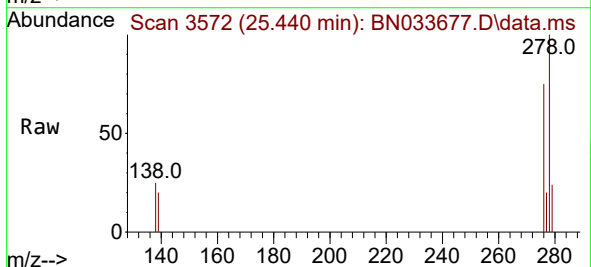

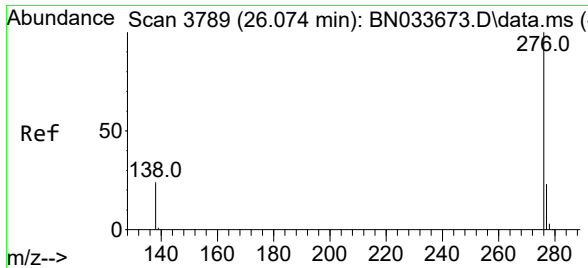

#41
Benzo(g,h,i)perylene
Concen: 5.181 ng
RT: 26.071 min Scan# 31
Delta R.T. -0.003 min
Lab File: BN033677.D
Acq: 29 Aug 2024 19:45

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

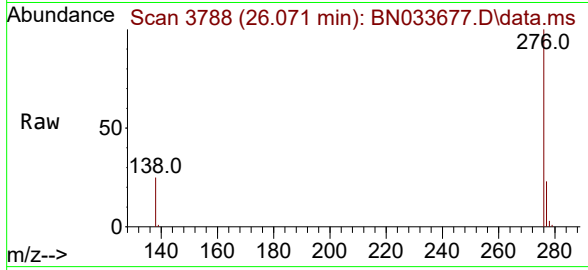

Tgt Ion:276 Resp: 207672
Ion Ratio Lower Upper
276 100
277 23.5 20.2 30.2
138 25.0 21.1 31.7

