
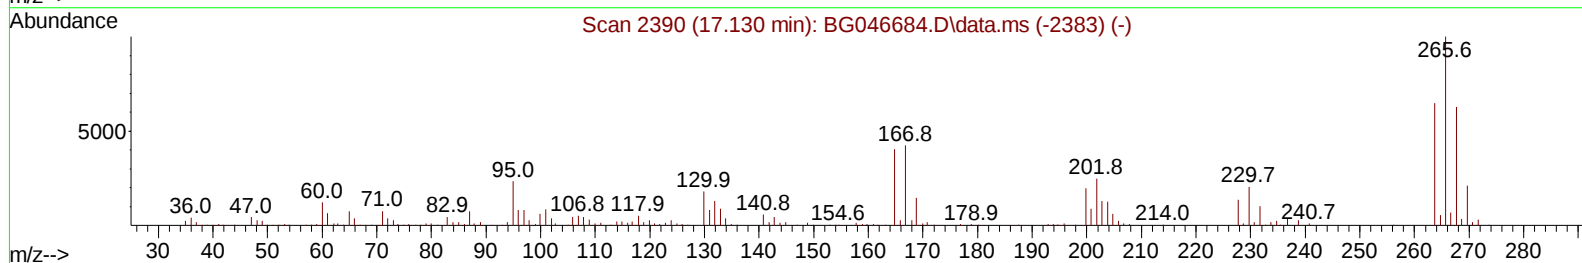
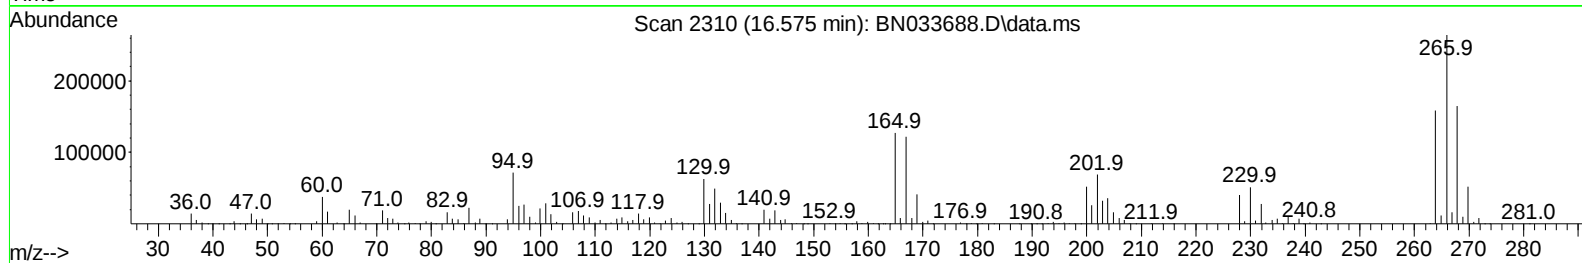


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033688.D
Acq On : 30 Aug 2024 03:38
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 05:54:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 05:53:24 2024
Response via : Initial Calibration

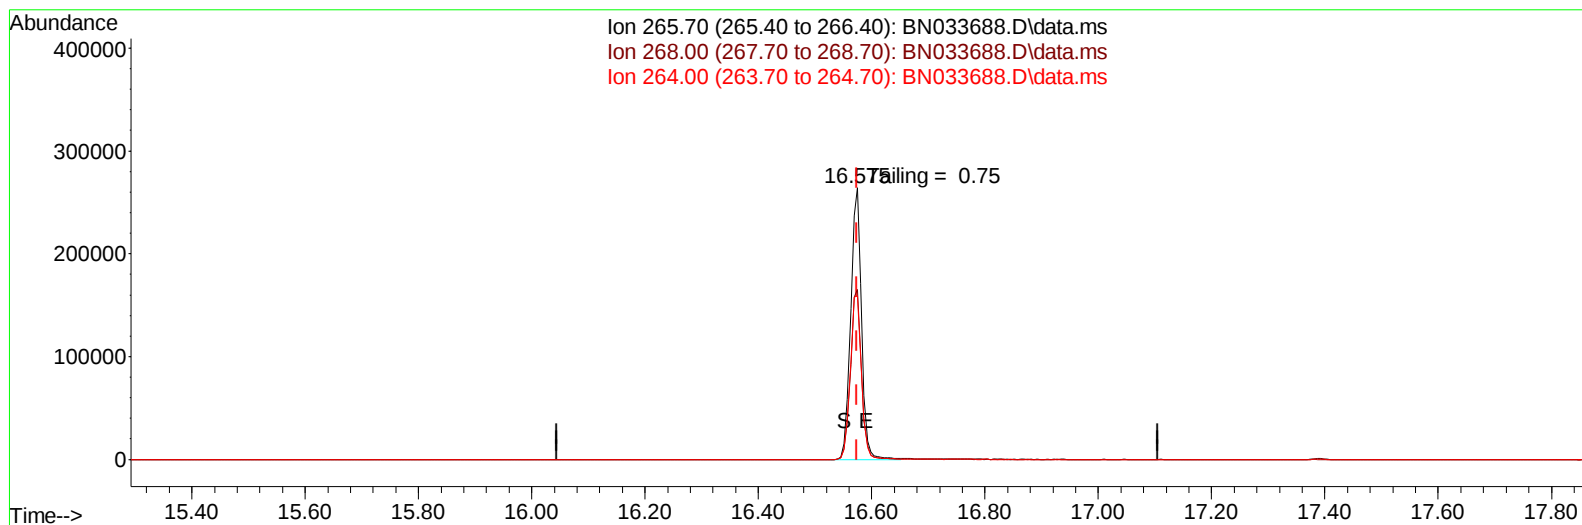

TIC: BN033688.D\data.ms

(70) Pentachlorophenol (C)




16.575min (+ 0.000) 21138.53 ng

response 353843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.55
264.00	61.60	60.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033688.D
Acq On : 30 Aug 2024 03:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 05:54:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 05:53:24 2024
Response via : Initial Calibration

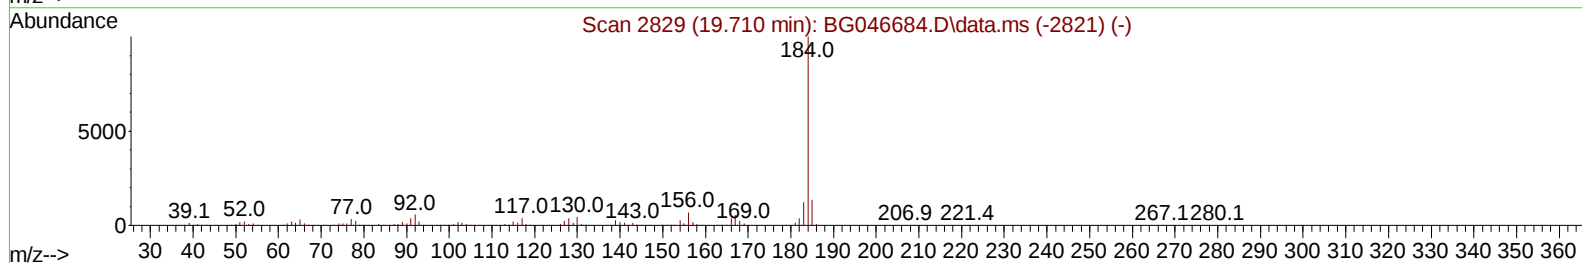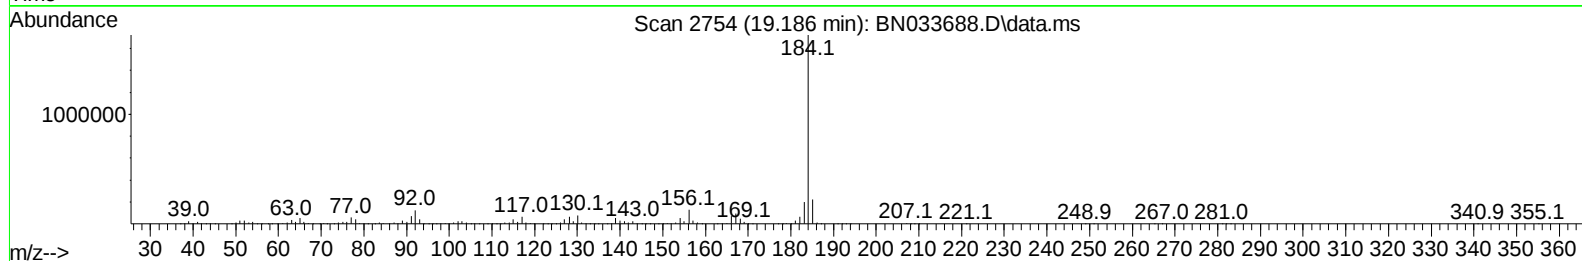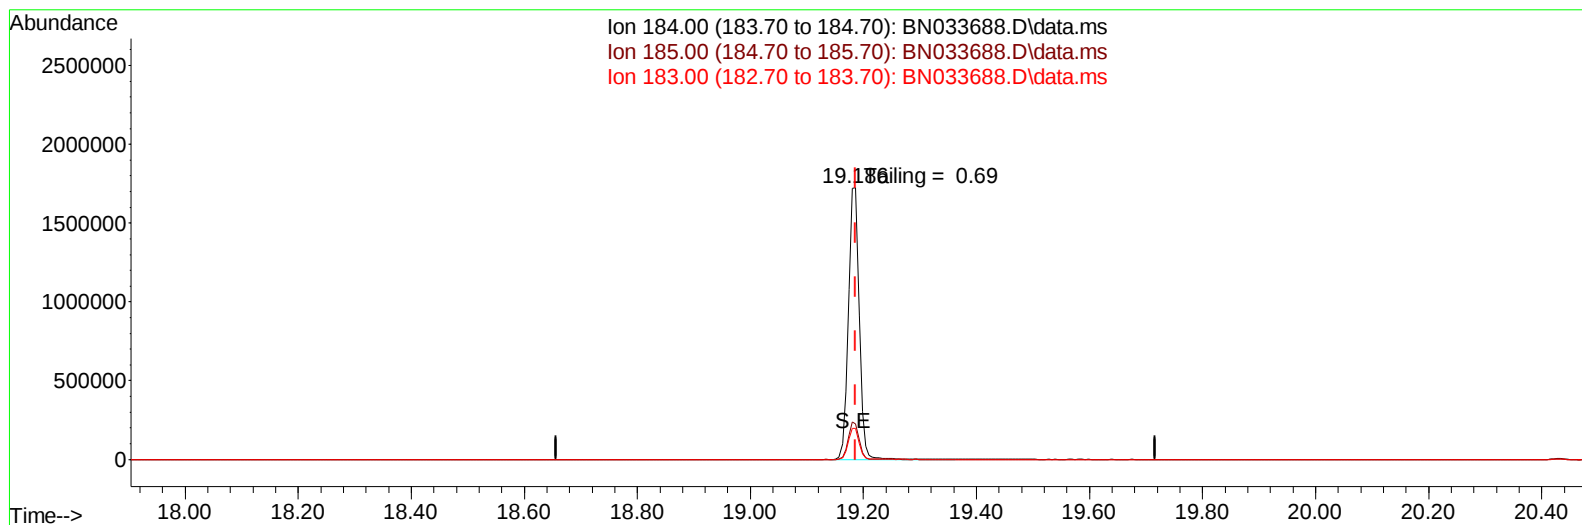

TIC: BN033688.D\data.ms

(77) Benzidine**19.186min (+ 0.000) 0.00 ng****response 2303776**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	11.50
0.00	0.00	0.00