

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
 Data File : BN033698.D
 Acq On : 30 Aug 2024 09:42
 Operator : MA/JU
 Sample : P3769-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 OW-02B-21.2-082724

Quant Time: Aug 30 10:59:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 29 23:33:13 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 09/02/2024
 Supervised By :mohammad ahmed 09/02/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.530	152	5593	0.400	ng	0.00
7) Naphthalene-d8	10.282	136	14523	0.400	ng	#-0.01
13) Acenaphthene-d10	14.157	164	7492	0.400	ng	-0.01
19) Phenanthrene-d10	16.917	188	14418	0.400	ng	0.00
29) Chrysene-d12	21.121	240	12503m	0.400	ng	0.00
35) Perylene-d12	23.285	264	13654	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.169	112	2358	0.140	ng	0.00
5) Phenol-d6	6.722	99	1844	0.093	ng	0.00
8) Nitrobenzene-d5	8.659	82	4047	0.335	ng	0.00
11) 2-Methylnaphthalene-d10	11.881	152	7600	0.371	ng	0.00
14) 2,4,6-Tribromophenol	15.663	330	1454	0.405	ng	0.00
15) 2-Fluorobiphenyl	12.777	172	11041	0.350	ng	0.00
27) Fluoranthene-d10	18.956	212	15922	0.448	ng	0.00
31) Terphenyl-d14	19.569	244	11937	0.451	ng	0.00
Target Compounds						Qvalue
3) n-Nitrosodimethylamine	3.457	42	706	0.092	ng	# 1
9) Naphthalene	10.336	128	1569	0.040	ng	# 64
12) 2-Methylnaphthalene	11.956	142	1116	0.047	ng	# 84
17) Acenaphthene	14.221	154	1701	0.075	ng	# 99
18) Fluorene	15.215	166	2763	0.099	ng	# 39
20) 4,6-Dinitro-2-methylph...	15.290	198	531	0.243	ng	# 1
24) Pentachlorophenol	16.569	266	154	0.036	ng	# 80
25) Phenanthrene	16.954	178	3099	0.077	ng	# 83
26) Anthracene	17.041	178	1302	0.037	ng	# 28
34) Bis(2-ethylhexyl)phtha...	21.068	149	6921m	0.277	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033698.D
Acq On : 30 Aug 2024 09:42
Operator : MA/JU
Sample : P3769-04
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724

Quant Time: Aug 30 10:59:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 29 23:33:13 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

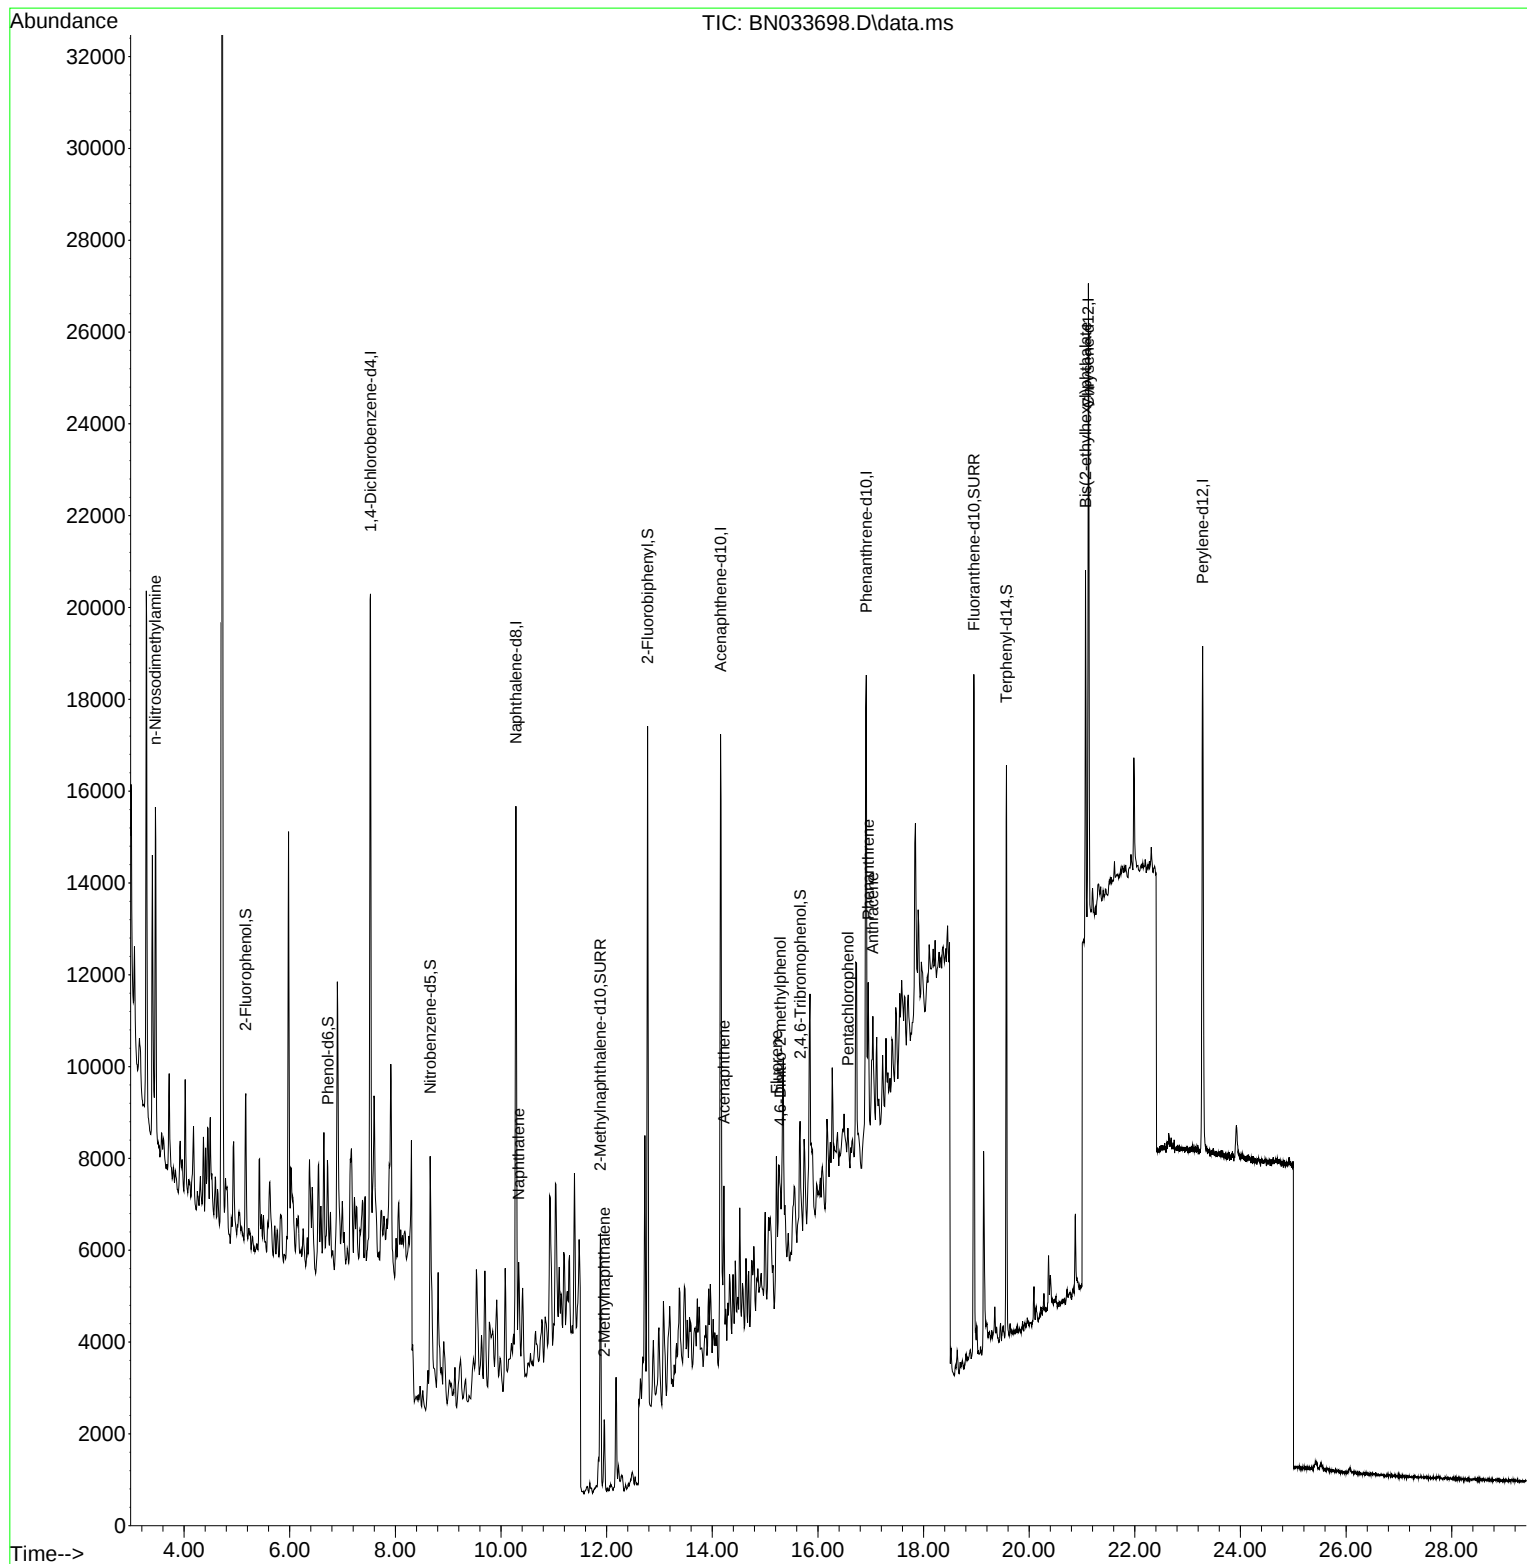

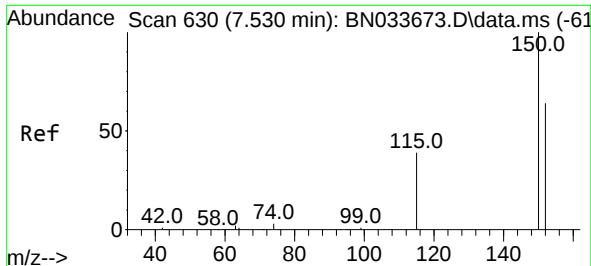

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.530 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724

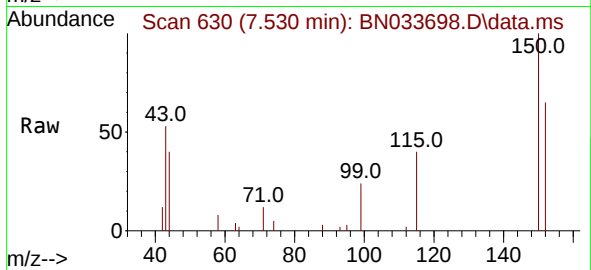

Tgt Ion: 152 Resp: 559
Ion Ratio Lower Upper
152 100
150 153.6 123.4 185.0
115 61.3 51.3 76.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

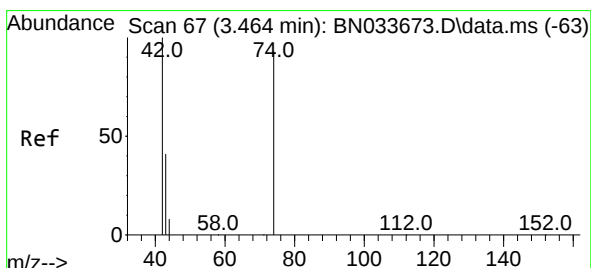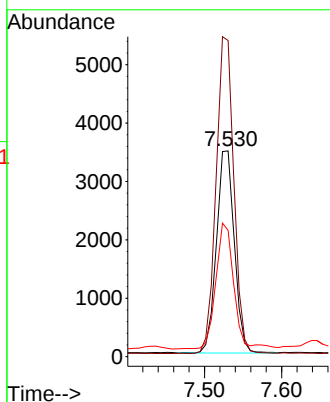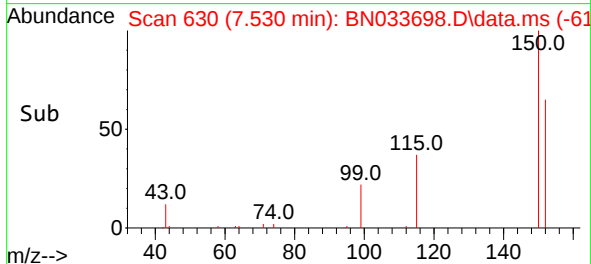

#3
n-Nitrosodimethylamine
Concen: 0.092 ng
RT: 3.457 min Scan# 66
Delta R.T. -0.007 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42


Tgt Ion: 42 Resp: 706
Ion Ratio Lower Upper
42 100
74 2.4 91.8 137.6#
44 31.0 6.2 9.4#

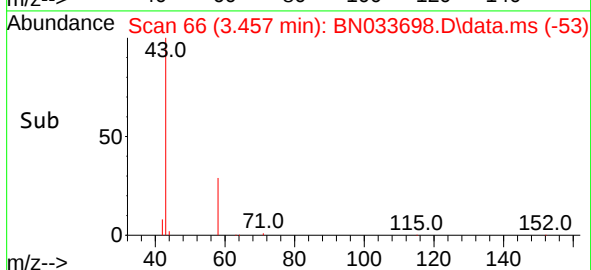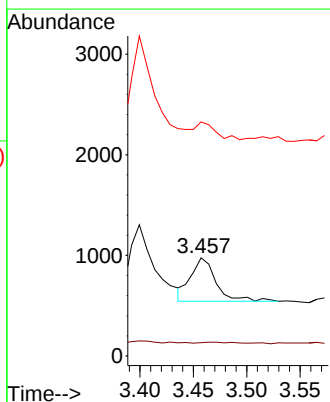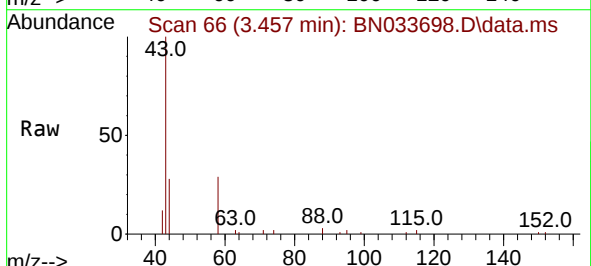

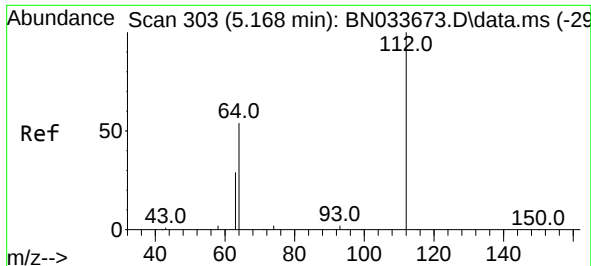

#4
2-Fluorophenol
Concen: 0.140 ng
RT: 5.169 min Scan# 303
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724

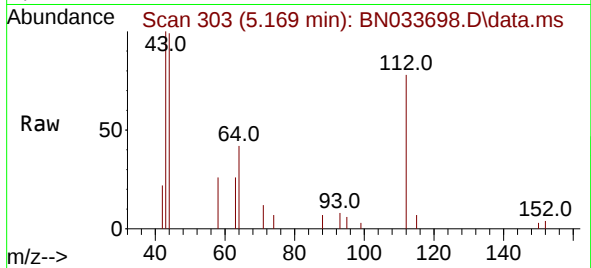

Tgt Ion:112 Resp: 2358
Ion Ratio Lower Upper
112 100
64 56.6 48.6 72.8
63 30.3 26.6 39.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

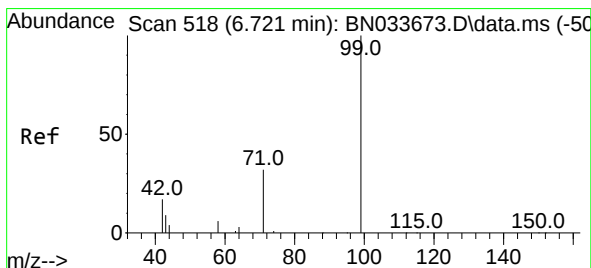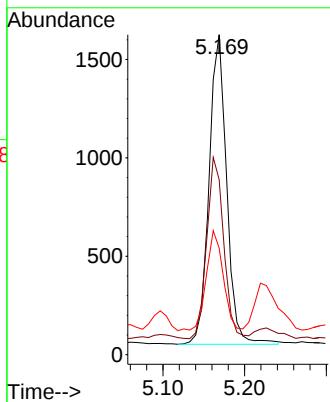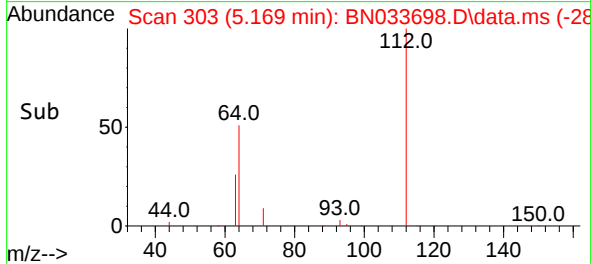

#5
Phenol-d6
Concen: 0.093 ng
RT: 6.722 min Scan# 518
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42


Tgt Ion: 99 Resp: 1844
Ion Ratio Lower Upper
99 100
42 20.3 17.8 26.8
71 42.5 28.0 42.0#

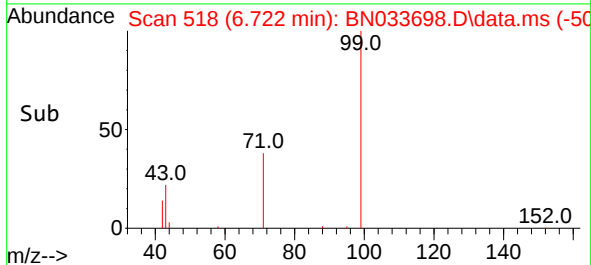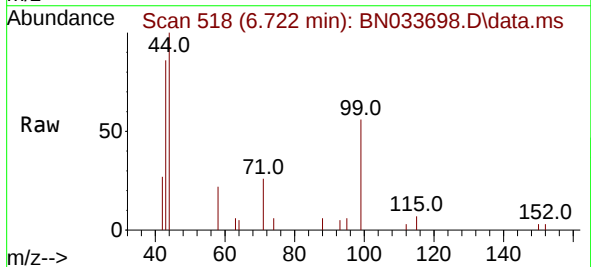

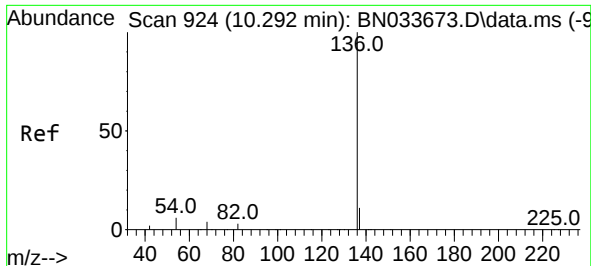

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.282 min Scan# 91
Delta R.T. -0.010 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724

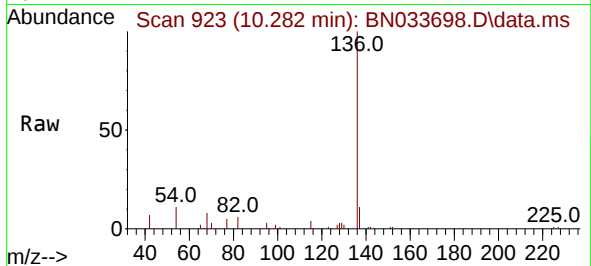

Tgt Ion:136 Resp: 1452
Ion Ratio Lower Upper
136 100
137 11.5 9.1 13.7
54 10.7 5.8 8.6
68 8.1 4.2 6.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

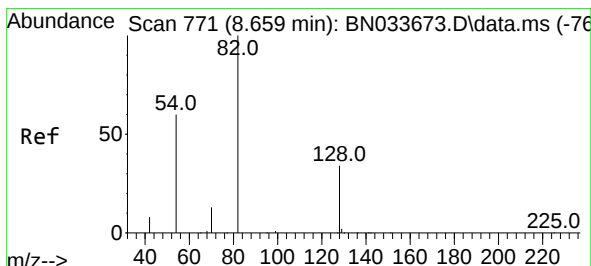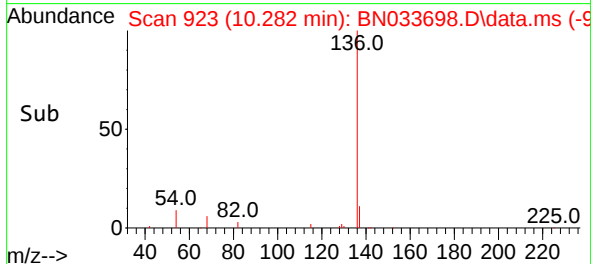

#8
Nitrobenzene-d5
Concen: 0.335 ng
RT: 8.659 min Scan# 771
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42

Tgt Ion: 82 Resp: 4047
Ion Ratio Lower Upper
82 100
128 40.1 29.3 43.9
54 58.0 49.4 74.0

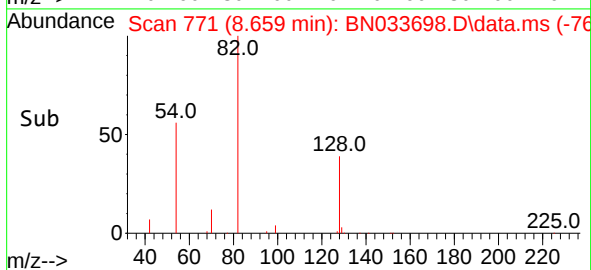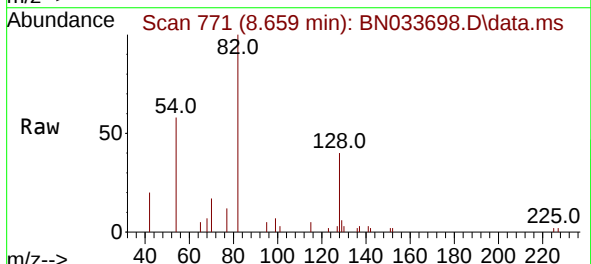

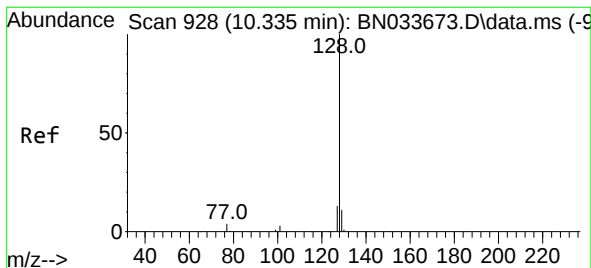

#9

Naphthalene

Concen: 0.040 ng

RT: 10.336 min Scan# 91

Delta R.T. 0.000 min

Lab File: BN033698.D

Acq: 30 Aug 2024 09:42

Instrument :

BN_A_N

ClientSampleId :

OW-02B-21.2-082724





Tgt Ion:	128	Resp:	1569
Ion Ratio	Lower	Upper	
128	100		
129	31.0	9.4	14.0
127	23.6	11.0	16.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 09/02/2024

Supervised By :mohammad ahmed 09/02/2024

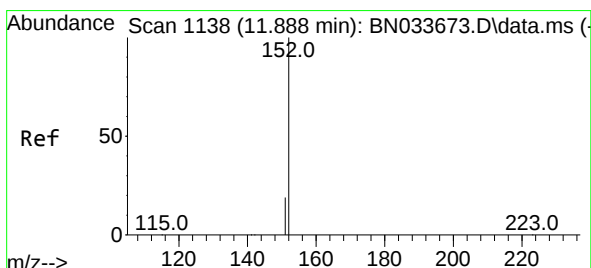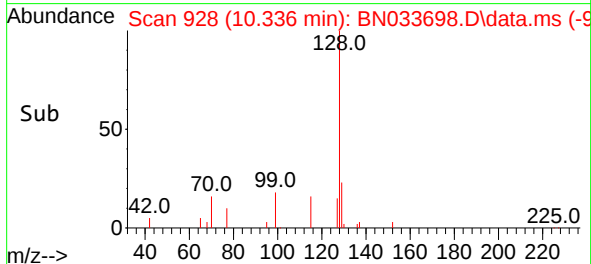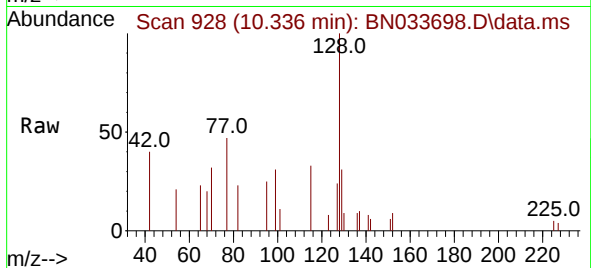

#11

2-Methylnaphthalene-d10

Concen: 0.371 ng




RT: 11.881 min Scan# 1136


Delta R.T. -0.007 min

Lab File: BN033698.D

Acq: 30 Aug 2024 09:42


Tgt Ion:	152	Resp:	7600
Ion Ratio	Lower	Upper	
152	100		
151	21.0	16.7	25.1

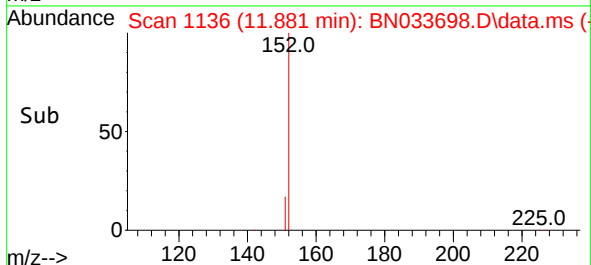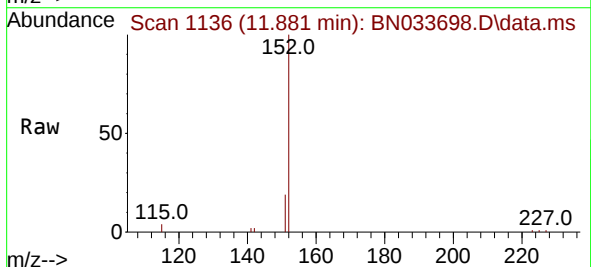

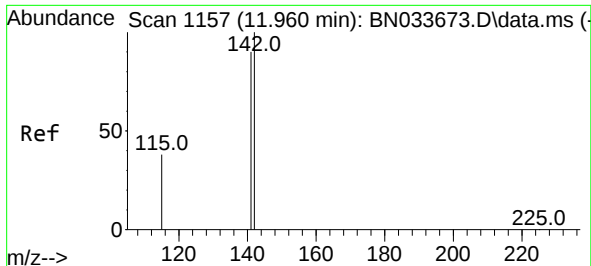

#12
2-Methylnaphthalene
Concen: 0.047 ng
RT: 11.956 min Scan# 1156
Delta R.T. -0.003 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724

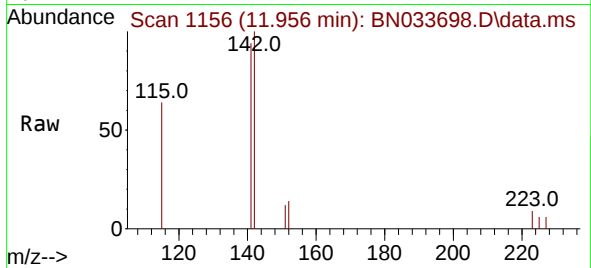


Tgt Ion:142 Resp: 1110
Ion Ratio Lower Upper
142 100
141 94.3 71.8 107.8
115 64.4 31.4 47.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

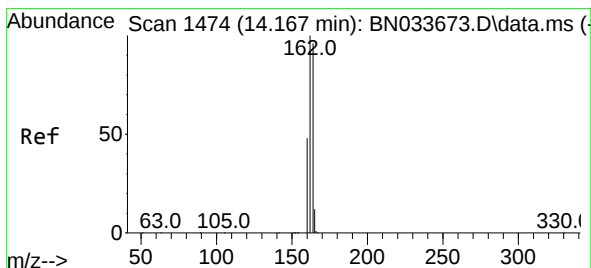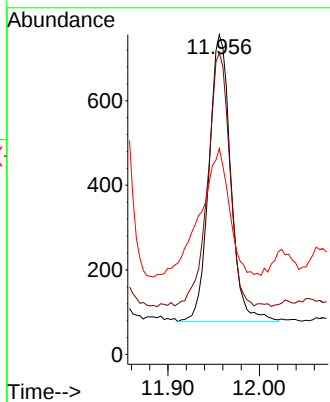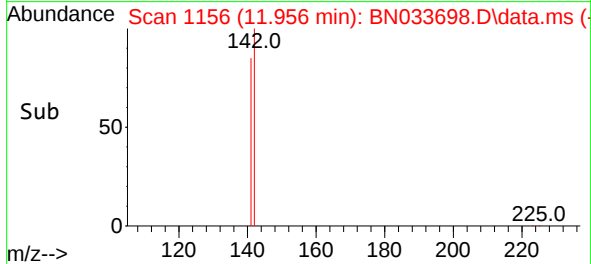


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.157 min Scan# 1473
Delta R.T. -0.010 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42

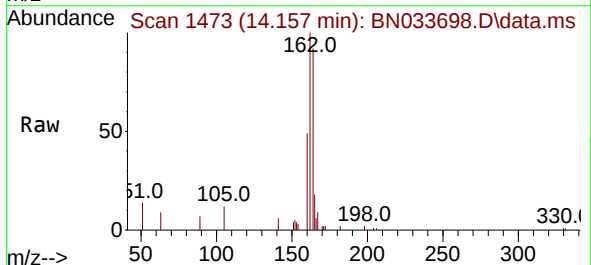


Tgt Ion:164 Resp: 7492
Ion Ratio Lower Upper
164 100
162 108.5 83.4 125.2
160 53.7 40.2 60.2

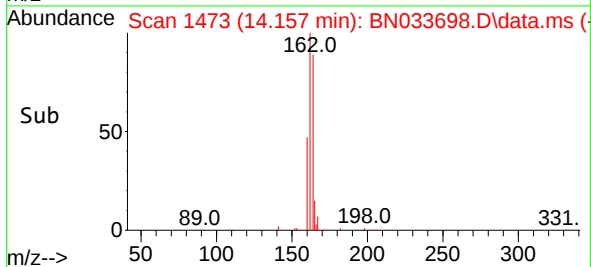

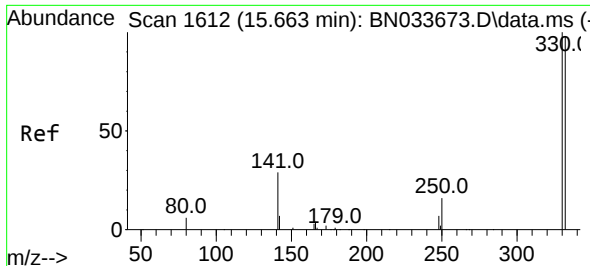

#14
2,4,6-Tribromophenol
Concen: 0.405 ng
RT: 15.663 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724




Tgt Ion:330 Resp: 1454
Ion Ratio Lower Upper
330 100
332 95.0 78.6 118.0
141 66.3 35.0 52.6

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

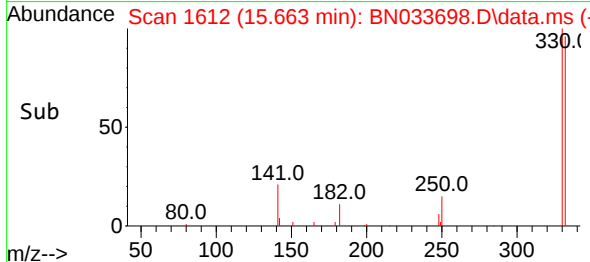


#15
2-Fluorobiphenyl
Concen: 0.350 ng
RT: 12.777 min Scan# 1344
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42

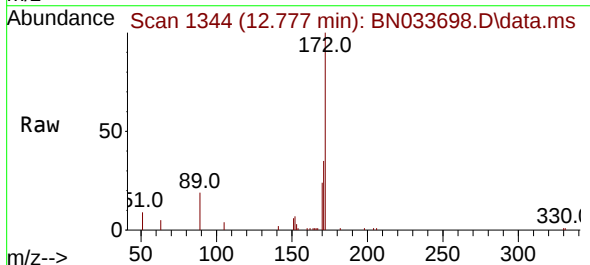


Tgt Ion:172 Resp: 11041
Ion Ratio Lower Upper
172 100
171 35.4 29.2 43.8
170 24.2 19.7 29.5

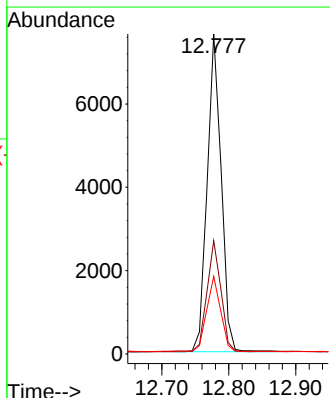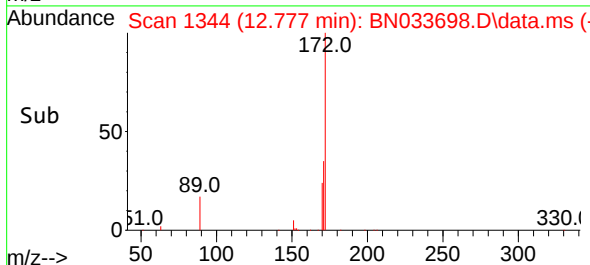

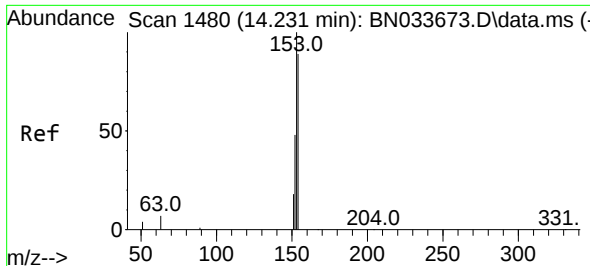

#17
Acenaphthene
Concen: 0.075 ng
RT: 14.221 min Scan# 1479
Delta R.T. -0.010 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724



Tgt Ion:154 Resp: 170
Ion Ratio Lower Upper
154 100
153 114.5 91.8 137.8
152 58.6 45.4 68.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

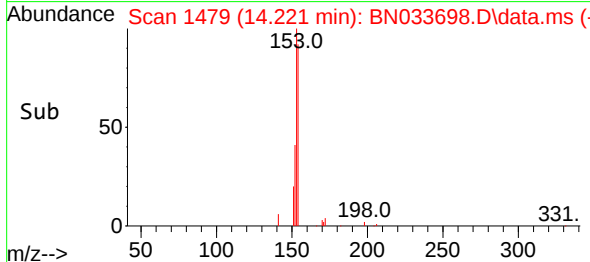

#18
Fluorene
Concen: 0.099 ng
RT: 15.215 min Scan# 1572
Delta R.T. -0.010 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42


Tgt Ion:166 Resp: 2763
Ion Ratio Lower Upper
166 100
165 32.0 78.6 118.0#
167 19.1 10.7 16.1#

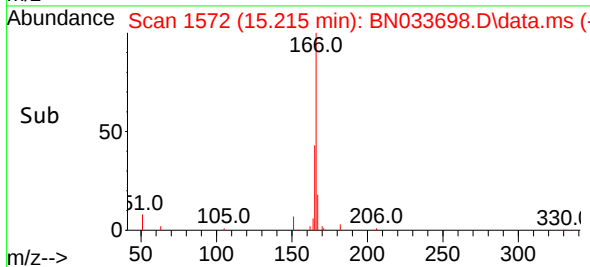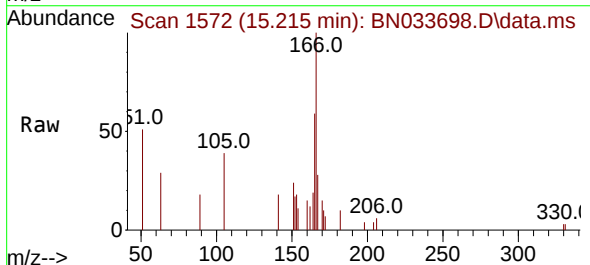

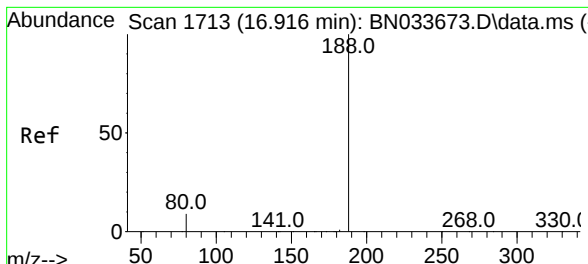

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.917 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724

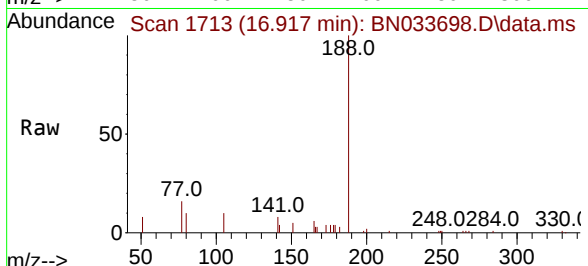


Tgt Ion:188 Resp: 14418
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.4 7.4 11.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

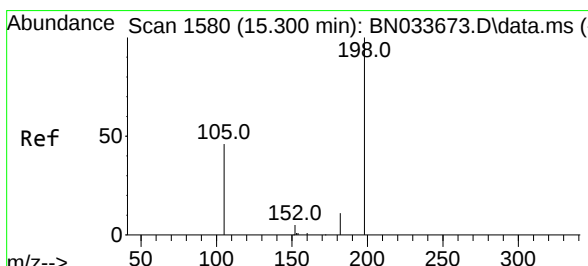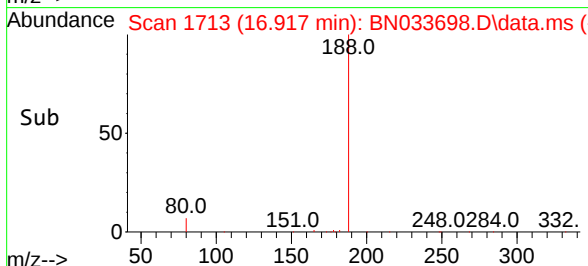


#20
4,6-Dinitro-2-methylphenol
Concen: 0.243 ng
RT: 15.290 min Scan# 1579
Delta R.T. -0.010 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42

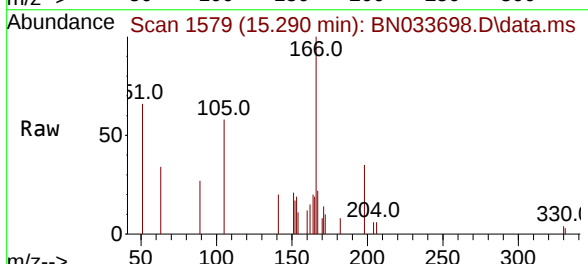


Tgt Ion:198 Resp: 531
Ion Ratio Lower Upper
198 100
51 190.8 82.9 124.3#
105 168.4 53.4 80.0#

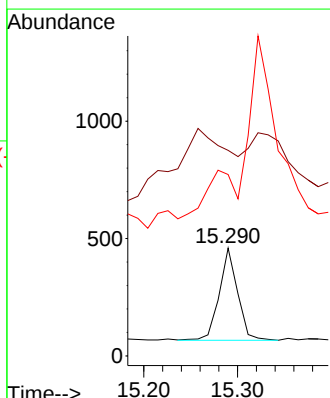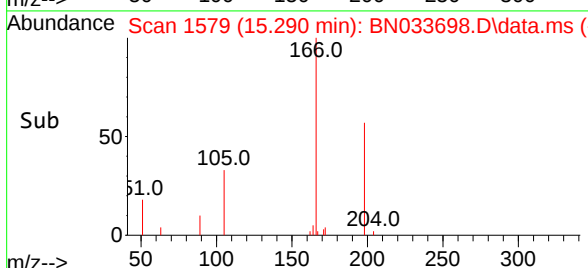

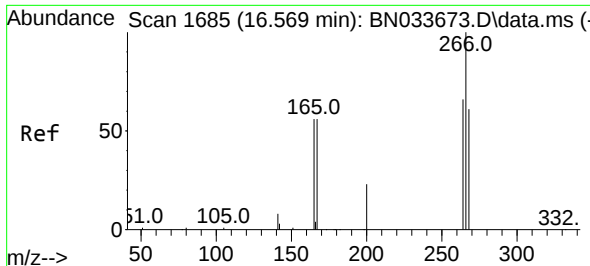

#24
Pentachlorophenol
Concen: 0.036 ng
RT: 16.569 min Scan# 1685
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724



Tgt Ion:266 Resp: 154
Ion Ratio Lower Upper
266 100
264 44.8 51.4 77.2#
268 52.6 51.9 77.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

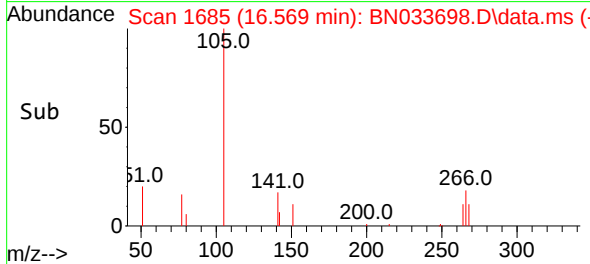

#25
Phenanthrene
Concen: 0.077 ng
RT: 16.954 min Scan# 1716
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42


Tgt Ion:178 Resp: 3099
Ion Ratio Lower Upper
178 100
176 25.8 15.4 23.2#
179 23.6 12.2 18.2#

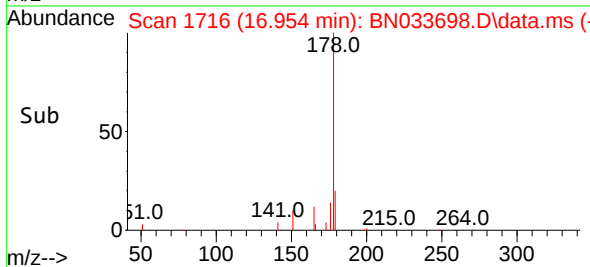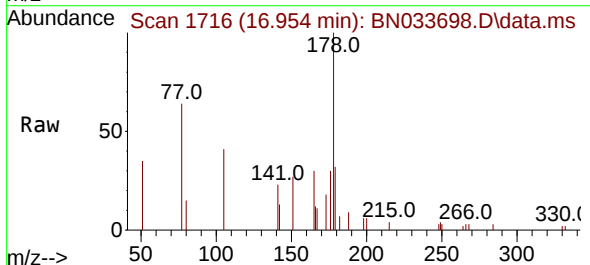



#26
 Anthracene
 Concen: 0.037 ng
 RT: 17.041 min Scan# 1724
 Delta R.T. -0.012 min
 Lab File: BN033698.D
 Acq: 30 Aug 2024 09:42




Instrument :
 BNA_N
 ClientSampleId :
 OW-02B-21.2-082724



Tgt Ion:178 Resp: 1302
 Ion Ratio Lower Upper
 178 100
 176 54.9 14.9 22.3
 179 40.6 12.2 18.4




Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 09/02/2024
 Supervised By :mohammad ahmed 09/02/2024

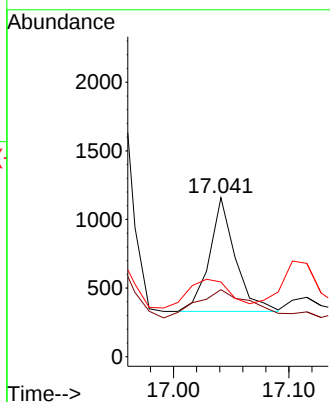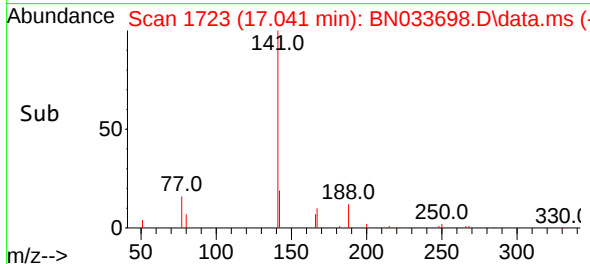

#27
 Fluoranthene-d10
 Concen: 0.448 ng
 RT: 18.956 min Scan# 1938
 Delta R.T. 0.000 min
 Lab File: BN033698.D
 Acq: 30 Aug 2024 09:42


Tgt Ion:212 Resp: 15922
 Ion Ratio Lower Upper
 212 100
 106 15.0 11.8 17.6
 104 8.8 6.9 10.3

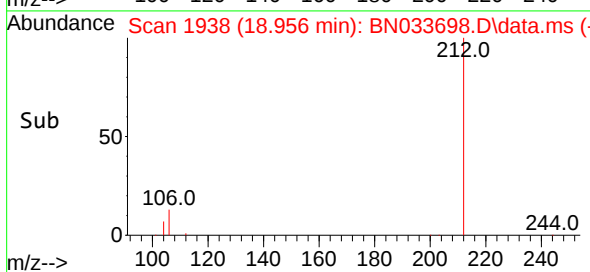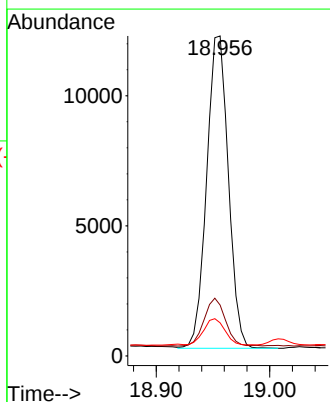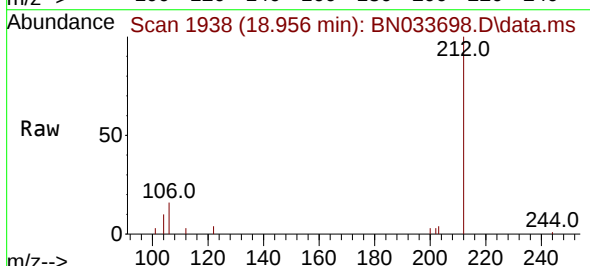



#29
Chrysene-d12
Concen: 0.400 ng m
RT: 21.121 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724

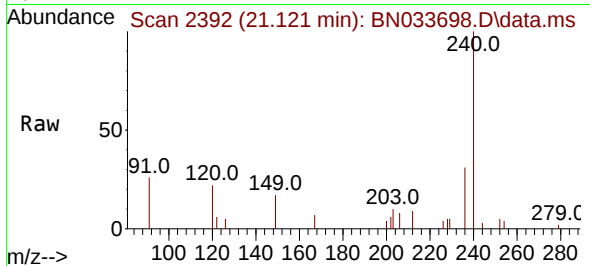


Tgt Ion:240 Resp: 1250
Ion Ratio Lower Upper
240 100
120 21.5 13.3 19.9
236 31.3 23.4 35.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

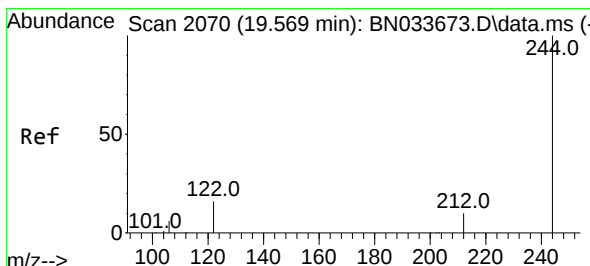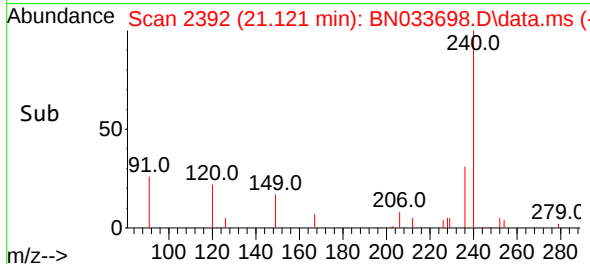


#31
Terphenyl-d14
Concen: 0.451 ng
RT: 19.569 min Scan# 2070
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42

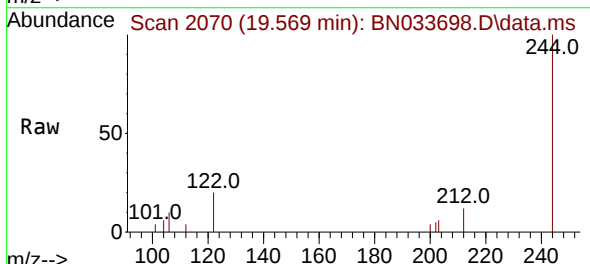


Tgt Ion:244 Resp: 11937
Ion Ratio Lower Upper
244 100
212 11.9 8.2 12.4
122 20.3 13.6 20.4

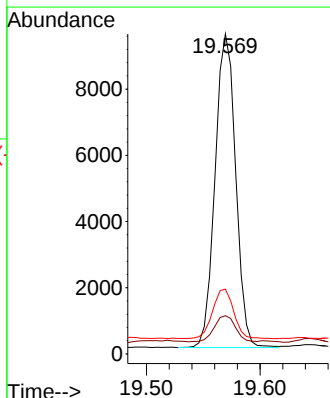

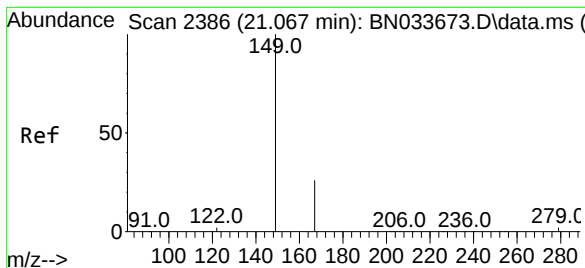

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.277 ng m
RT: 21.068 min Scan# 2106
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42




Instrument :
BNA_N
ClientSampleId :
OW-02B-21.2-082724

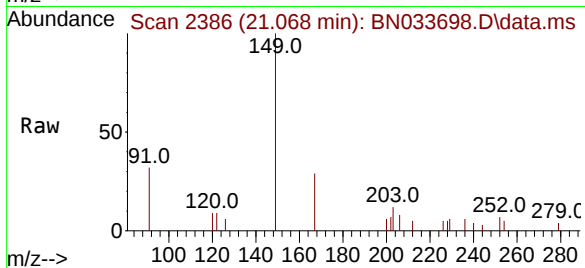

Tgt Ion:149 Resp: 692
Ion Ratio Lower Upper
149 100
167 43.0 28.3 42.5
279 25.8 4.2 6.2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/02/2024

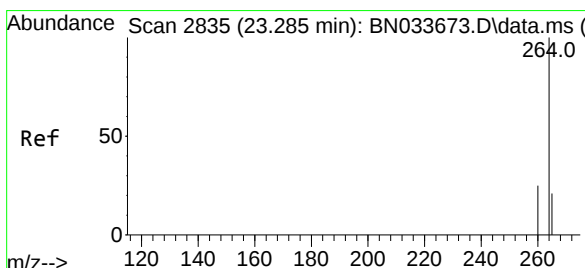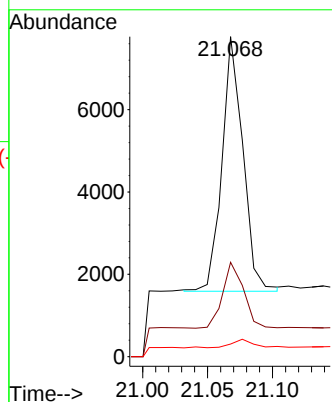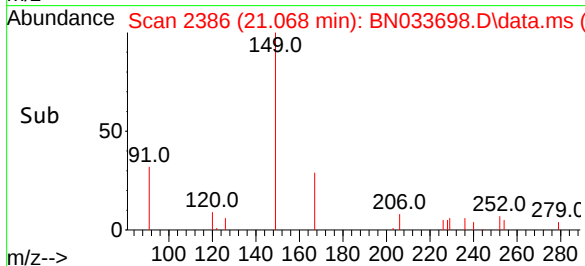

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.285 min Scan# 2835
Delta R.T. 0.000 min
Lab File: BN033698.D
Acq: 30 Aug 2024 09:42

Tgt Ion:264 Resp: 13654
Ion Ratio Lower Upper
264 100
260 26.8 20.7 31.1
265 81.6 69.9 104.9

