


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033669.D
Acq On : 29 Aug 2024 14:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 29 23:33:13 2024

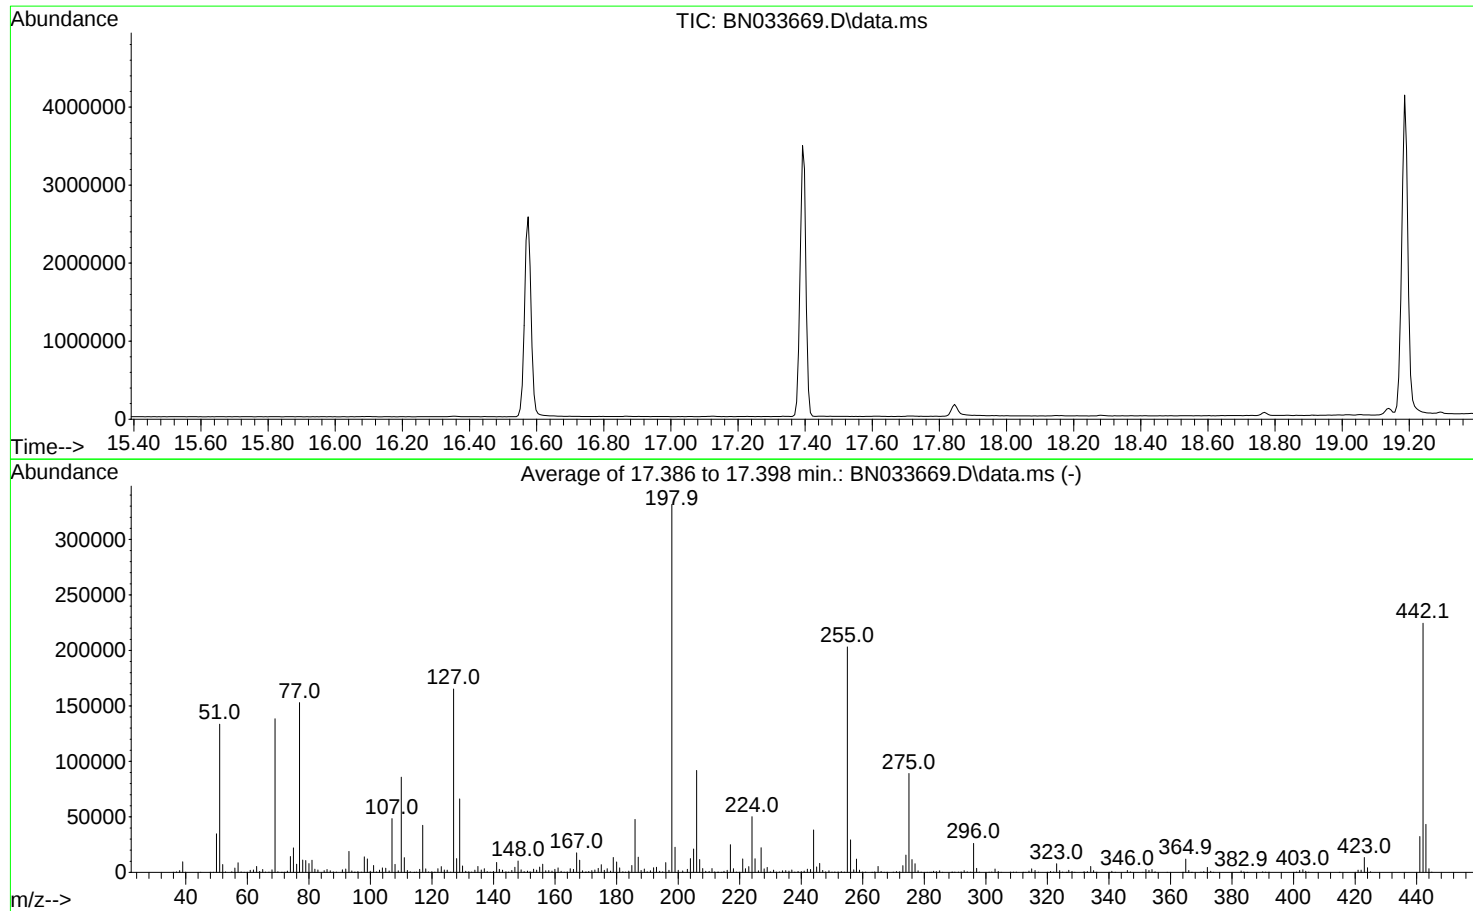

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	133486	PASS
68	69	0.00	2	1.6	2269	PASS
69	198	0.00	100	41.8	138444	PASS
70	69	0.00	2	0.4	539	PASS
127	198	10	80	49.8	165227	PASS
197	198	0.00	2	0.6	1877	PASS
198	198	100	100	100.0	331499	PASS
199	198	5	9	6.8	22611	PASS
275	198	10	60	26.9	89093	PASS
365	198	1	100	3.6	12023	PASS
441	198	0.01	100	9.8	32360	PASS
442	442	50	100	100.0	224557	PASS
443	442	15	24	19.2	43227	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/29/2024	BNA_N	<u>BN033669.D</u>
Compound Name	Response	Retention Time
DDT	1065612	20.439
DDD	23502	19.992
DDE	1079	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24581	1090193	2.25

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033669.D
Acq On : 29 Aug 2024 14:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 30 05:53:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 05:53:24 2024
Response via : Initial Calibration

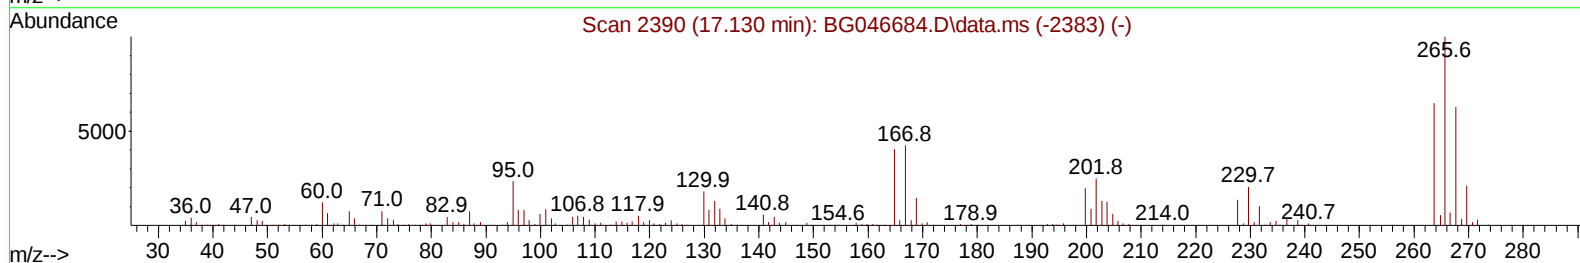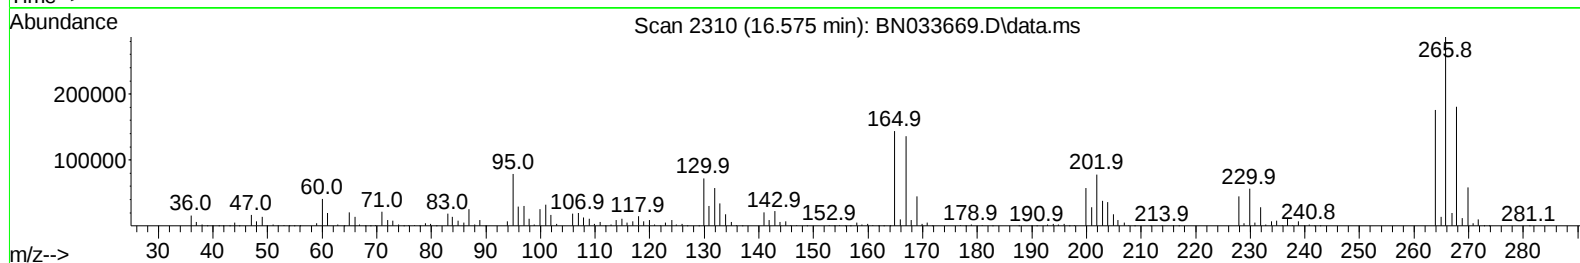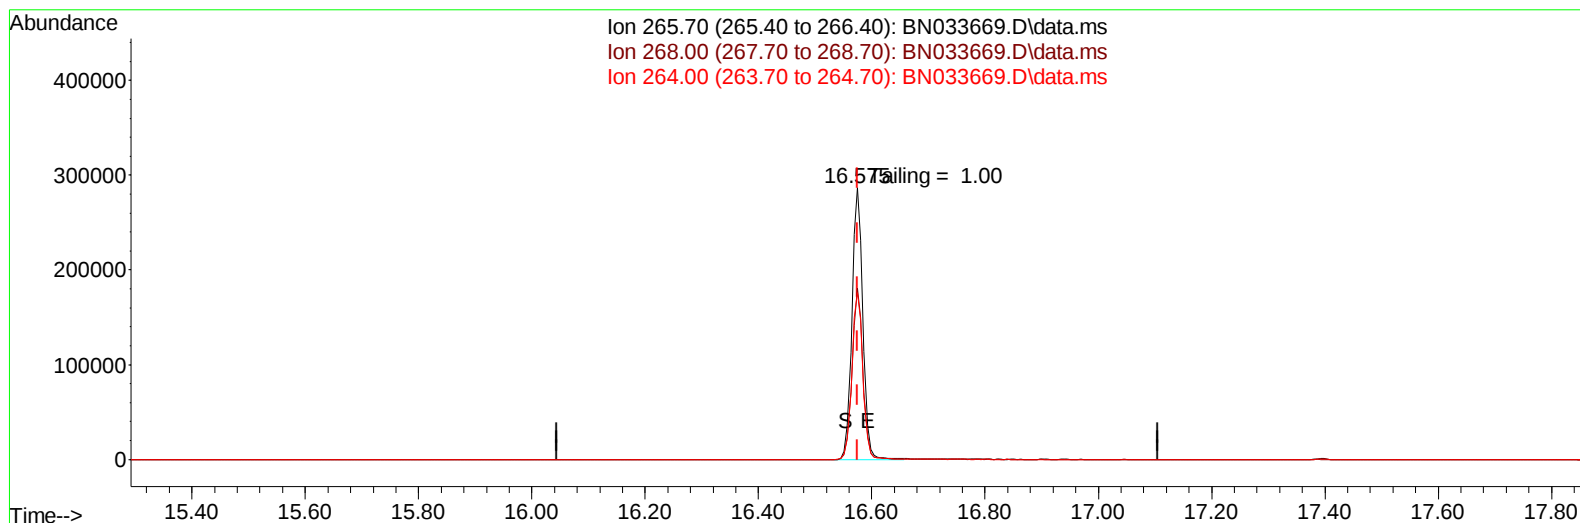

TIC: BN033669.D\data.ms

(70) Pentachlorophenol (C)

16.575min (0.000) 20678.77 ng




response 387042

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.08
264.00	61.60	61.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033669.D
Acq On : 29 Aug 2024 14:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 30 05:53:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 05:53:24 2024
Response via : Initial Calibration

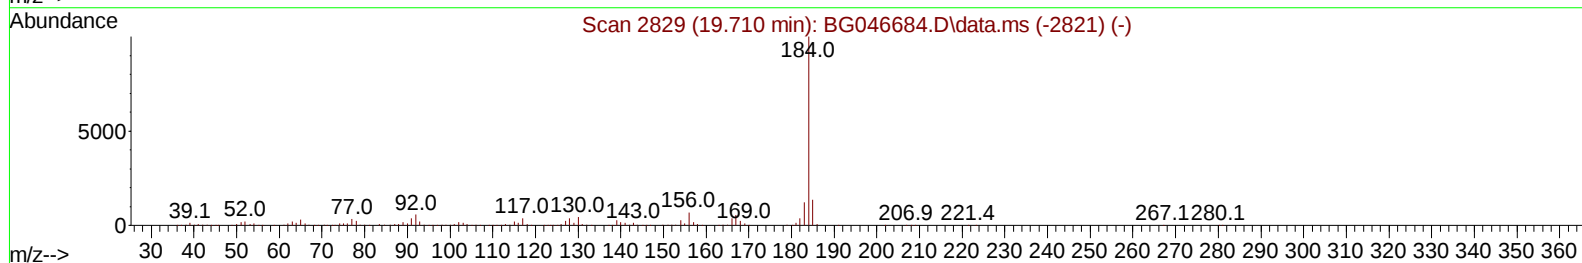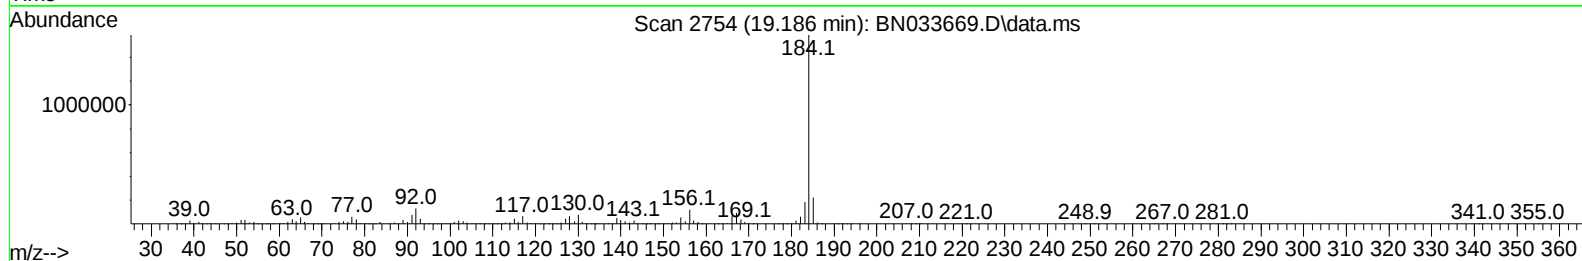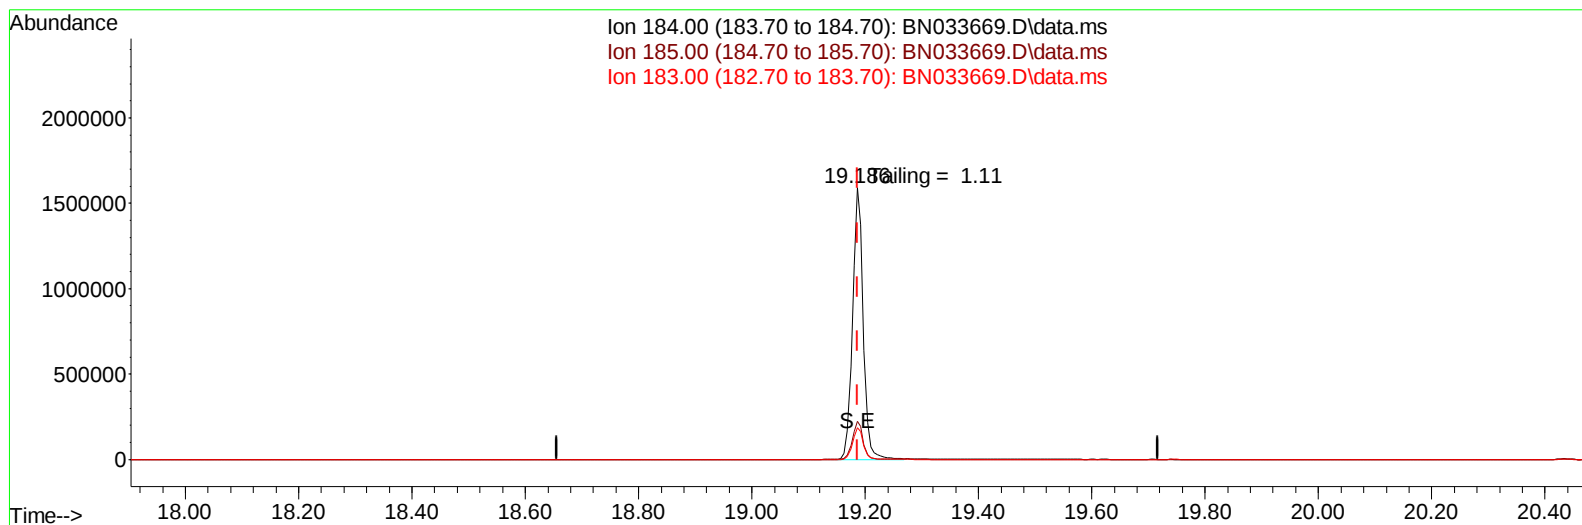

TIC: BN033669.D\data.ms

(77) Benzidine

19.186min (0.000) 0.00 ng

response 2101876

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	11.65
0.00	0.00	0.00