
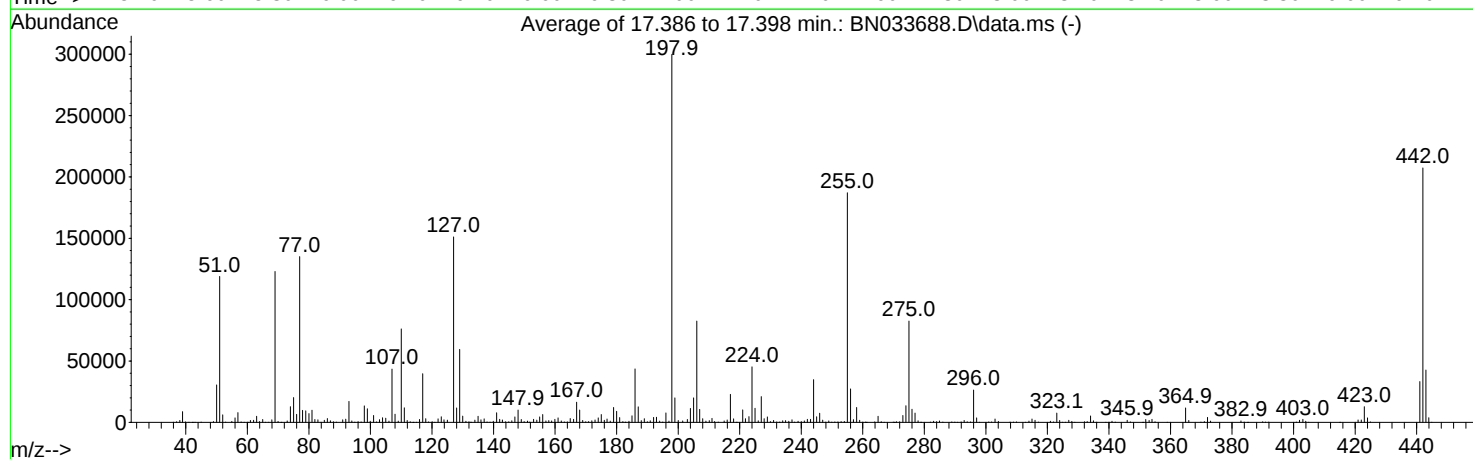


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033688.D
Acq On : 30 Aug 2024 03:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 29 23:33:13 2024

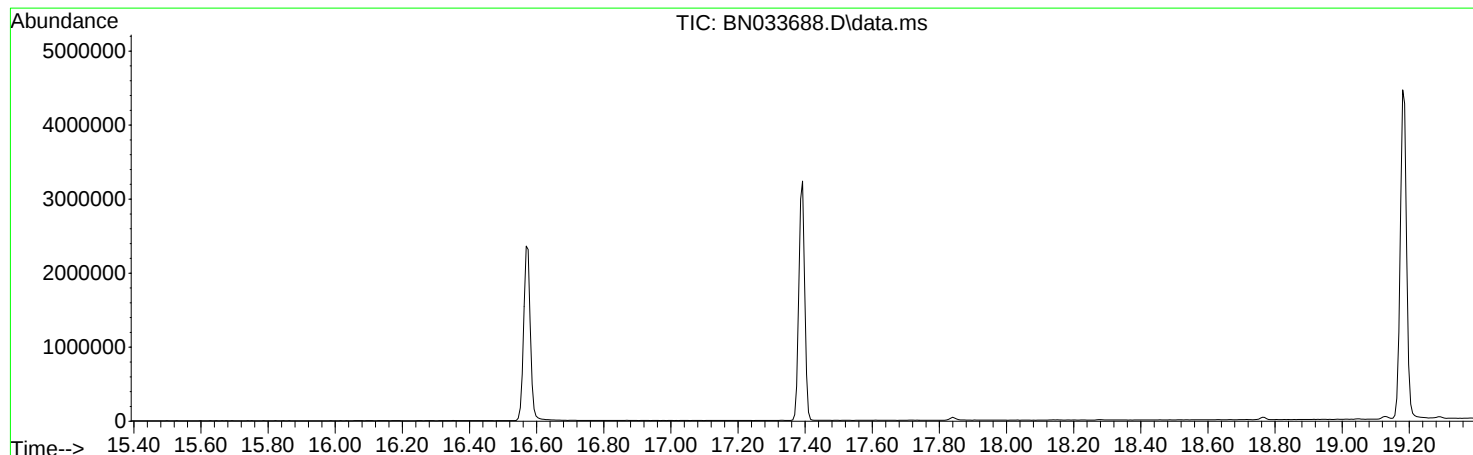




AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	39.7	118920	PASS
68	69	0.00	2	1.7	2147	PASS
69	198	0.00	100	41.0	122912	PASS
70	69	0.00	2	0.6	743	PASS
127	198	10	80	50.4	151149	PASS
197	198	0.00	2	0.3	1020	PASS
198	198	100	100	100.0	299776	PASS
199	198	5	9	6.7	20025	PASS
275	198	10	60	27.6	82603	PASS
365	198	1	100	3.9	11791	PASS
441	198	0.01	100	11.1	33224	PASS
442	442	50	100	100.0	207275	PASS
443	442	15	24	20.6	42691	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033688.D
Acq On : 30 Aug 2024 03:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 30 05:54:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 05:53:24 2024
Response via : Initial Calibration

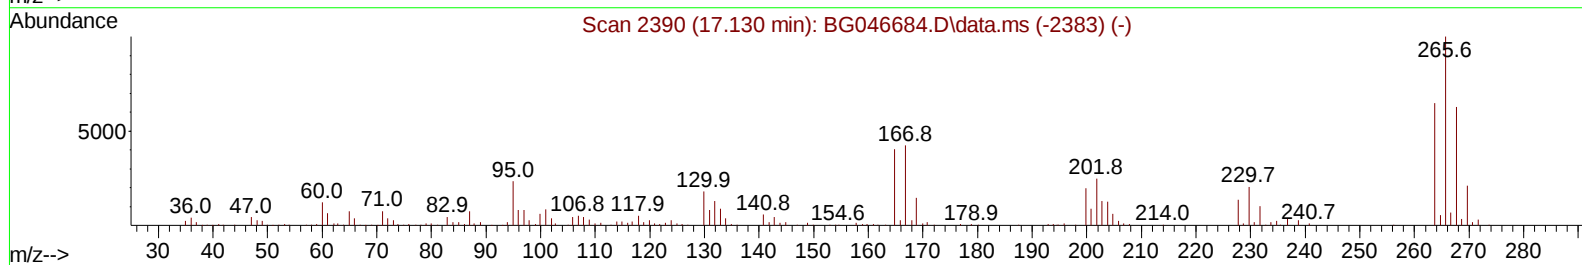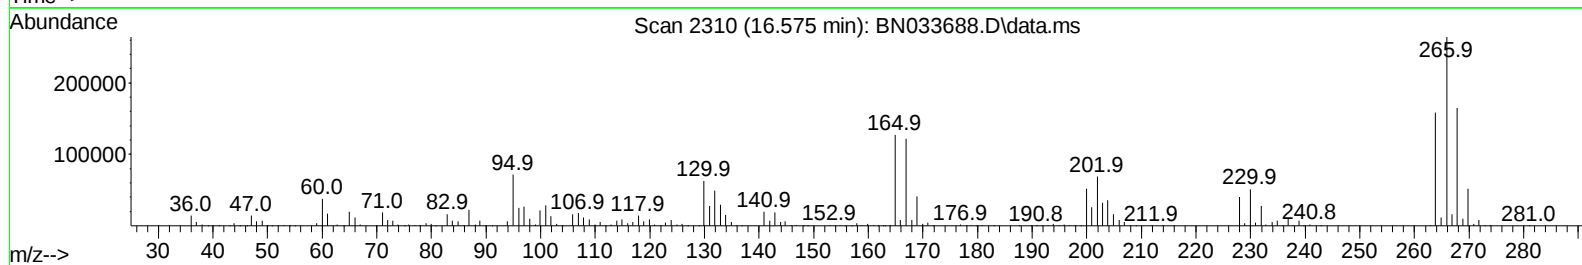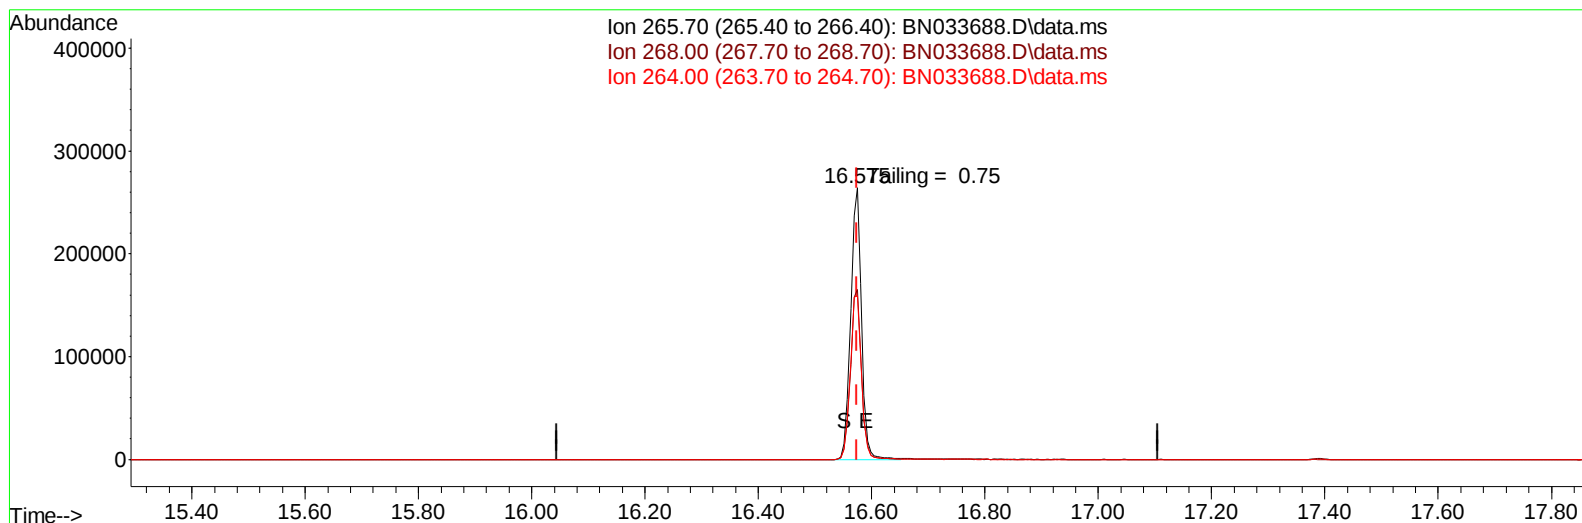

TIC: BN033688.D\data.ms

(70) Pentachlorophenol (C)

16.575min (+ 0.000) 21138.53 ng




response 353843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.55
264.00	61.60	60.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082924\
Data File : BN033688.D
Acq On : 30 Aug 2024 03:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 30 05:54:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 05:53:24 2024
Response via : Initial Calibration

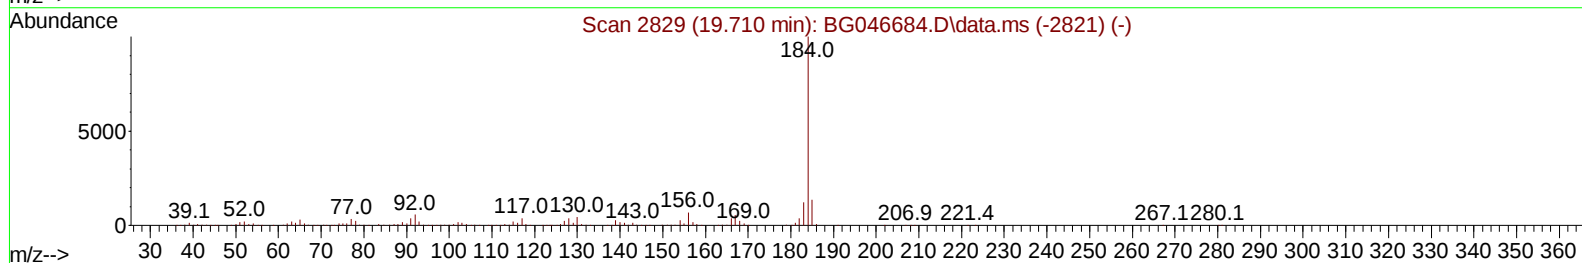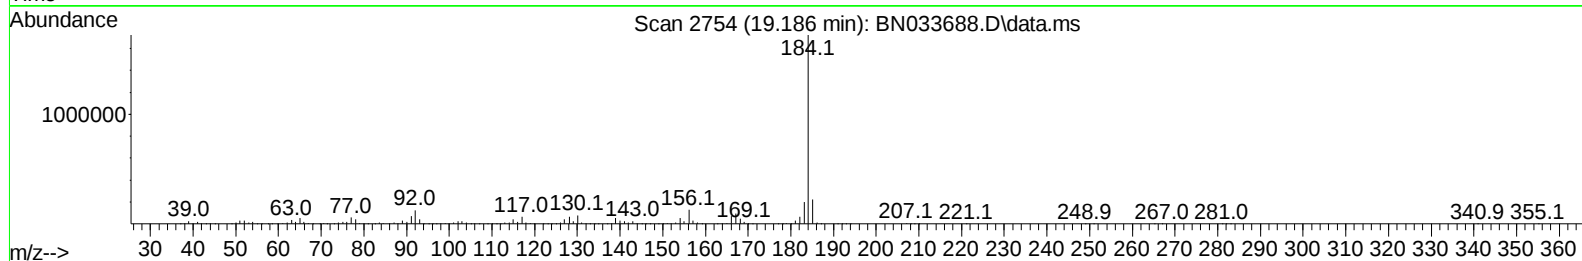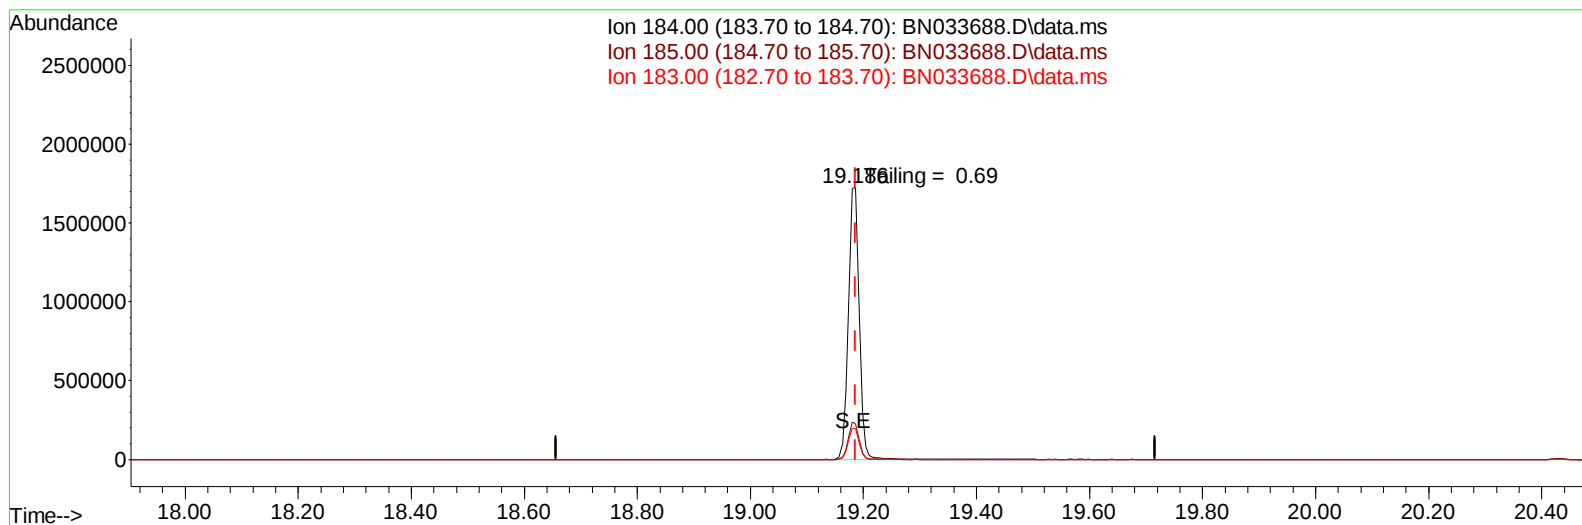

TIC: BN033688.D\data.ms

(77) Benzidine

19.186min (+ 0.000) 0.00 ng

response 2303776

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/29/2024	BNA_N	<u>BN033688.D</u>
Compound Name	Response	Retention Time
DDT	1094989	20.433
DDD	20714	19.986
DDE	720	19.475
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21434	1116423	1.92

Instrument :
BNA_N
ClientSampleId :
DFTPP