
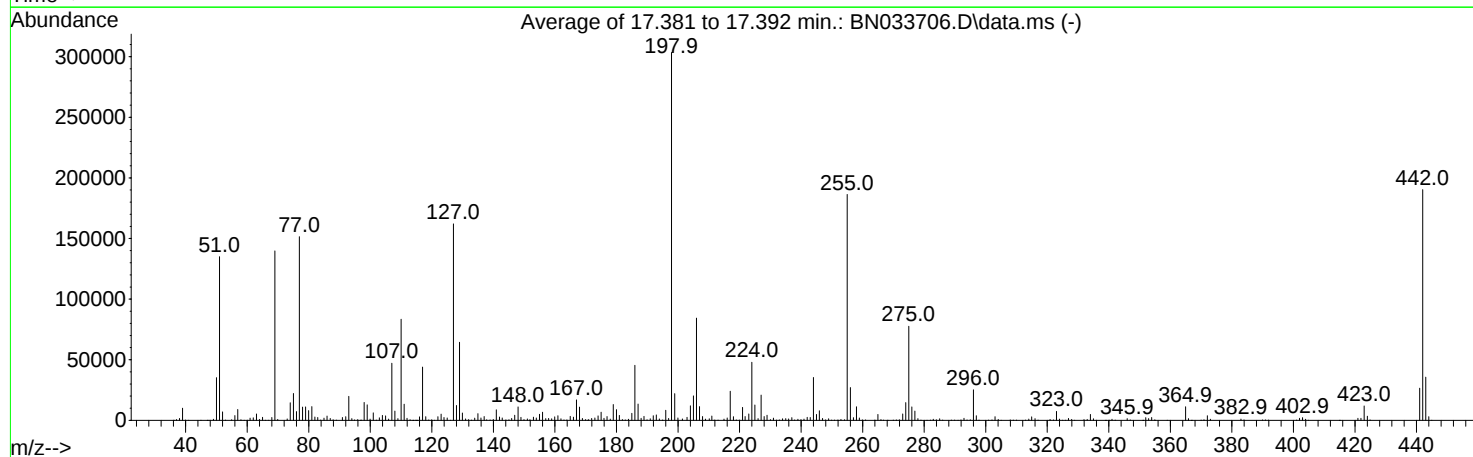


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083024\
Data File : BN033706.D
Acq On : 30 Aug 2024 14:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 29 23:33:13 2024

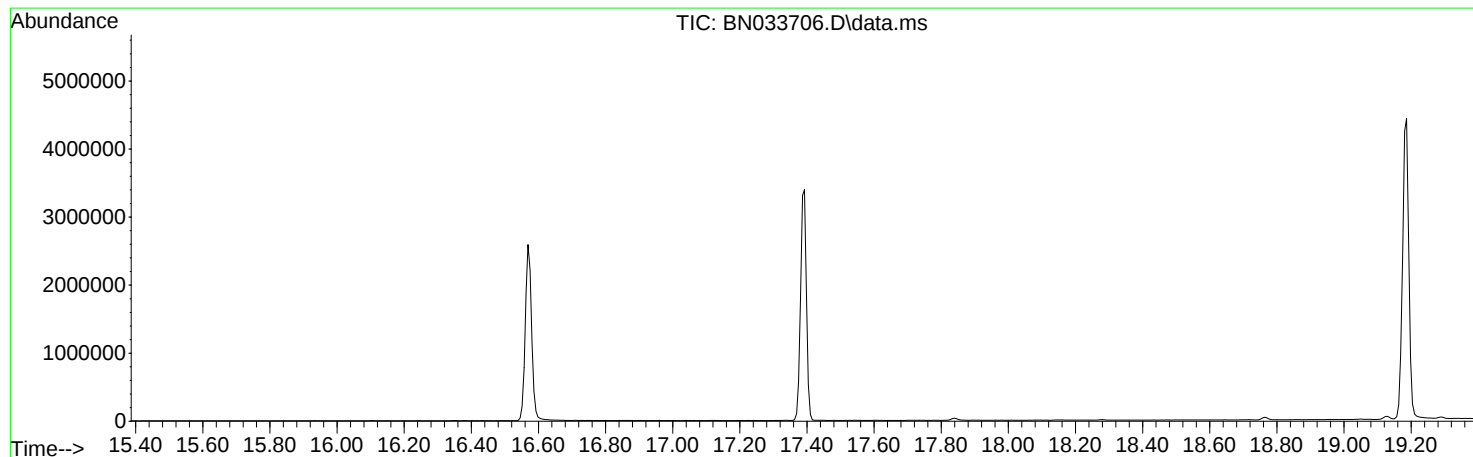

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	135056	PASS
68	69	0.00	2	1.7	2390	PASS
69	198	0.00	100	46.1	139742	PASS
70	69	0.00	2	0.5	761	PASS
127	198	10	80	53.4	162085	PASS
197	198	0.00	2	0.5	1642	PASS
198	198	100	100	100.0	303424	PASS
199	198	5	9	7.3	22101	PASS
275	198	10	60	25.6	77677	PASS
365	198	1	100	3.7	11219	PASS
441	198	0.01	100	8.7	26505	PASS
442	442	50	100	100.0	190269	PASS
443	442	15	24	18.7	35620	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/30/2024	BNA_N	<u>BN033706.D</u>
Compound Name	Response	Retention Time
DDT	1104917	20.433
DDD	45235	19.986
DDE	870	19.481
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
46105	1151022	4.01

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083024\
Data File : BN033706.D
Acq On : 30 Aug 2024 14:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 31 04:51:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:51:24 2024
Response via : Initial Calibration

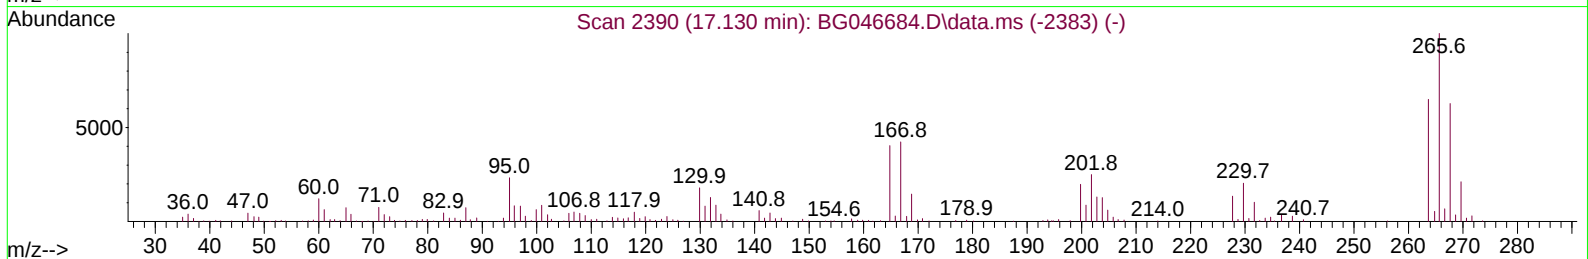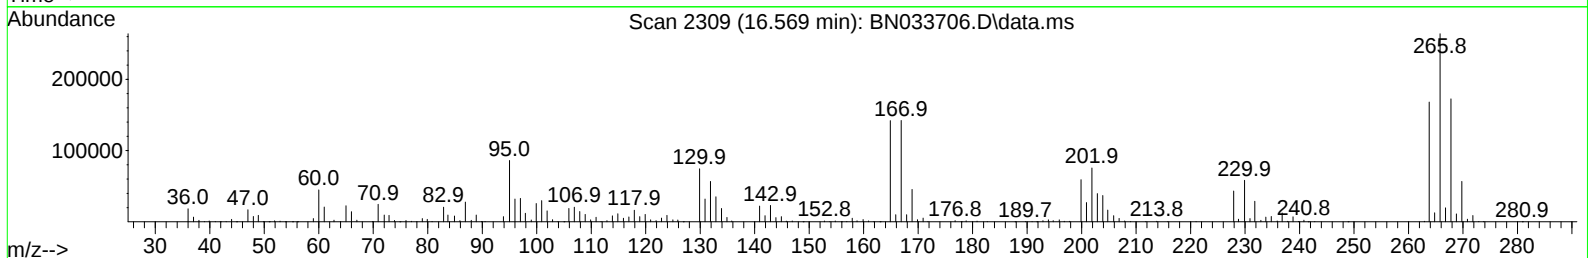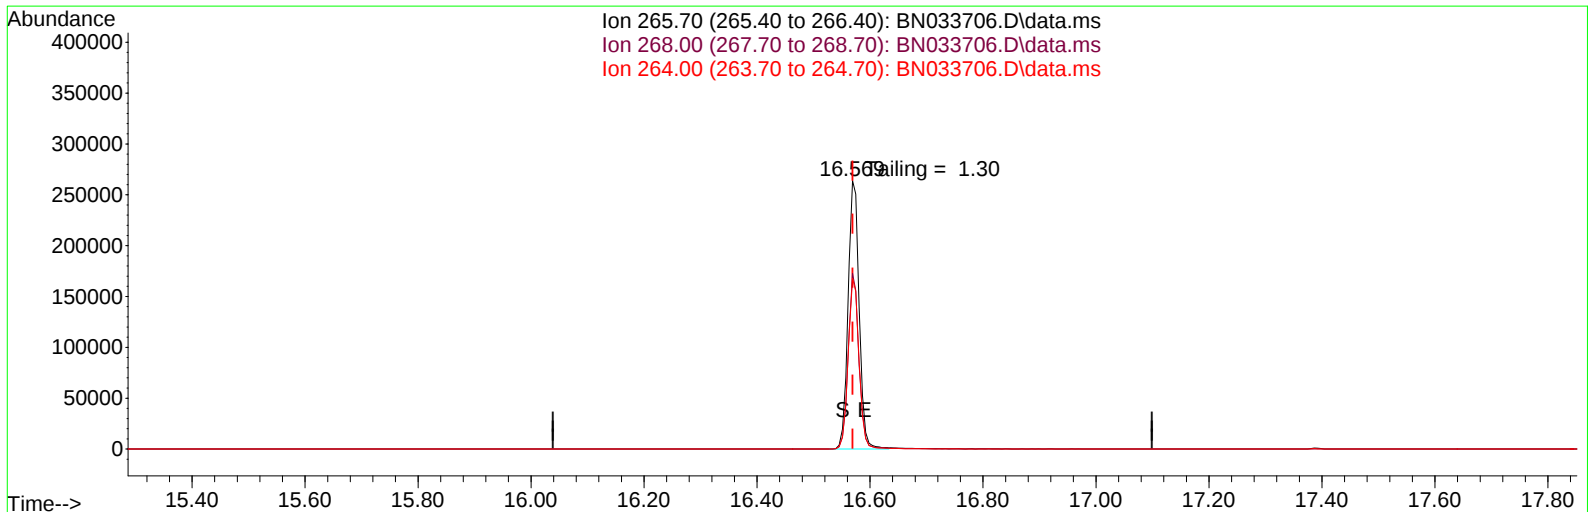

TIC: BN033706.D\data.ms

(70) Pentachlorophenol (C)

16.569min (0.000) 19020.84 ng




response 362728

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.40
264.00	61.60	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083024\
Data File : BN033706.D
Acq On : 30 Aug 2024 14:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 31 04:51:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:51:24 2024
Response via : Initial Calibration

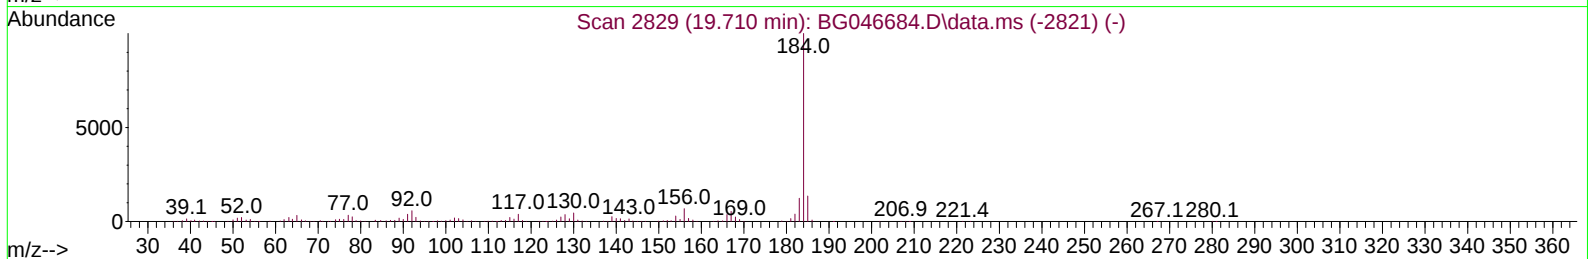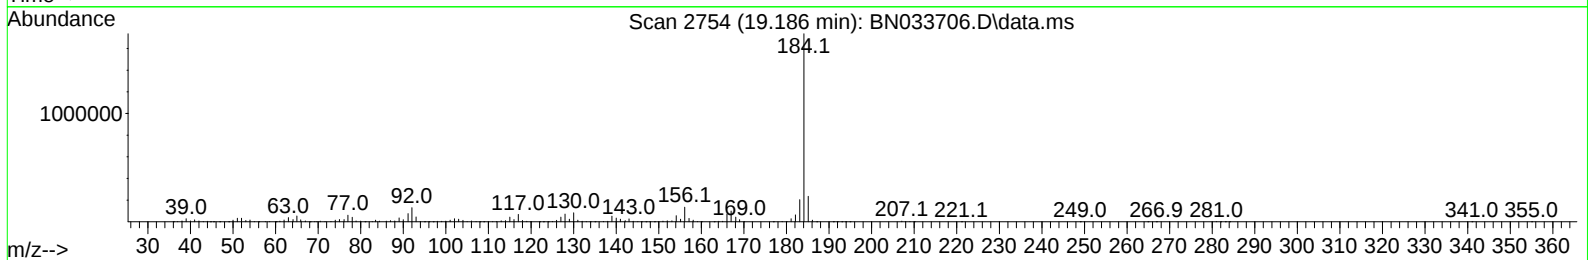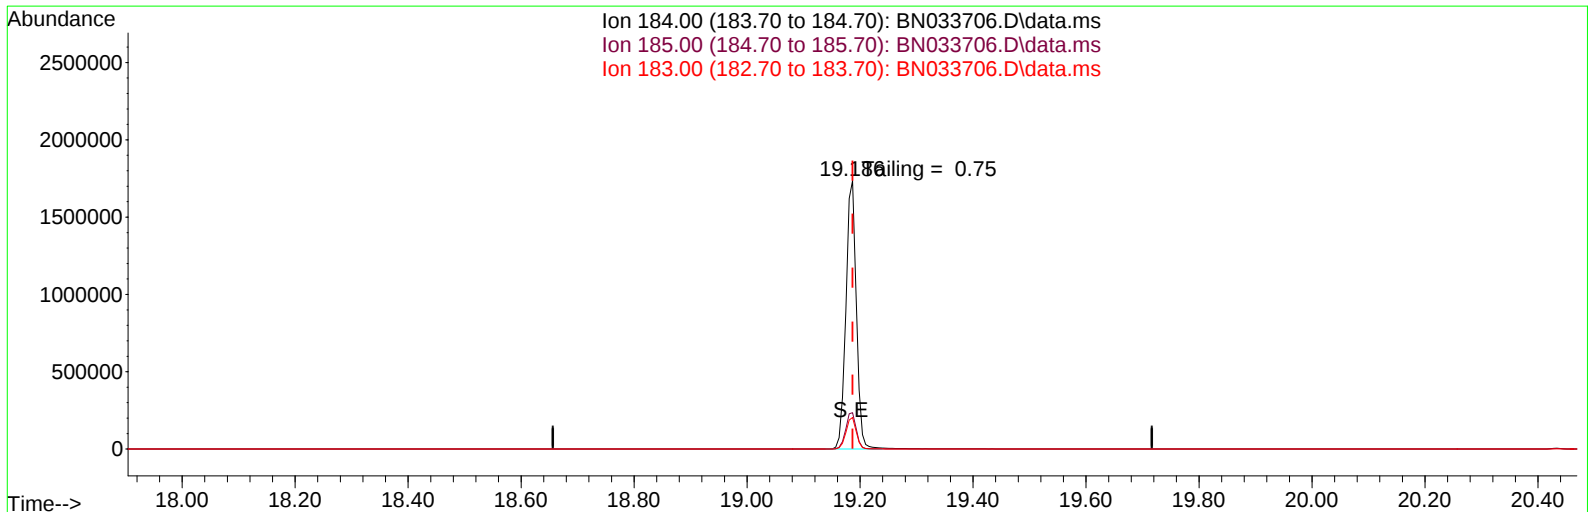

TIC: BN033706.D\data.ms

(77) Benzidine

19.186min (0.000) 0.00 ng

response 2233991

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.56
183.00	13.20	11.79
0.00	0.00	0.00