


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083024\
Data File : BN033719.D
Acq On : 30 Aug 2024 23:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN082924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 29 23:33:13 2024

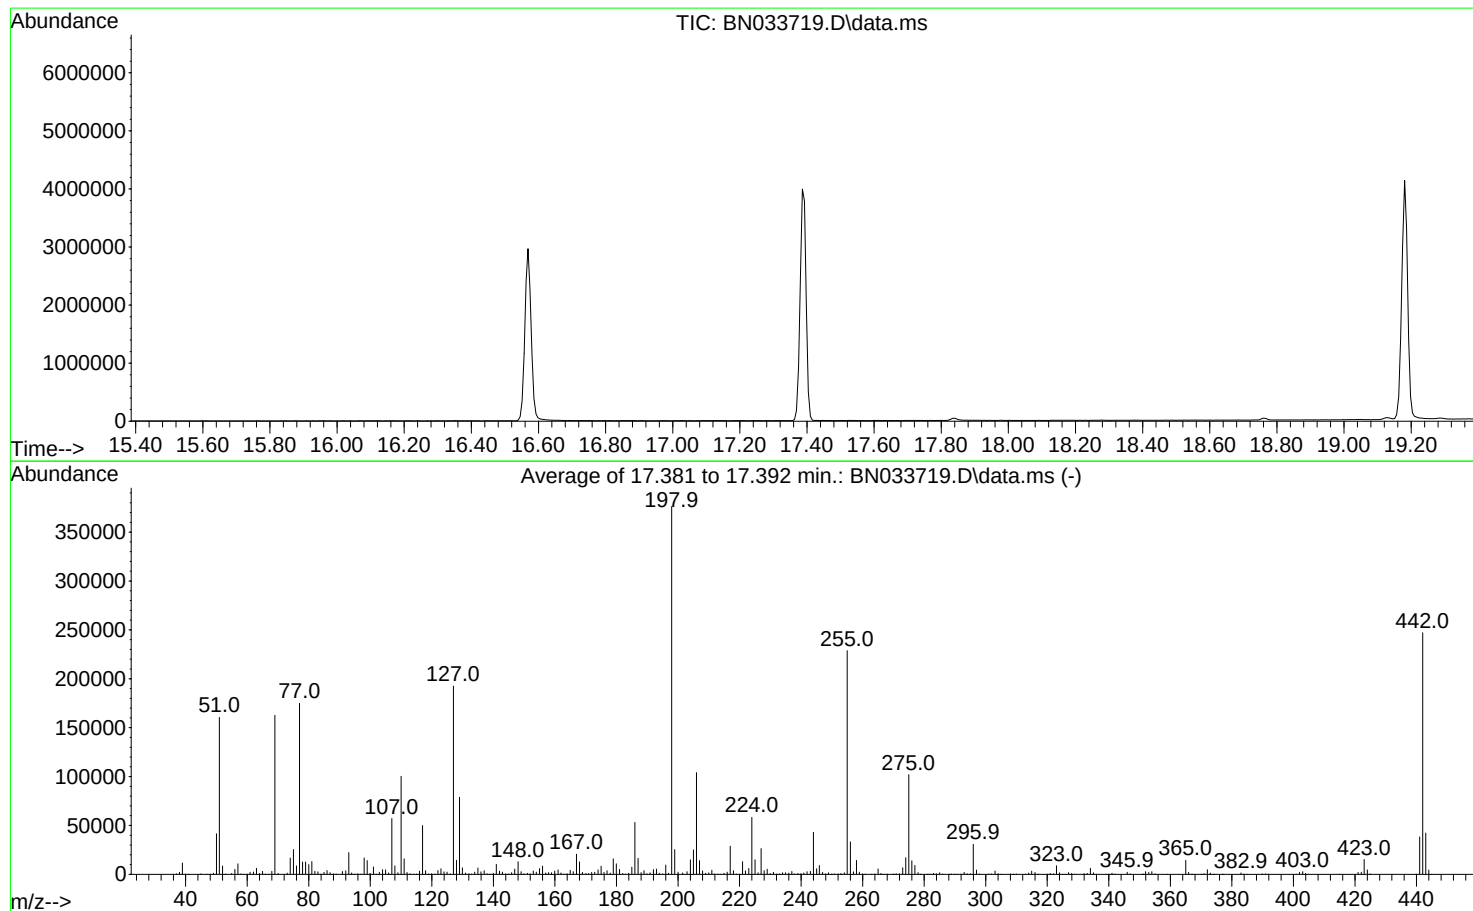

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	160567	PASS
68	69	0.00	2	1.9	3049	PASS
69	198	0.00	100	43.2	162688	PASS
70	69	0.00	2	0.6	922	PASS
127	198	10	80	51.2	192597	PASS
197	198	0.00	2	0.3	1127	PASS
198	198	100	100	100.0	376171	PASS
199	198	5	9	6.8	25421	PASS
275	198	10	60	27.1	101995	PASS
365	198	1	100	3.8	14449	PASS
441	198	0.01	100	10.2	38349	PASS
442	442	50	100	100.0	247091	PASS
443	442	15	24	17.1	42299	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/30/2024	BNA_N	<u>BN033719.D</u>
Compound Name	Response	Retention Time
DDT	1365932	20.427
DDD	21248	19.986
DDE	774	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22022	1387954	1.59

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083024\
Data File : BN033719.D
Acq On : 30 Aug 2024 23:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 31 04:52:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:51:24 2024
Response via : Initial Calibration

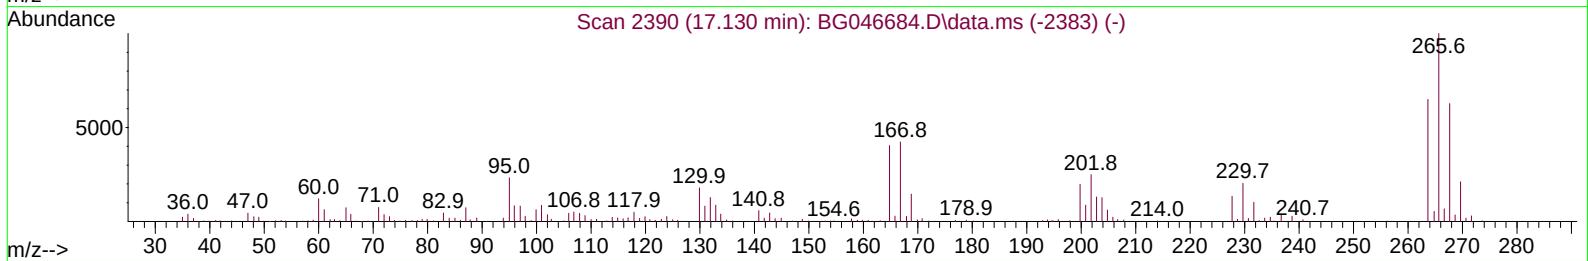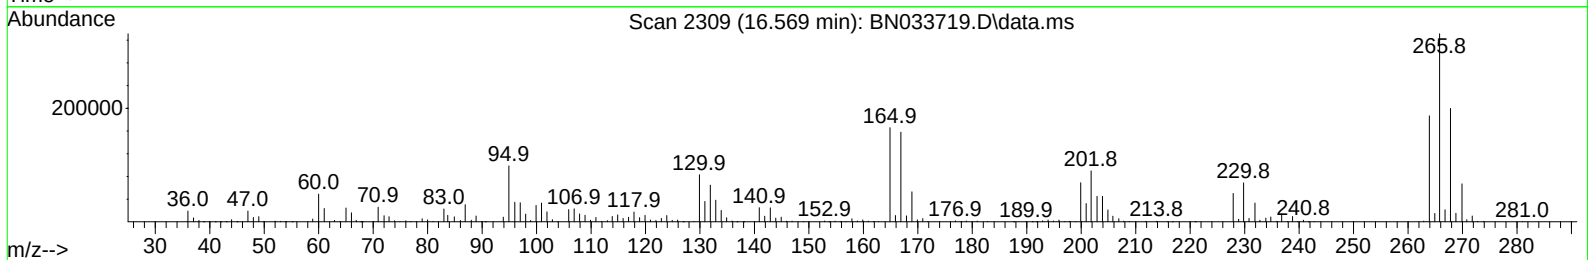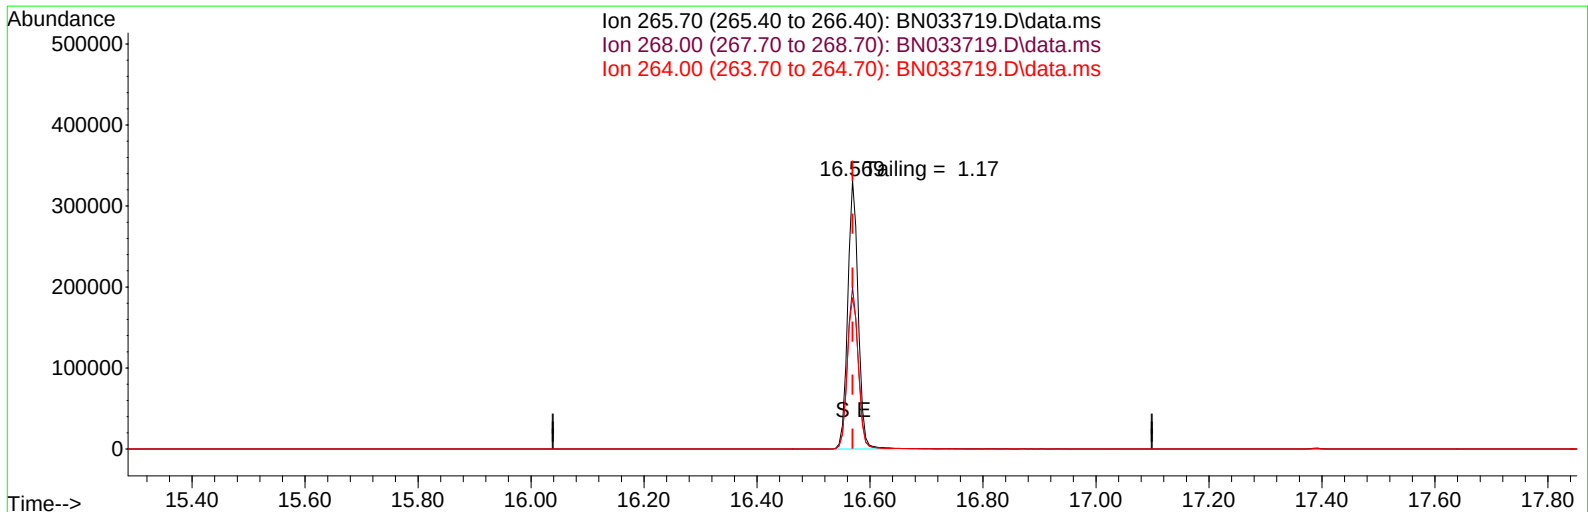

TIC: BN033719.D\data.ms

(70) Pentachlorophenol (C)

16.569min (-0.000) 20619.65 ng




response 428979

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.31
264.00	61.60	56.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083024\
Data File : BN033719.D
Acq On : 30 Aug 2024 23:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 31 04:52:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 31 04:51:24 2024
Response via : Initial Calibration

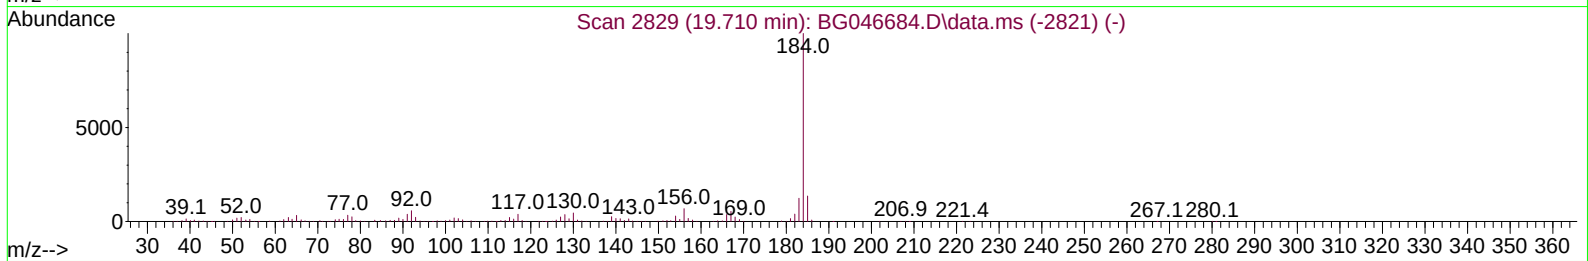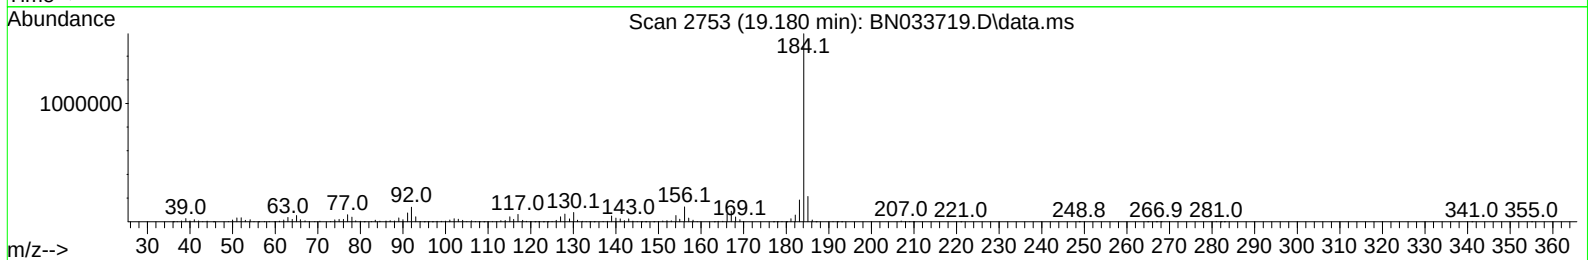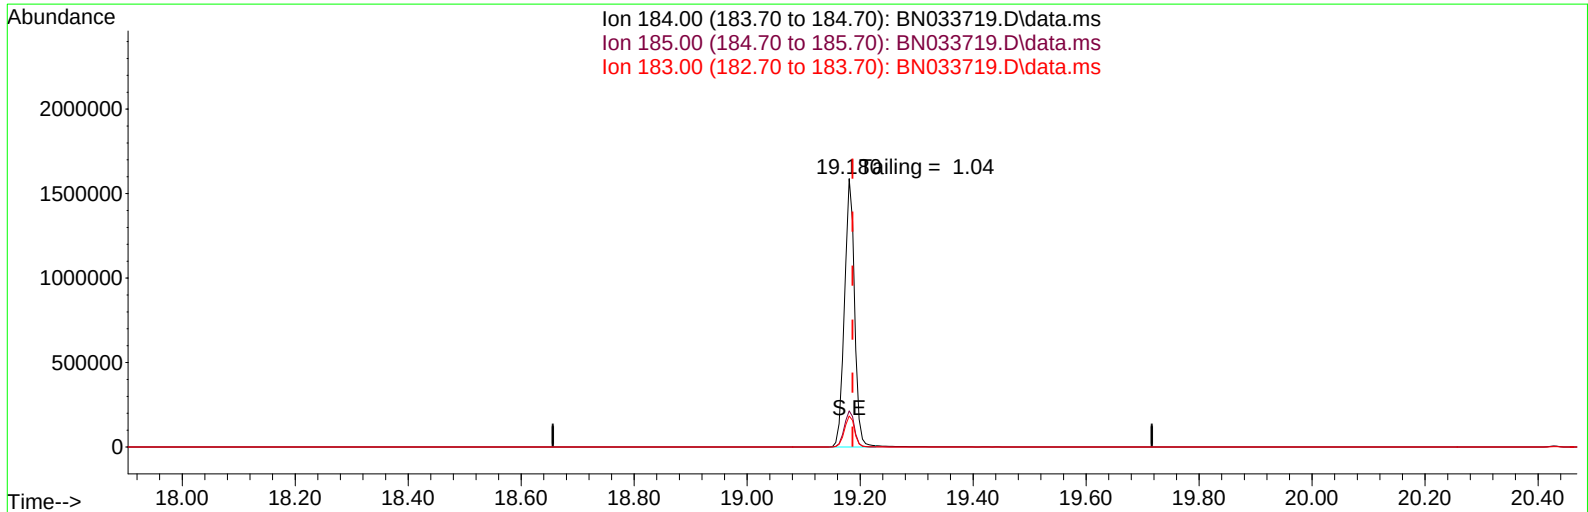

TIC: BN033719.D\data.ms

(77) Benzidine

19.180min (-0.006) 0.00 ng

response 1975039

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.47
183.00	13.20	11.60
0.00	0.00	0.00