
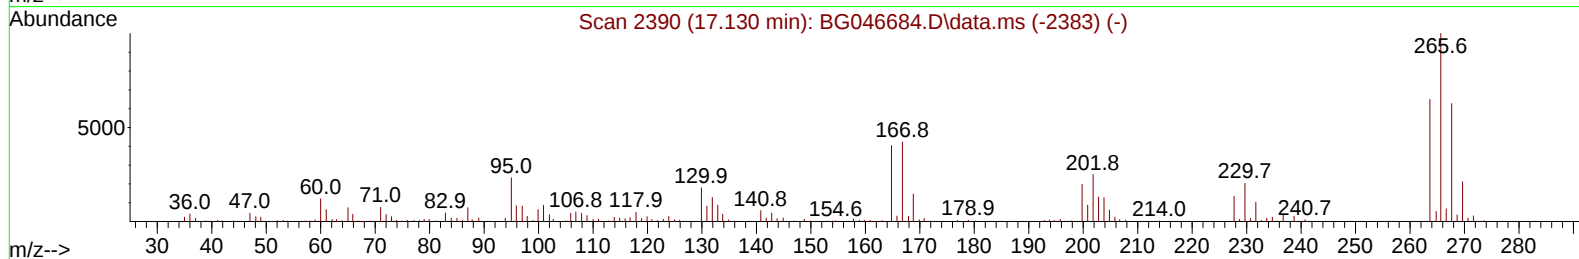
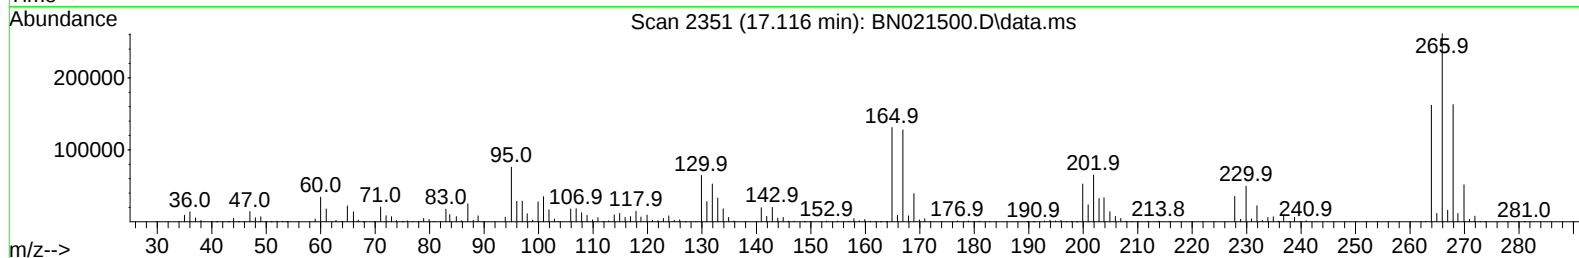


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083122\
 Data File : BN021500.D
 Acq On : 31 Aug 2022 22:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 06:52:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 01 06:50:58 2022
 Response via : Initial Calibration

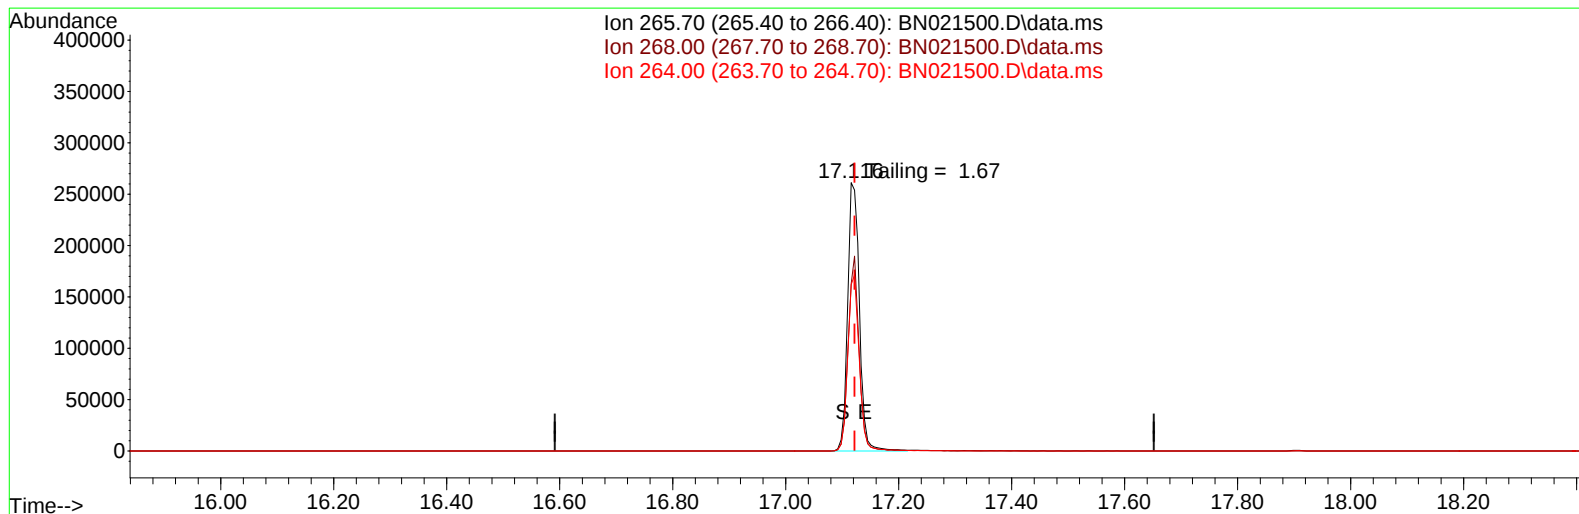

TIC: BN021500.D\data.ms

(70) Pentachlorophenol (C)




17.116min (-0.006) 23932.71 ng

response 380519

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.36
264.00	61.60	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083122\
Data File : BN021500.D
Acq On : 31 Aug 2022 22:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 06:52:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 01 06:50:58 2022
Response via : Initial Calibration

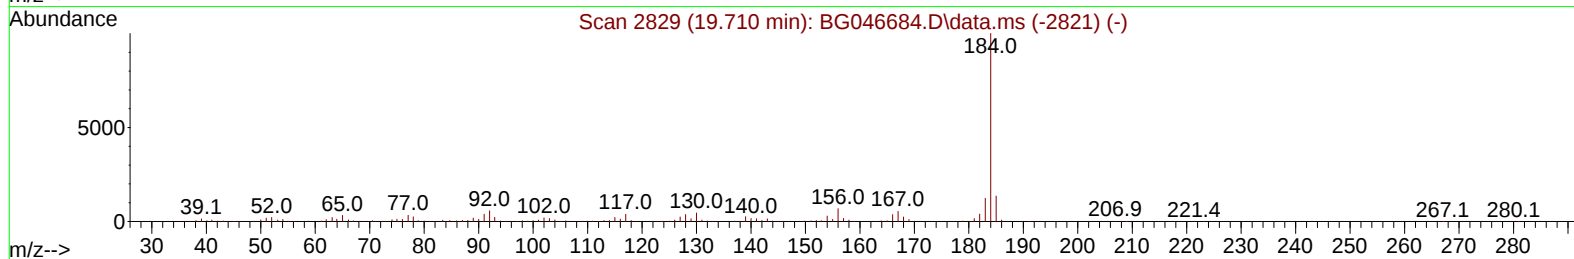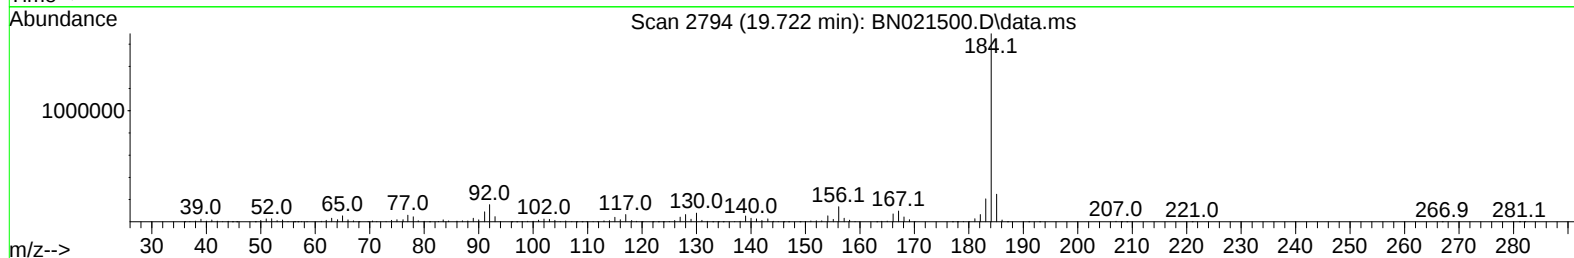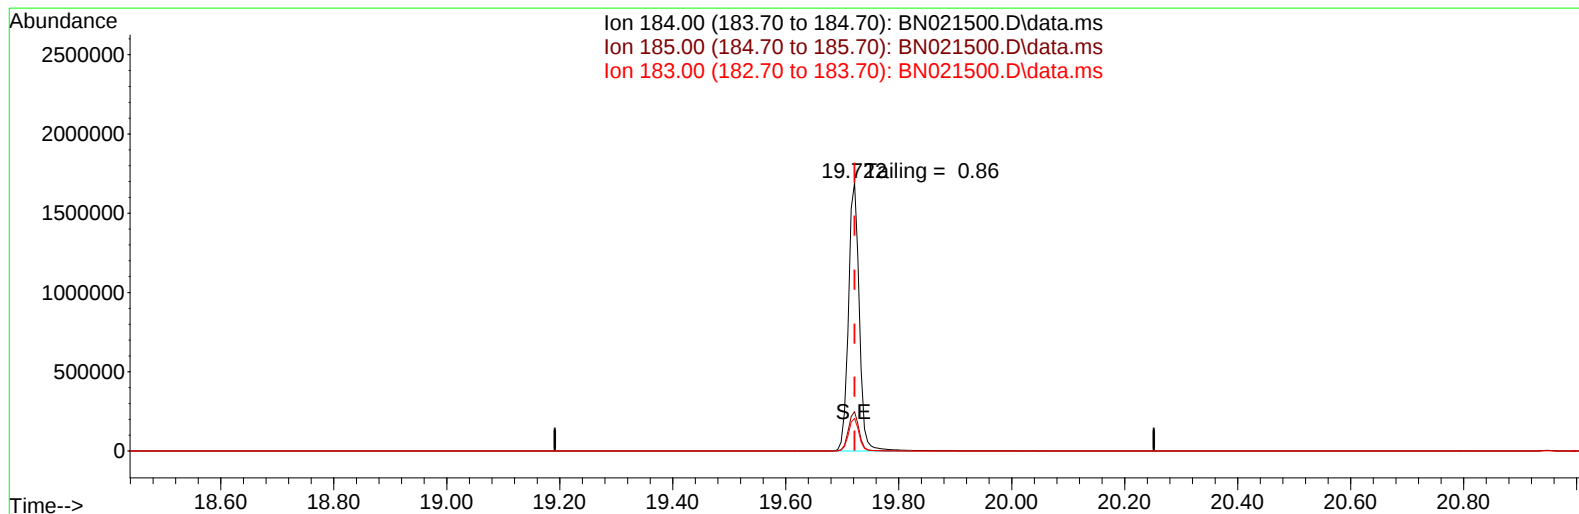

TIC: BN021500.D\data.ms

(77) Benzidine

19.722min (+ 0.000) 0.00 ng

response 2265759

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.65
183.00	13.20	12.19
0.00	0.00	0.00