

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN083122\  
 Data File : BN021496.D  
 Acq On : 31 Aug 2022 18:28  
 Operator : CG/JU  
 Sample : N4297-14  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 RE131D2-20220821

Quant Time: Sep 01 03:21:11 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN082922.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 29 16:30:43 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc  | Units | Dev(Min) |
|-------------------------------|--------|------|----------|-------|-------|----------|
| Internal Standards            |        |      |          |       |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.076  | 152  | 4129     | 0.400 | ng    | 0.00     |
| 7) Naphthalene-d8             | 10.909 | 136  | 12844    | 0.400 | ng    | 0.00     |
| 13) Acenaphthene-d10          | 14.728 | 164  | 6907     | 0.400 | ng    | 0.00     |
| 19) Phenanthrene-d10          | 17.480 | 188  | 15442    | 0.400 | ng    | 0.00     |
| 29) Chrysene-d12              | 21.664 | 240  | 12299    | 0.400 | ng    | # 0.00   |
| 35) Perylene-d12              | 24.191 | 264  | 8346     | 0.400 | ng    | 0.00     |
| System Monitoring Compounds   |        |      |          |       |       |          |
| 4) 2-Fluorophenol             | 5.599  | 112  | 1253     | 0.155 | ng    | 0.00     |
| 5) Phenol-d6                  | 7.224  | 99   | 911      | 0.088 | ng    | 0.00     |
| 8) Nitrobenzene-d5            | 9.243  | 82   | 2909     | 0.335 | ng    | -0.01    |
| 11) 2-Methylnaphthalene-d10   | 12.490 | 152  | 11549    | 0.399 | ng    | 0.00     |
| 14) 2,4,6-Tribromophenol      | 16.218 | 330  | 737      | 0.325 | ng    | 0.00     |
| 15) 2-Fluorobiphenyl          | 13.360 | 172  | 10845    | 0.359 | ng    | 0.00     |
| 27) Fluoranthene-d10          | 19.506 | 212  | 20158    | 0.508 | ng    | 0.00     |
| 31) Terphenyl-d14             | 20.097 | 244  | 13967    | 0.505 | ng    | 0.00     |
| Target Compounds              |        |      |          |       |       |          |
| 2) 1,4-Dioxane                | 3.403  | 88   | 45649    | 8.839 | ng    | # 89     |
| 34) Bis(2-ethylhexyl)phtha... | 21.566 | 149  | 1314     | 0.076 | ng    | 99       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN083122\  
Data File : BN021496.D  
Acq On : 31 Aug 2022 18:28  
Operator : CG/JU  
Sample : N4297-14  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
RE131D2-20220821


Quant Time: Sep 01 03:21:11 2022  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN082922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 29 16:30:43 2022  
Response via : Initial Calibration

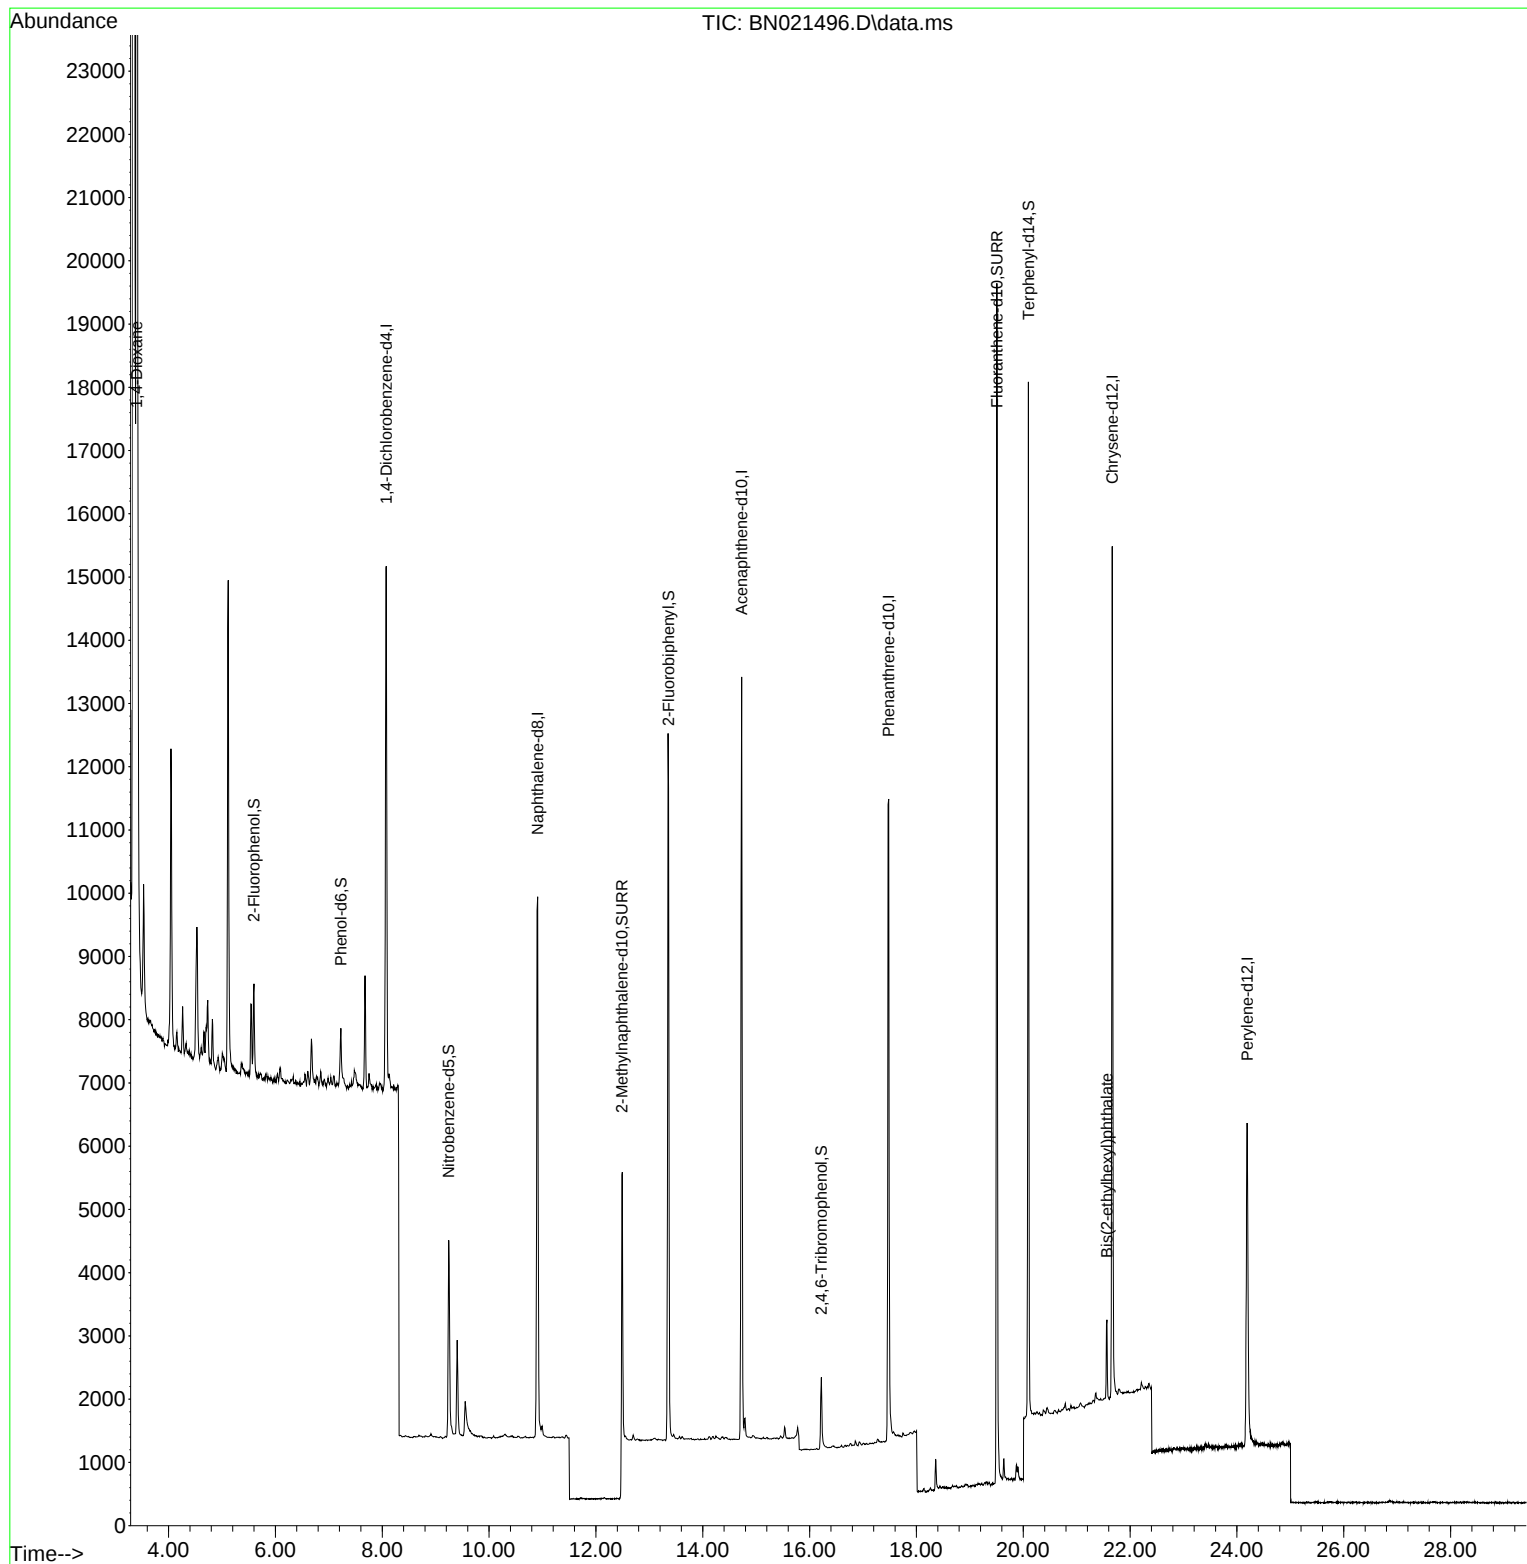





#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 8.076 min Scan# 60  
Delta R.T. -0.007 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28

Instrument :  
BNA\_N  
ClientSampleId :  
RE131D2-20220821



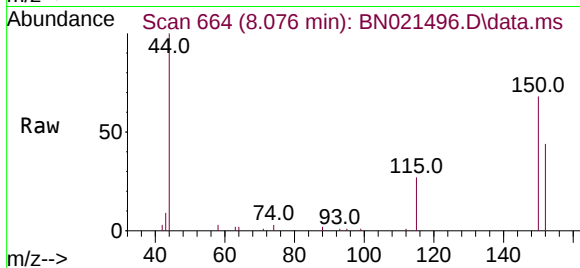


Tgt Ion:152 Resp: 4129  
Ion Ratio Lower Upper  
152 100  
150 152.2 121.4 182.0  
115 59.8 48.6 72.8

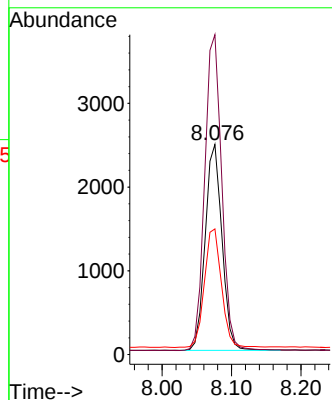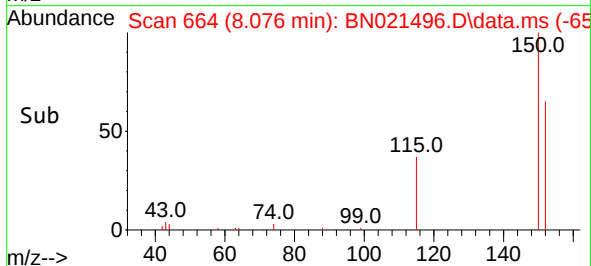

#2  
1,4-Dioxane  
Concen: 8.839 ng  
RT: 3.403 min Scan# 17  
Delta R.T. -0.007 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28

Tgt Ion: 88 Resp: 45649  
Ion Ratio Lower Upper  
88 100  
43 27.5 35.8 53.8#  
58 71.8 57.1 85.7

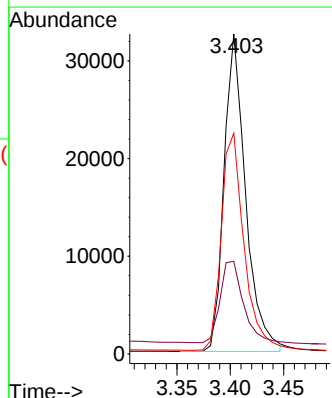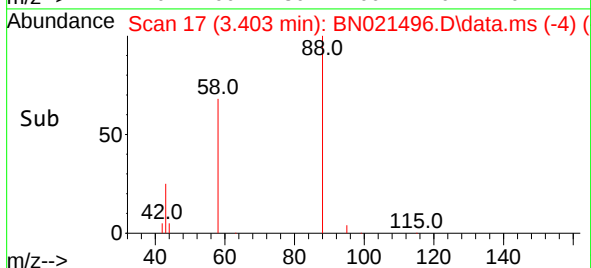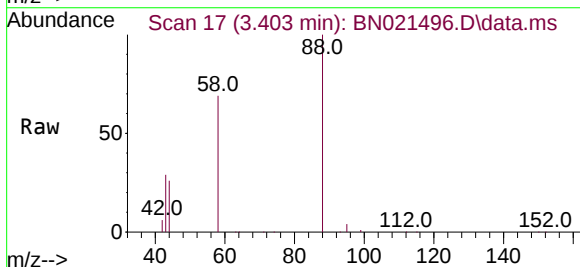



#4

2-Fluorophenol

Concen: 0.155 ng

RT: 5.599 min Scan# 321

Delta R.T. 0.000 min

Lab File: BN021496.D

Acq: 31 Aug 2022 18:28

Instrument :

BNA\_N

ClientSampleId :

RE131D2-20220821





Tgt Ion:112 Resp: 1253

Ion Ratio Lower Upper

112 100

64 57.1 43.5 65.3

63 28.9 22.6 34.0

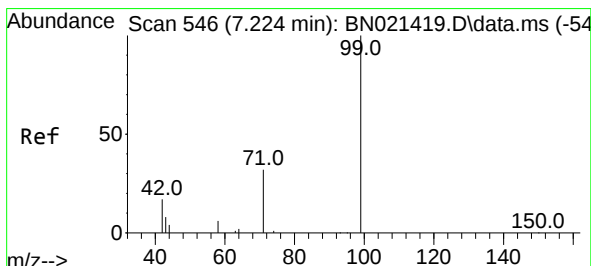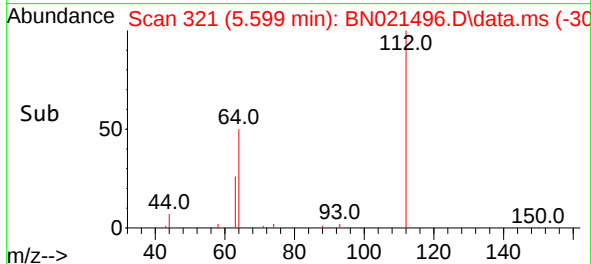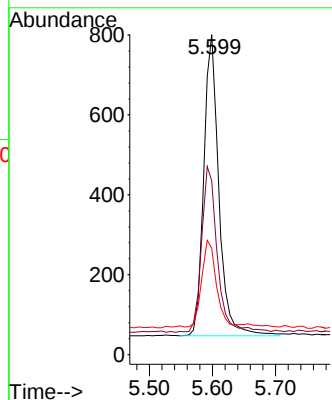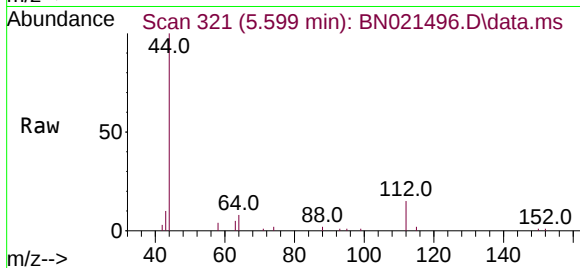

#5

Phenol-d6

Concen: 0.088 ng

RT: 7.224 min Scan# 546

Delta R.T. 0.000 min

Lab File: BN021496.D

Acq: 31 Aug 2022 18:28




Tgt Ion: 99 Resp: 911


Ion Ratio Lower Upper

99 100

42 17.8 15.5 23.3

71 46.1 24.2 36.2#


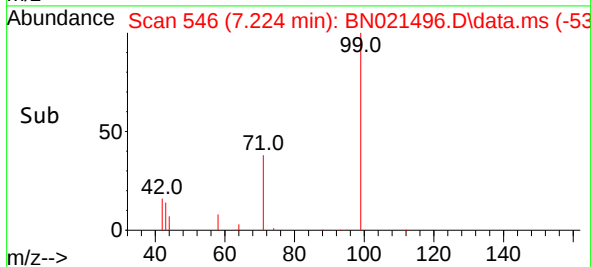
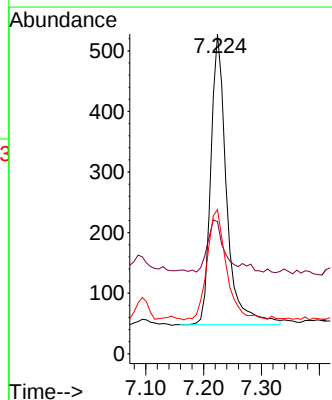
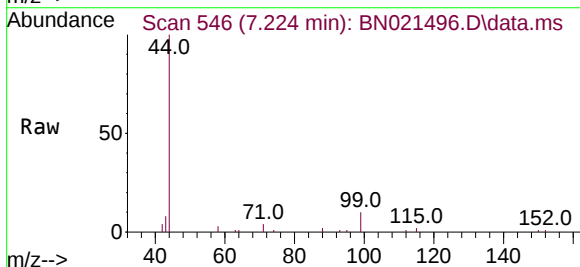


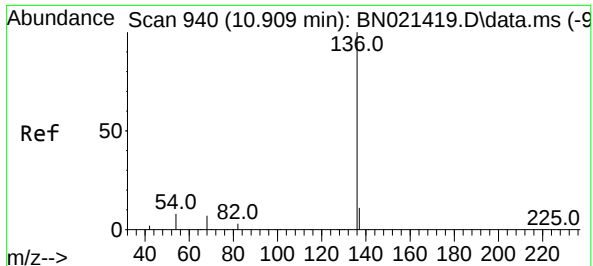

#7  
Naphthalene-d8  
Concen: 0.400 ng  
RT: 10.909 min Scan# 94  
Delta R.T. -0.000 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28




Instrument :  
BNA\_N  
ClientSampleId :  
RE131D2-20220821

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 136   | Resp: | 12844 |
| Ion Ratio | Lower | Upper |       |
| 136       | 100   |       |       |
| 137       | 11.8  | 9.3   | 13.9  |
| 54        | 7.0   | 6.9   | 10.3  |
| 68        | 6.1   | 6.1   | 9.1   |

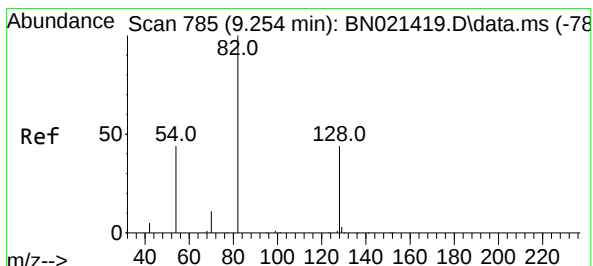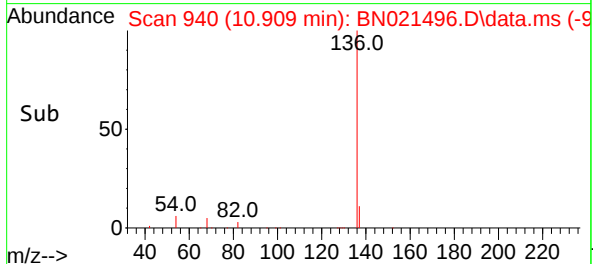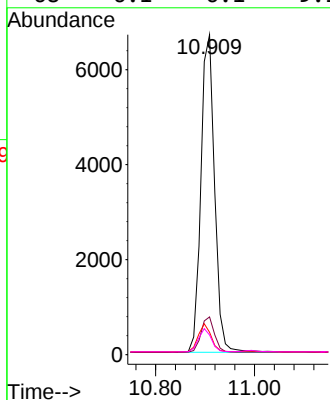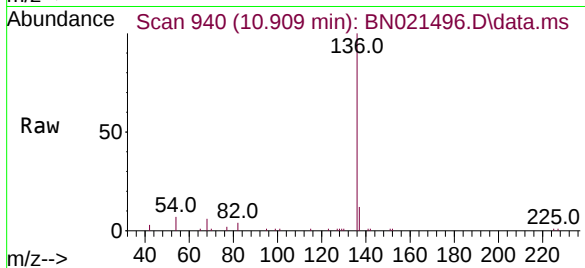

#8  
Nitrobenzene-d5  
Concen: 0.335 ng  
RT: 9.243 min Scan# 784  
Delta R.T. -0.011 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28

|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 82    | Resp: | 2909 |
| Ion Ratio | Lower | Upper |      |
| 82        | 100   |       |      |
| 128       | 38.3  | 30.9  | 46.3 |
| 54        | 53.2  | 42.7  | 64.1 |


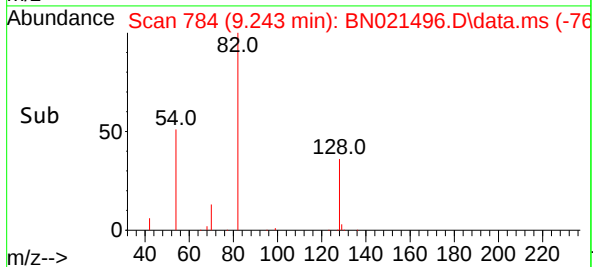
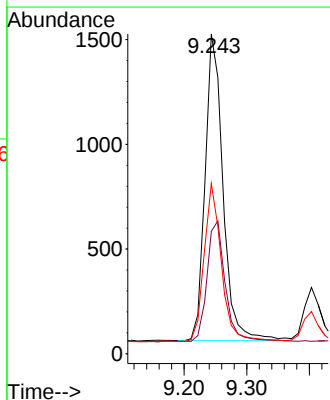
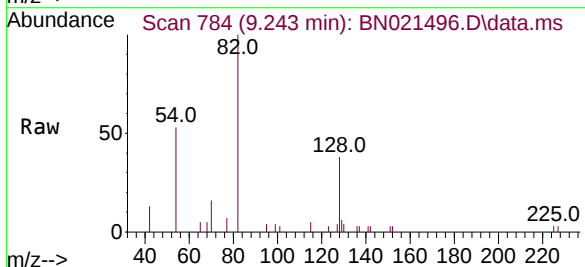




#11  
2-Methylnaphthalene-d10  
Concen: 0.399 ng  
RT: 12.490 min Scan# 11  
Delta R.T. -0.007 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28




Instrument :  
BNA\_N  
ClientSampleId :  
RE131D2-20220821

Tgt Ion:152 Resp: 11549  
Ion Ratio Lower Upper  
152 100  
151 18.3 14.5 21.7

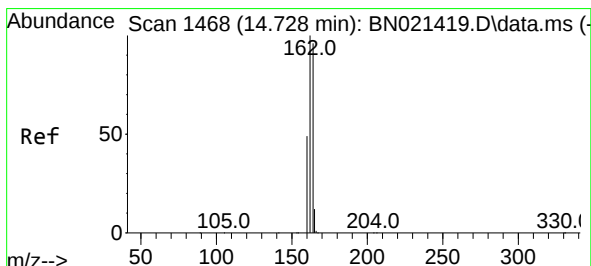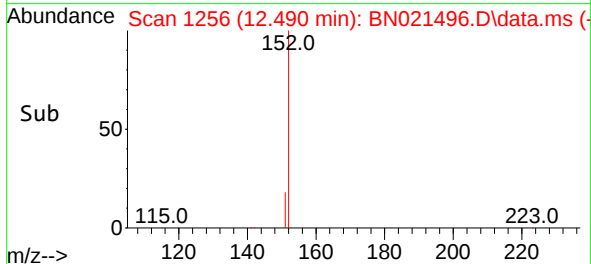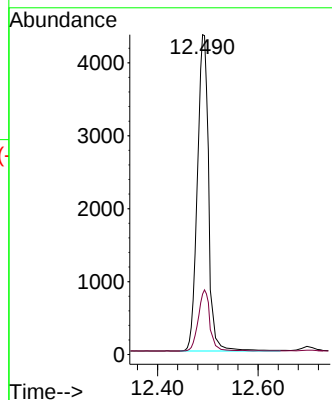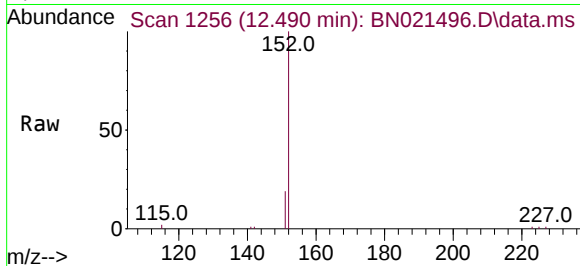

#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.728 min Scan# 1468  
Delta R.T. 0.000 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28

Tgt Ion:164 Resp: 6907  
Ion Ratio Lower Upper  
164 100  
162 104.1 82.2 123.4  
160 50.1 39.5 59.3


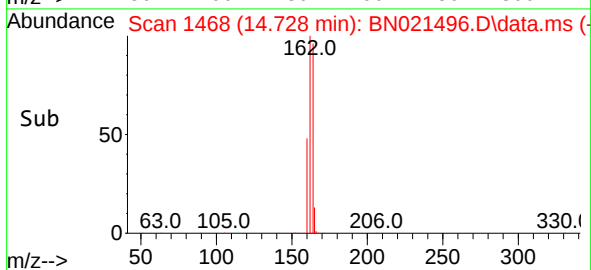
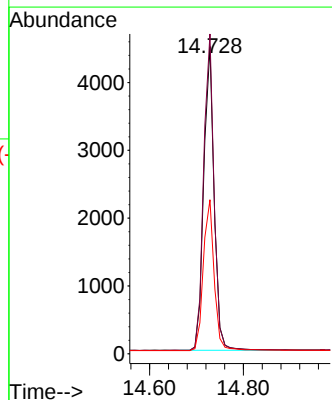
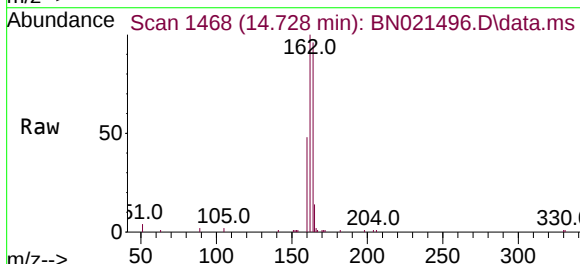




#14  
2,4,6-Tribromophenol  
Concen: 0.325 ng  
RT: 16.218 min Scan# 1609  
Delta R.T. 0.000 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28




Instrument :  
BNA\_N  
ClientSampleId :  
RE131D2-20220821


|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 330   | Resp: | 737   |
| Ion Ratio | Lower | Upper |       |
| 330       | 100   |       |       |
| 332       | 93.6  | 79.3  | 118.9 |
| 141       | 45.2  | 37.1  | 55.7  |

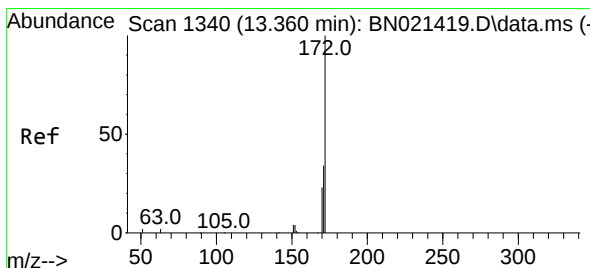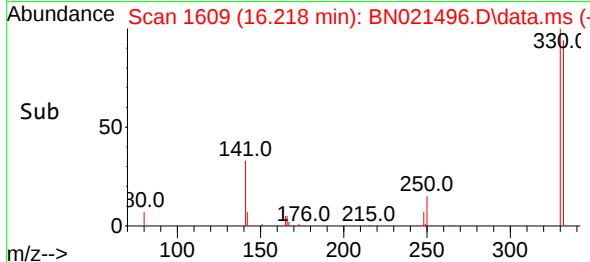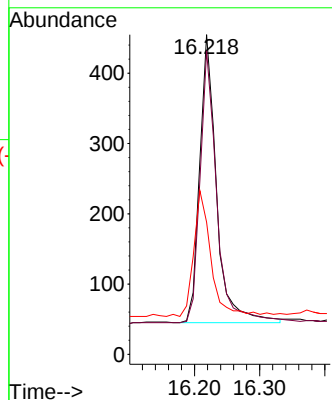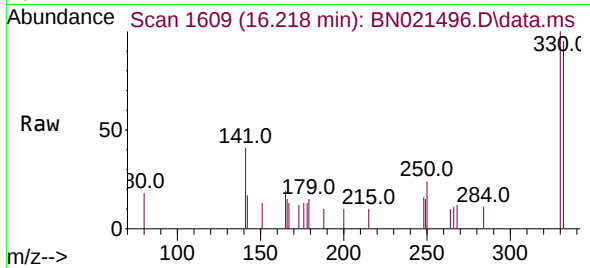

#15  
2-Fluorobiphenyl  
Concen: 0.359 ng  
RT: 13.360 min Scan# 1340  
Delta R.T. 0.000 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 172   | Resp: | 10845 |
| Ion Ratio | Lower | Upper |       |
| 172       | 100   |       |       |
| 171       | 33.3  | 27.8  | 41.6  |
| 170       | 22.5  | 18.6  | 28.0  |


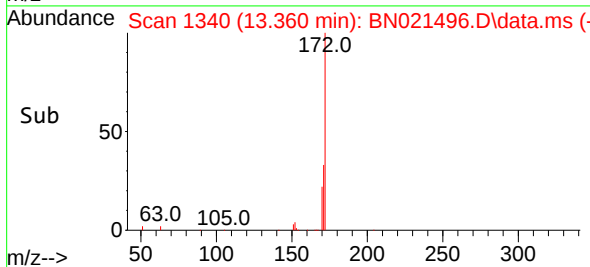
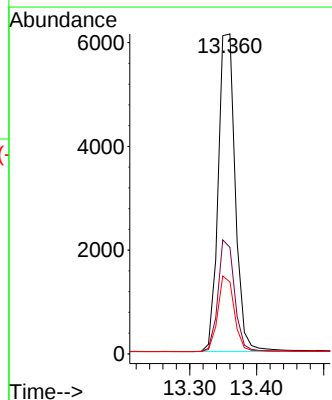
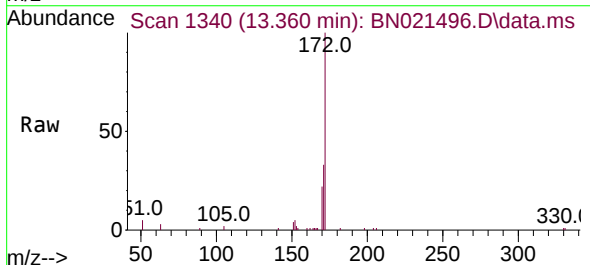


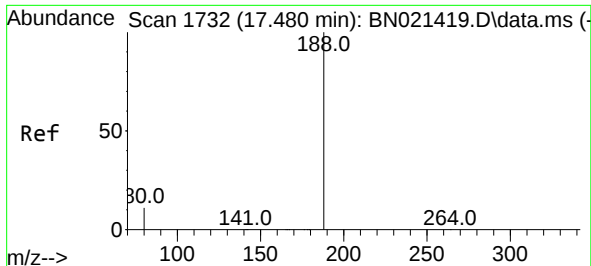

#19  
Phenanthrene-d10  
Concen: 0.400 ng  
RT: 17.480 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28




Instrument :  
BNA\_N  
ClientSampleId :  
RE131D2-20220821


Tgt Ion:188 Resp: 15442  
Ion Ratio Lower Upper  
188 100  
94 0.0 0.0 0.0  
80 10.1 9.5 14.3

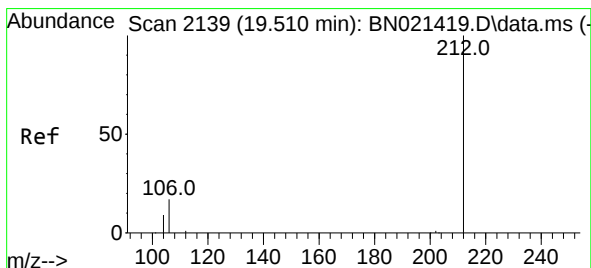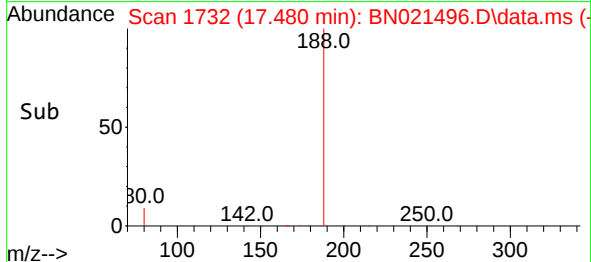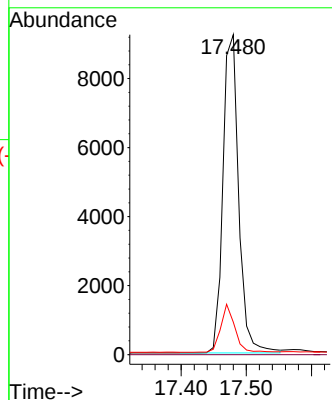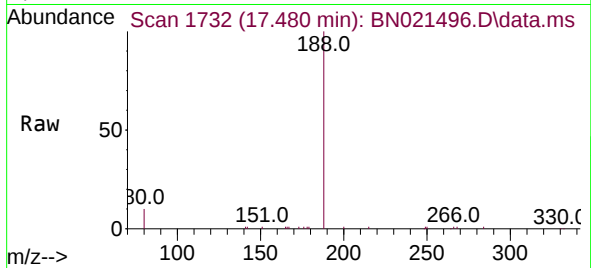

#27  
Fluoranthene-d10  
Concen: 0.508 ng  
RT: 19.506 min Scan# 2138  
Delta R.T. -0.004 min  
Lab File: BN021496.D  
Acq: 31 Aug 2022 18:28

Tgt Ion:212 Resp: 20158  
Ion Ratio Lower Upper  
212 100  
106 18.1 14.2 21.2  
104 10.2 7.8 11.6

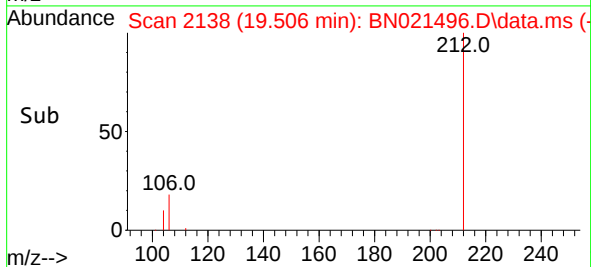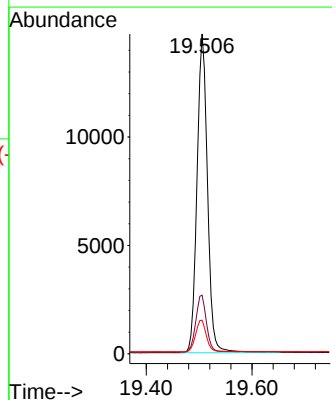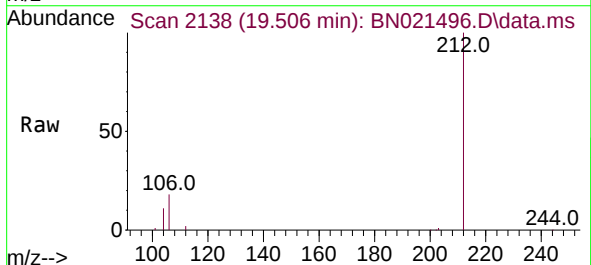

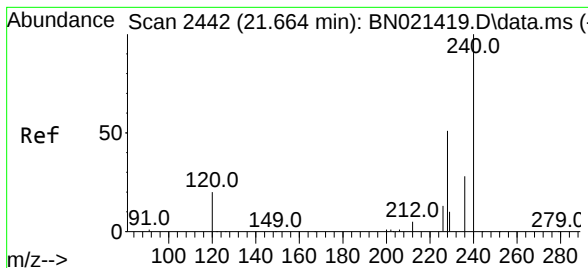

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.664 min Scan# 2442

Delta R.T. 0.000 min

Lab File: BN021496.D

Acq: 31 Aug 2022 18:28

Instrument :

BNA\_N

ClientSampleId :

RE131D2-20220821





Tgt Ion:240 Resp: 12299

Ion Ratio Lower Upper

240 100

120 17.5 10.2 15.4#

236 28.4 22.1 33.1

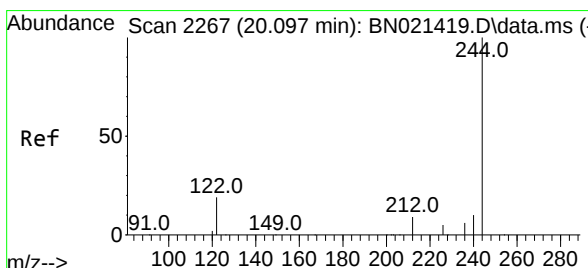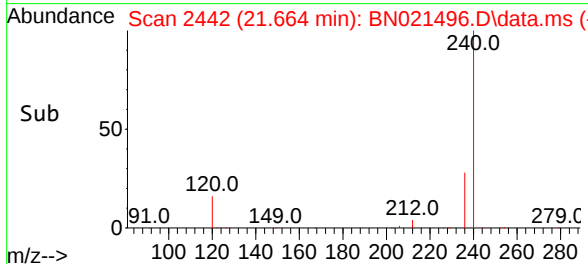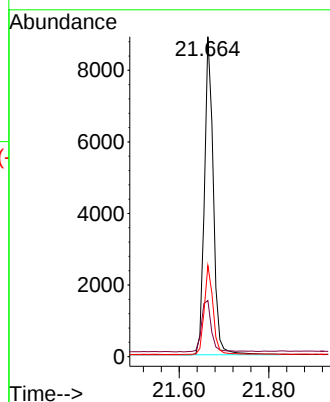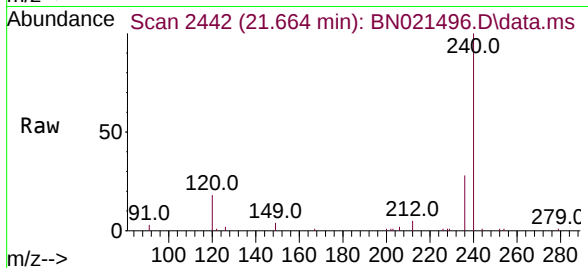

#31

Terphenyl-d14

Concen: 0.505 ng

RT: 20.097 min Scan# 2267

Delta R.T. 0.000 min

Lab File: BN021496.D

Acq: 31 Aug 2022 18:28




Tgt Ion:244 Resp: 13967


Ion Ratio Lower Upper

244 100

212 8.4 6.5 9.7

122 13.6 9.1 13.7


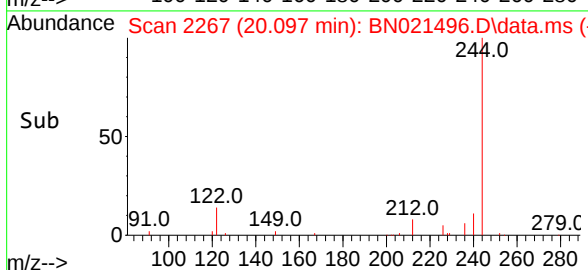
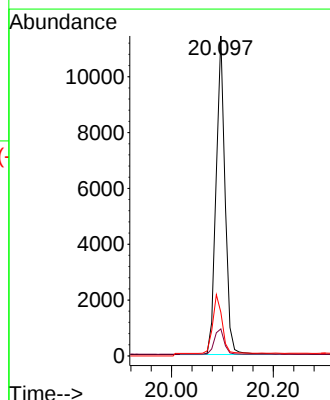
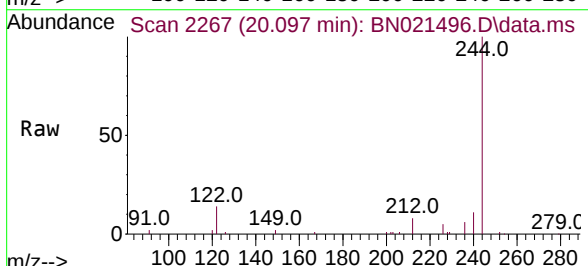


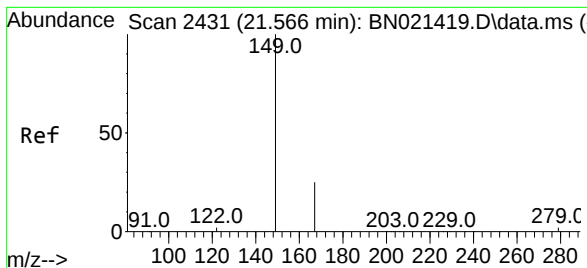

#34  
 Bis(2-ethylhexyl)phthalate  
 Concen: 0.076 ng  
 RT: 21.566 min Scan# 2431  
 Delta R.T. 0.000 min  
 Lab File: BN021496.D  
 Acq: 31 Aug 2022 18:28

Instrument :  
 BNA\_N  
 ClientSampleId :  
 RE131D2-20220821

Tgt Ion:149 Resp: 1314  
 Ion Ratio Lower Upper  
 149 100  
 167 26.4 21.4 32.0  
 279 3.0 2.2 3.2

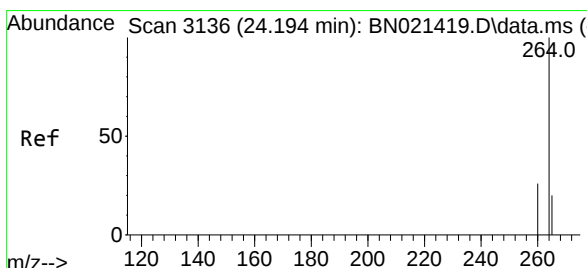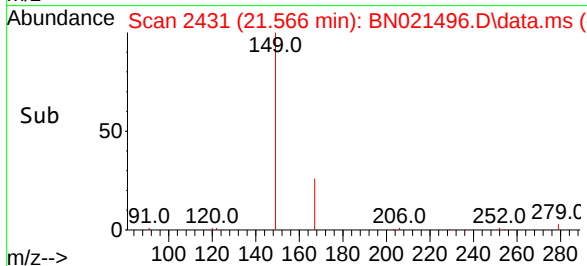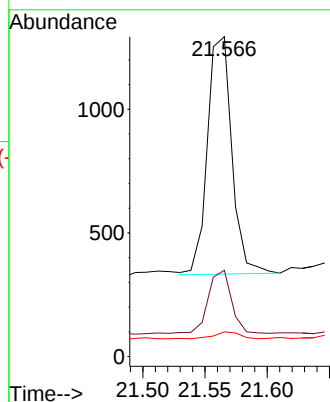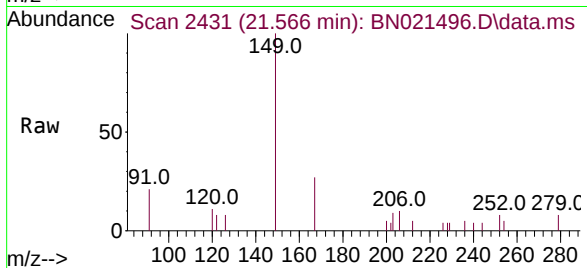

#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 24.191 min Scan# 3135  
 Delta R.T. -0.003 min  
 Lab File: BN021496.D  
 Acq: 31 Aug 2022 18:28

Tgt Ion:264 Resp: 8346  
 Ion Ratio Lower Upper  
 264 100  
 260 27.4 21.0 31.6  
 265 37.8 32.2 48.2

