
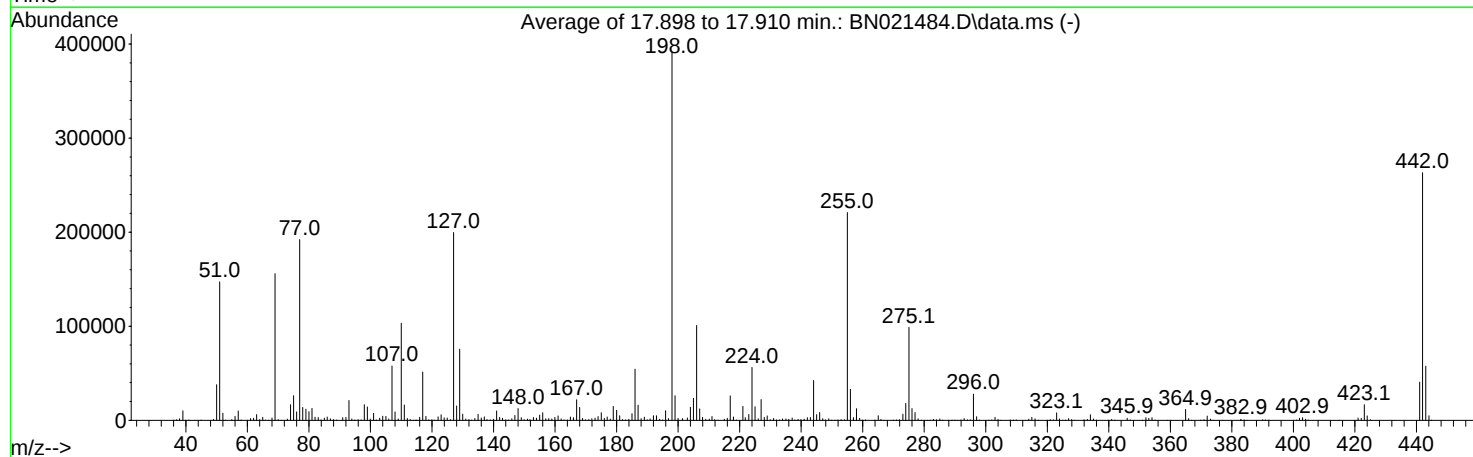


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083122\
 Data File : BN021484.D
 Acq On : 31 Aug 2022 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 29 16:30:43 2022

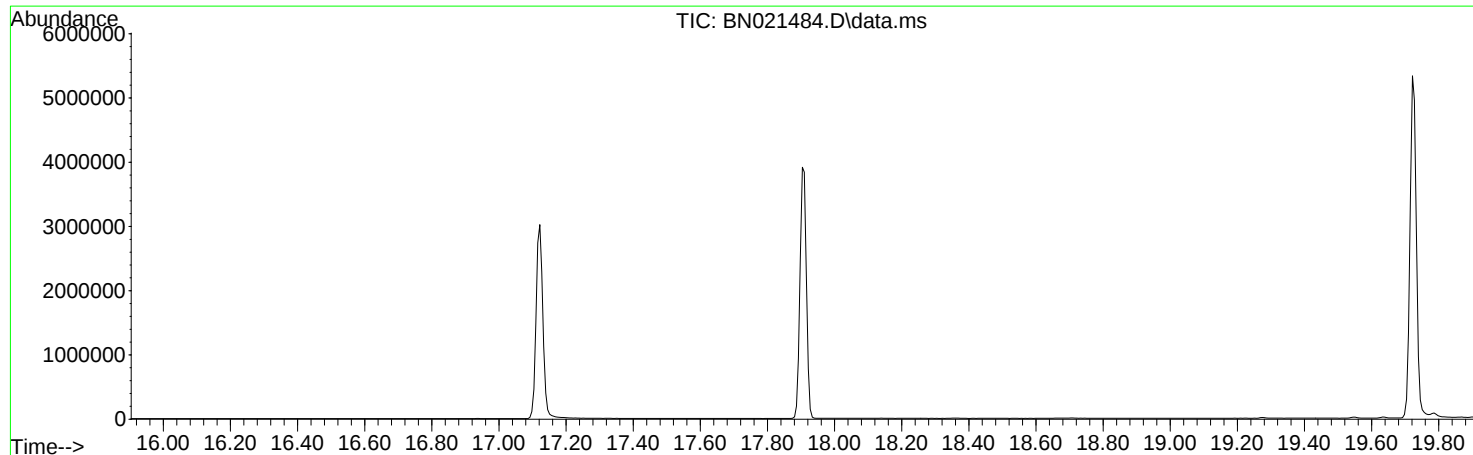




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	147305	PASS
68	69	0.00	2	1.6	2484	PASS
69	198	0.00	100	39.9	155947	PASS
70	69	0.00	2	0.5	786	PASS
127	198	10	80	51.0	199573	PASS
197	198	0.00	2	0.5	1820	PASS
198	198	100	100	100.0	391104	PASS
199	198	5	9	6.7	26053	PASS
275	198	10	60	25.3	98829	PASS
365	198	1	100	2.9	11420	PASS
441	198	0.01	100	10.4	40568	PASS
442	442	50	100	100.0	263189	PASS
443	442	15	24	21.9	57592	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083122\
 Data File : BN021484.D
 Acq On : 31 Aug 2022 09:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 01 06:51:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 01 06:50:58 2022
 Response via : Initial Calibration

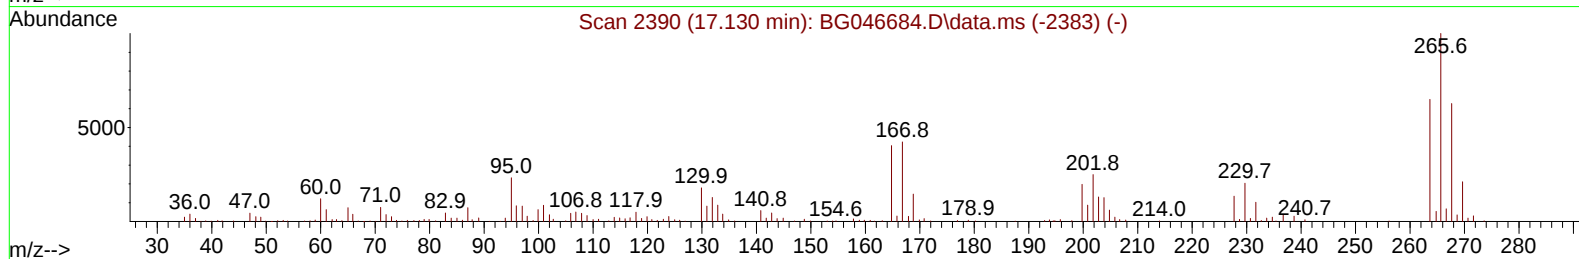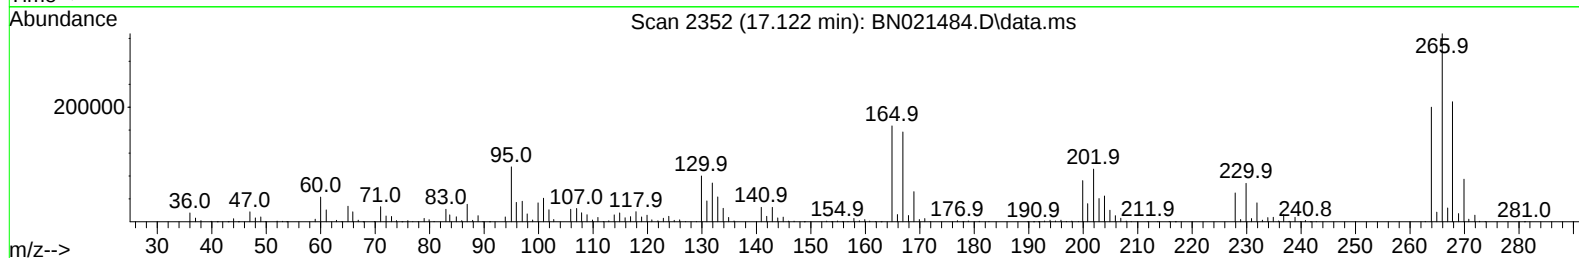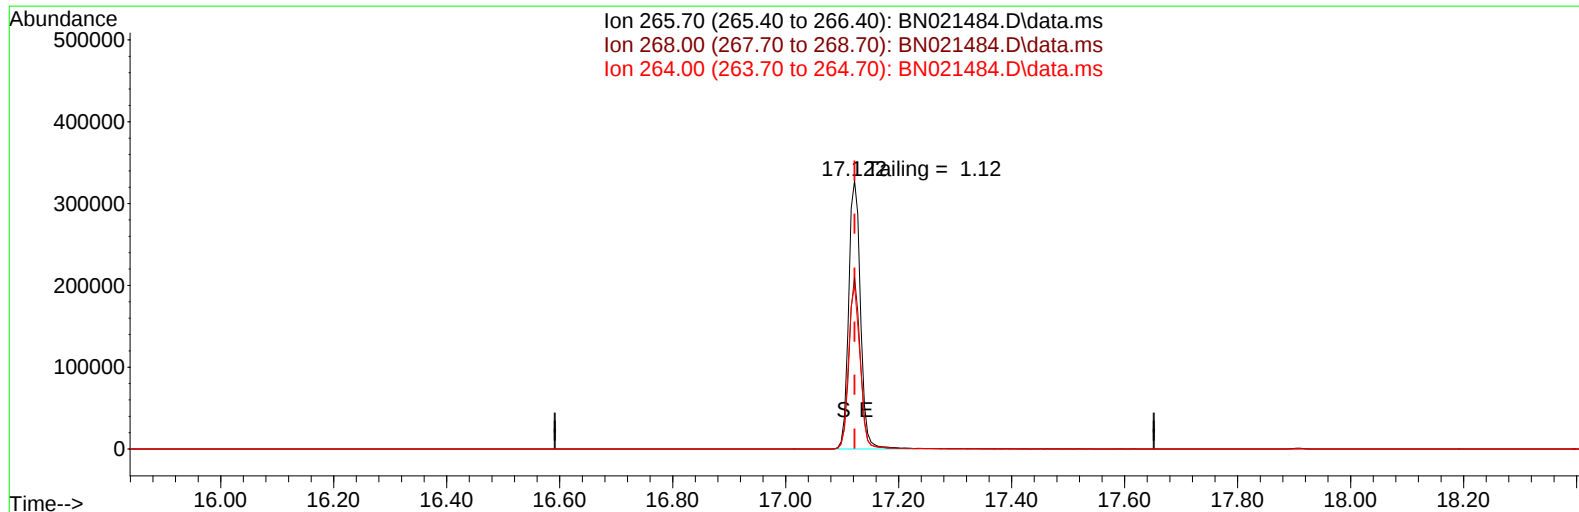

TIC: BN021484.D\data.ms

(70) Pentachlorophenol (C)

17.122min (0.000) 485283.27 ng




response 479856

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.83
264.00	61.60	60.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083122\
Data File : BN021484.D
Acq On : 31 Aug 2022 09:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 01 06:51:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 01 06:50:58 2022
Response via : Initial Calibration

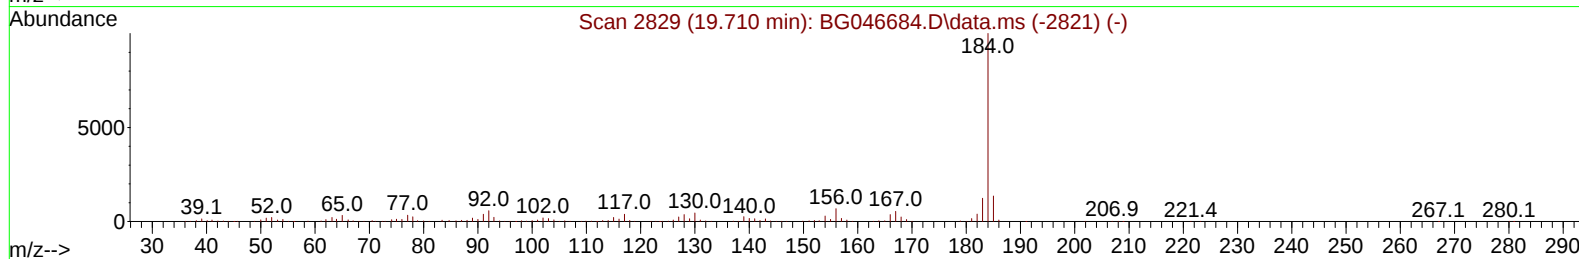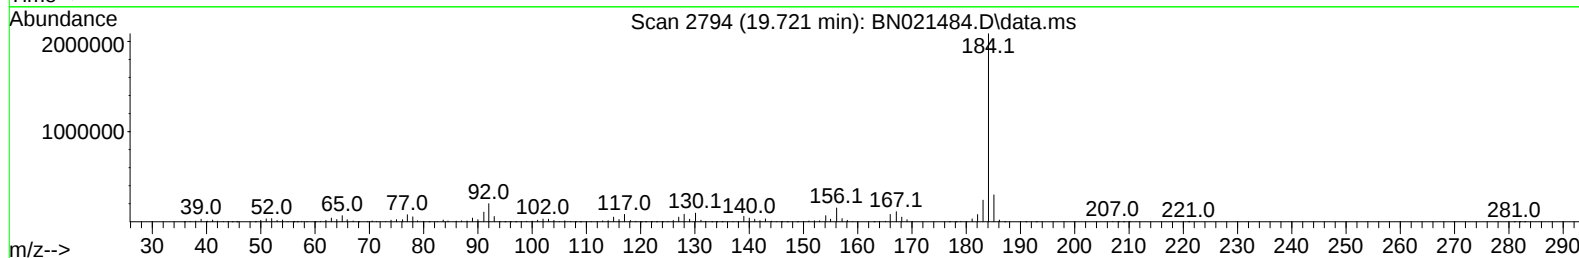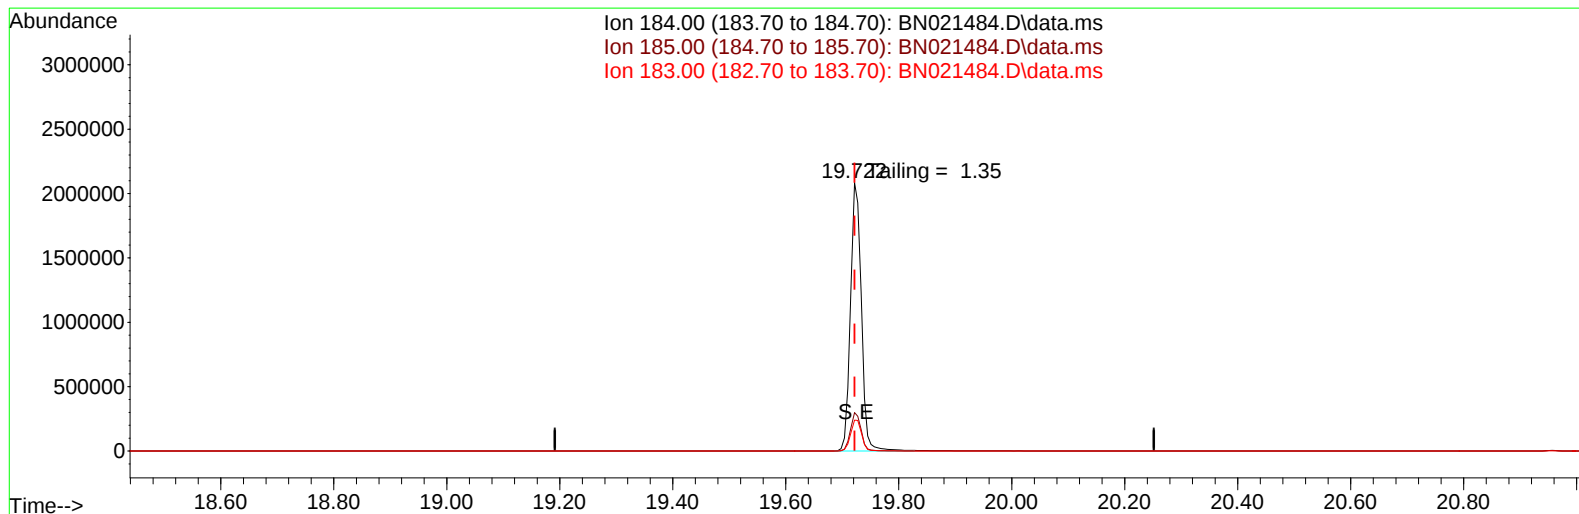

TIC: BN021484.D\data.ms

(77) Benzidine

19.721min (0.000) 0.00 ng

response 2814097

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.33
183.00	13.20	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/31/2022	BNA_N	<u>BN021484.D</u>
Compound Name	Response	Retention Time
DDT	1303544	20.957
DDD	14670	20.516
DDE	774	20.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15444	1318988	1.17

Instrument :
BNA_N
ClientSampleId :
DFTPP