
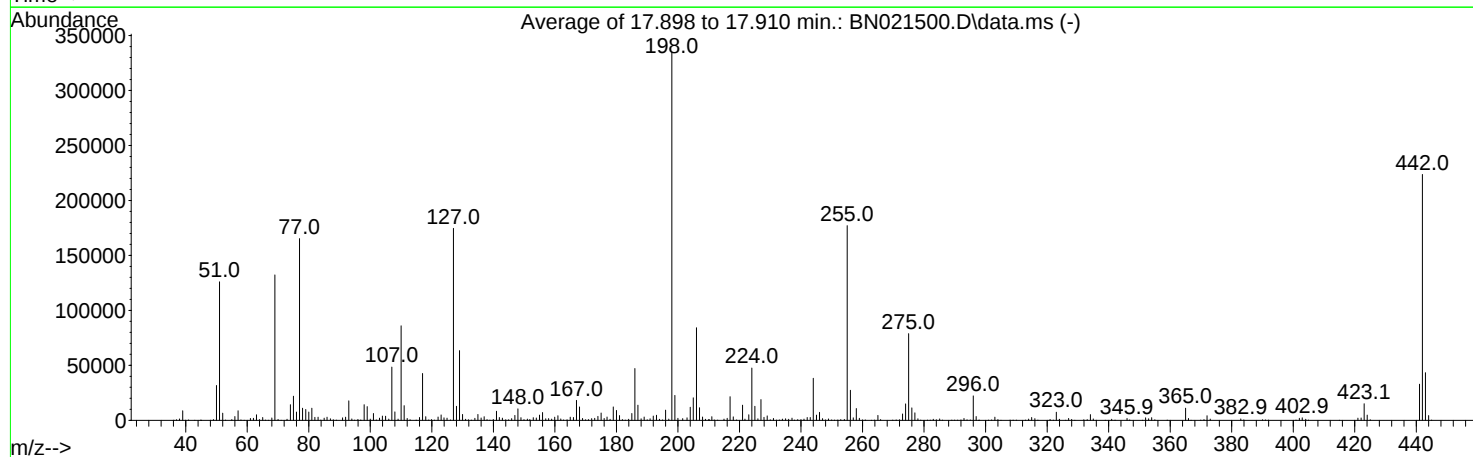


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083122\
 Data File : BN021500.D
 Acq On : 31 Aug 2022 22:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 29 16:30:43 2022

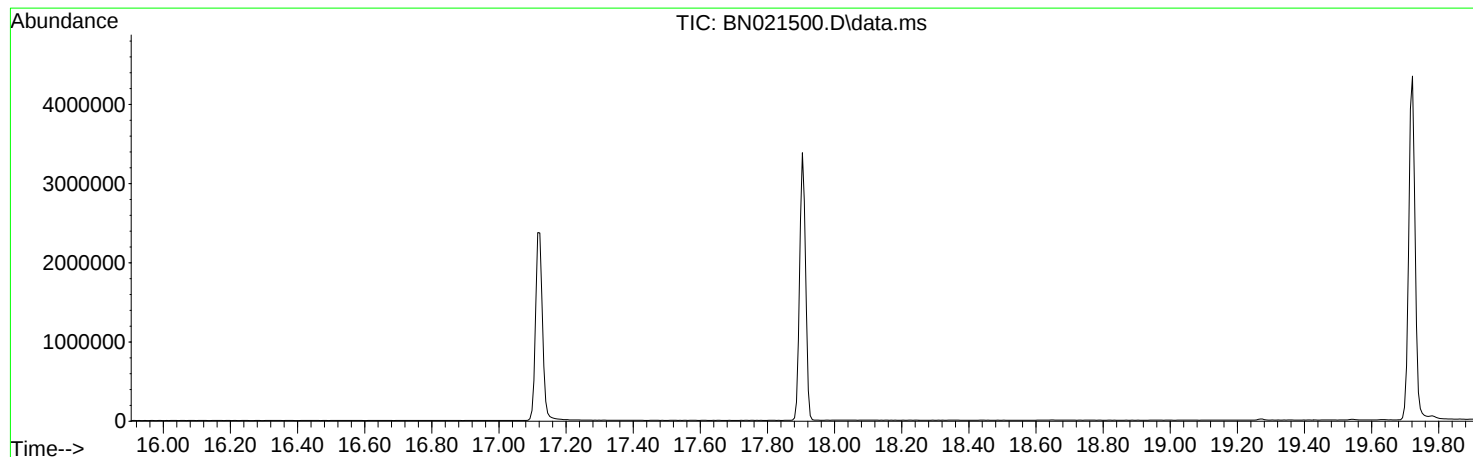




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	125960	PASS
68	69	0.00	2	1.6	2140	PASS
69	198	0.00	100	39.5	132304	PASS
70	69	0.00	2	0.6	782	PASS
127	198	10	80	52.2	174592	PASS
197	198	0.00	2	0.3	1033	PASS
198	198	100	100	100.0	334656	PASS
199	198	5	9	6.8	22637	PASS
275	198	10	60	23.5	78773	PASS
365	198	1	100	3.3	10963	PASS
441	198	0.01	100	9.8	32853	PASS
442	442	50	100	100.0	223680	PASS
443	442	15	24	19.4	43349	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083122\
 Data File : BN021500.D
 Acq On : 31 Aug 2022 22:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 01 06:52:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 01 06:50:58 2022
 Response via : Initial Calibration

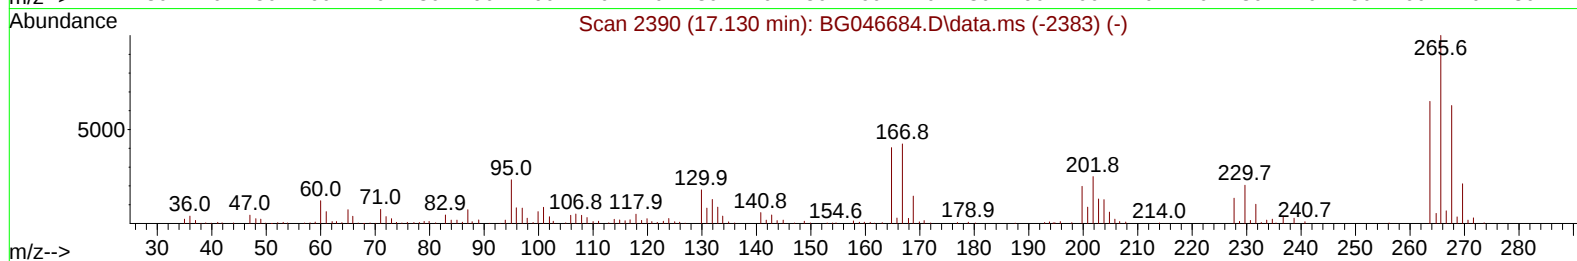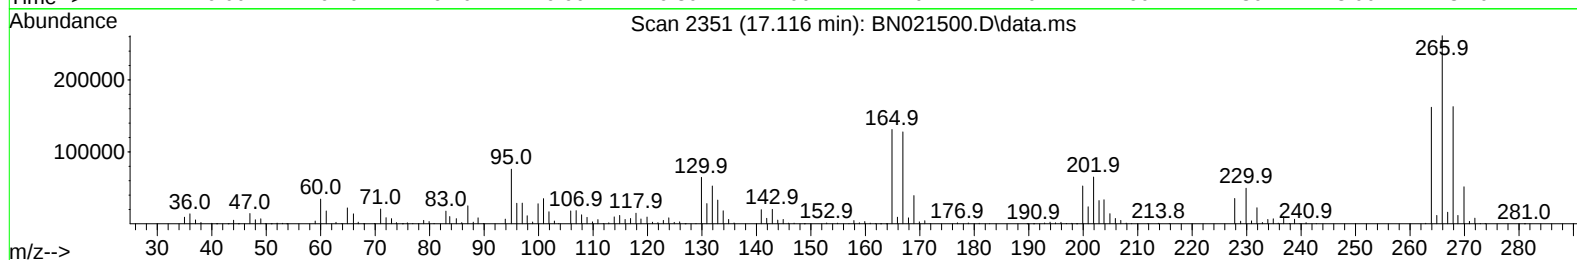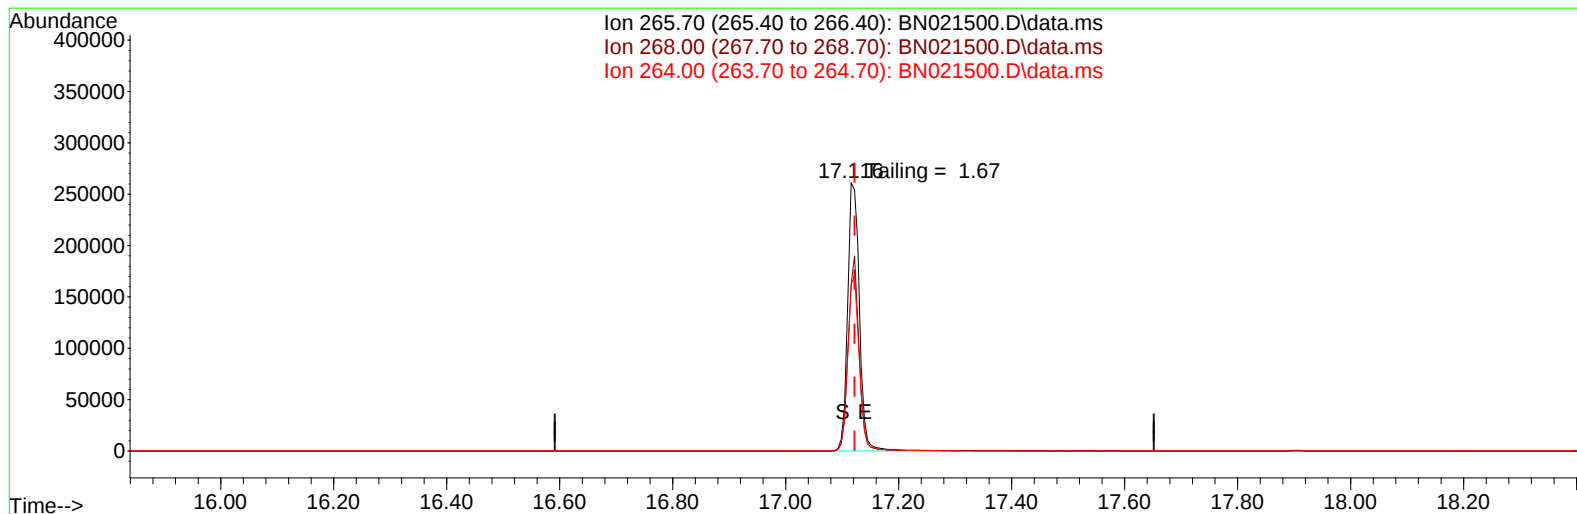

TIC: BN021500.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.006) 23932.71 ng




response 380519

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.36
264.00	61.60	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN083122\
Data File : BN021500.D
Acq On : 31 Aug 2022 22:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 01 06:52:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 01 06:50:58 2022
Response via : Initial Calibration

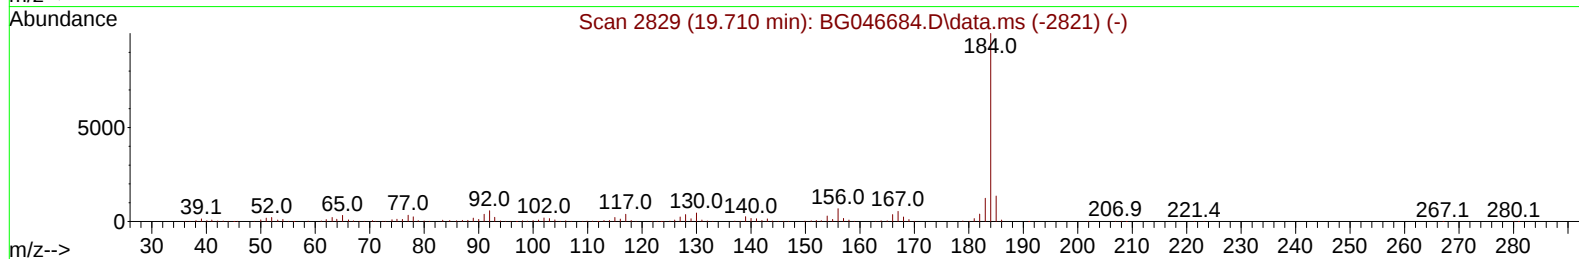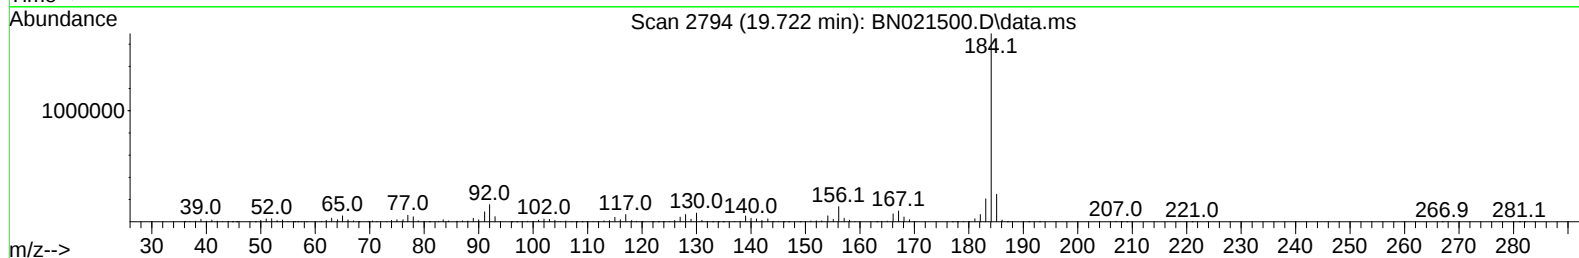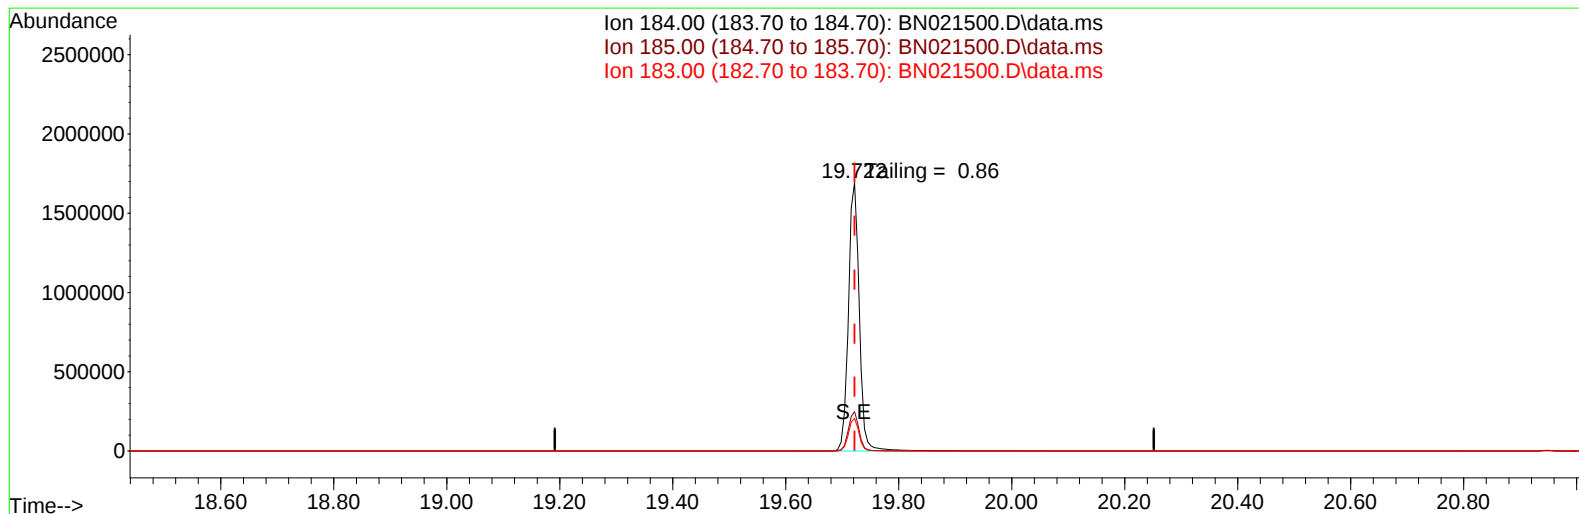

TIC: BN021500.D\data.ms

(77) Benzidine

19.722min (+ 0.000) 0.00 ng

response 2265759

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.65
183.00	13.20	12.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/31/2022	BNA_N	<u>BN021500.D</u>
Compound Name	Response	Retention Time
DDT	1112235	20.951
DDD	15315	20.51
DDE	728	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16043	1128278	1.42

Instrument :
BNA_N
ClientSampleId :
DFTPP