
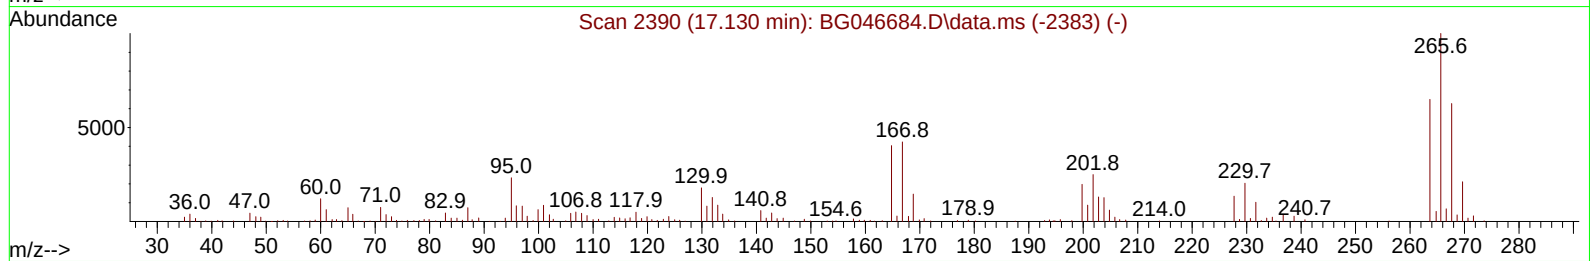
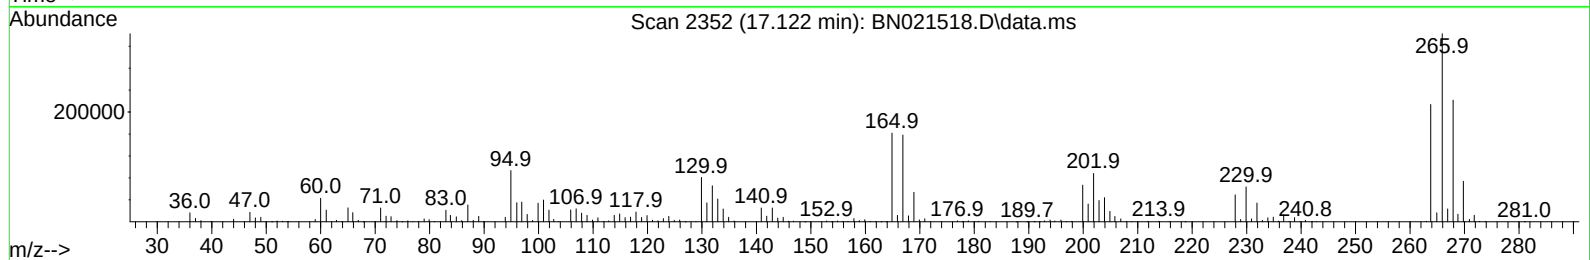


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN090122\  
Data File : BN021518.D  
Acq On : 01 Sep 2022 09:20  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 06:51:36 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 02 06:51:31 2022  
Response via : Initial Calibration

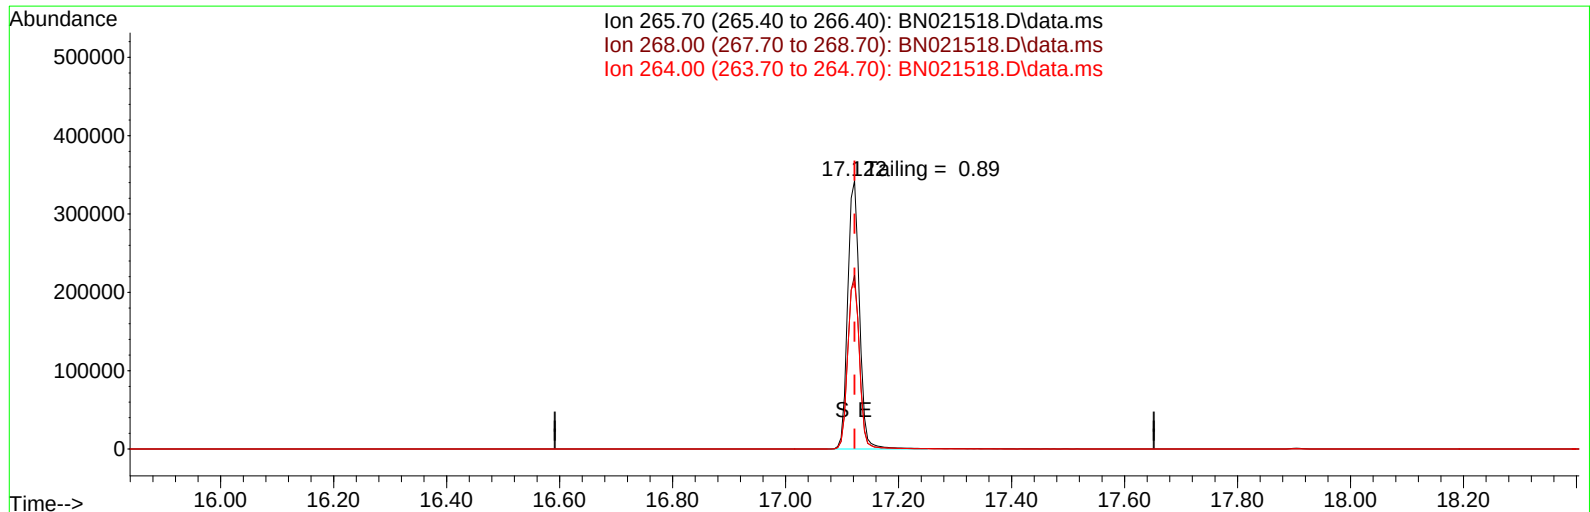

TIC: BN021518.D\data.ms

**(70) Pentachlorophenol (C)**




17.122min ( 0.000) 21889.07 ng

response 499536

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.71  |
| 264.00 | 61.60  | 62.43  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN090122\  
 Data File : BN021518.D  
 Acq On : 01 Sep 2022 09:20  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 06:51:36 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Sep 02 06:51:31 2022  
 Response via : Initial Calibration

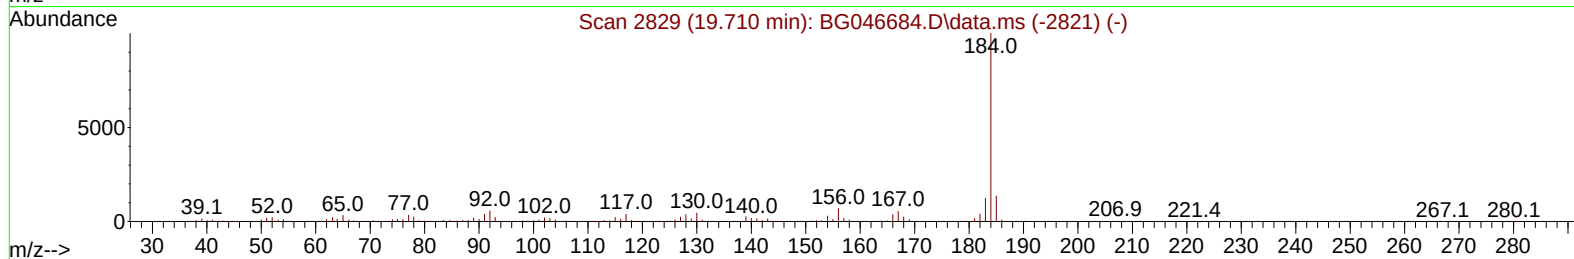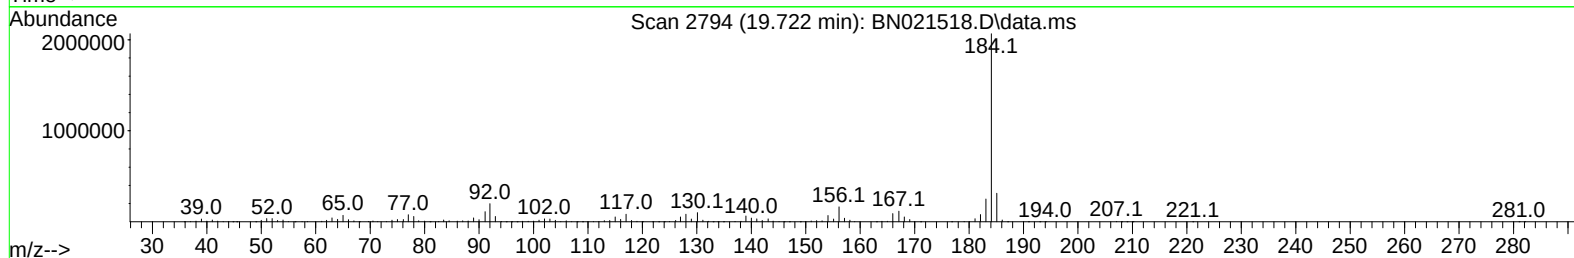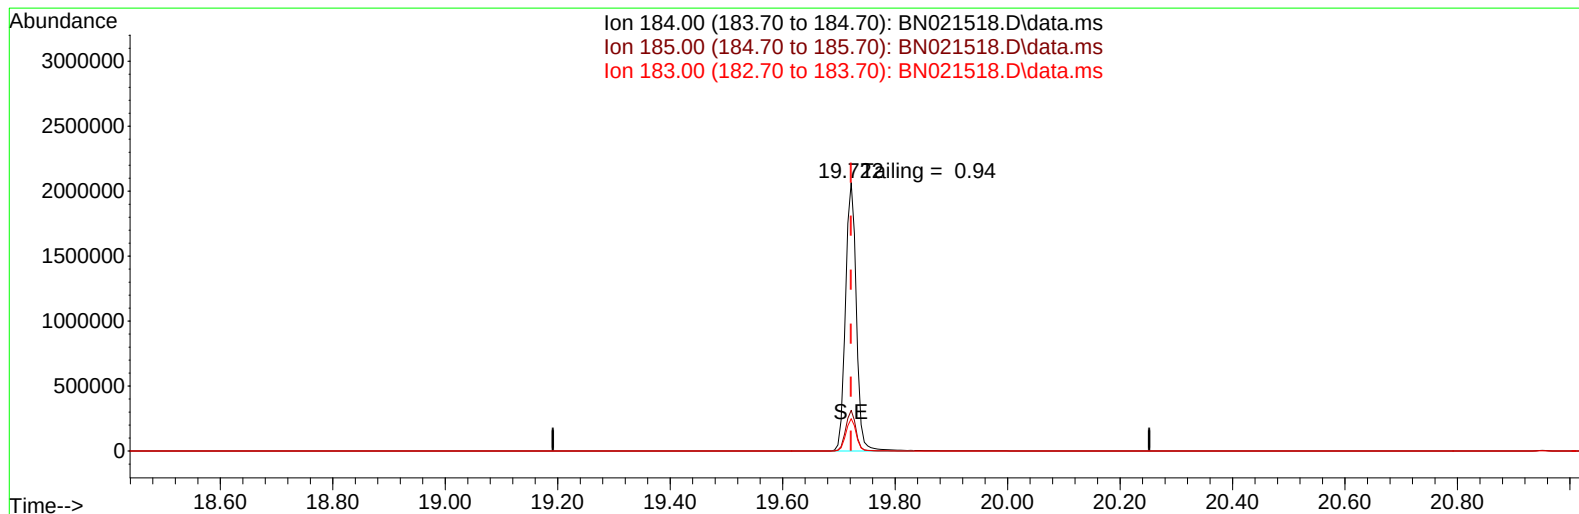

TIC: BN021518.D\data.ms

**(77) Benzidine**

19.722min ( 0.000) 0.00 ng

response 2783240

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 15.15  |
| 183.00 | 13.20  | 12.06  |
| 0.00   | 0.00   | 0.00   |