
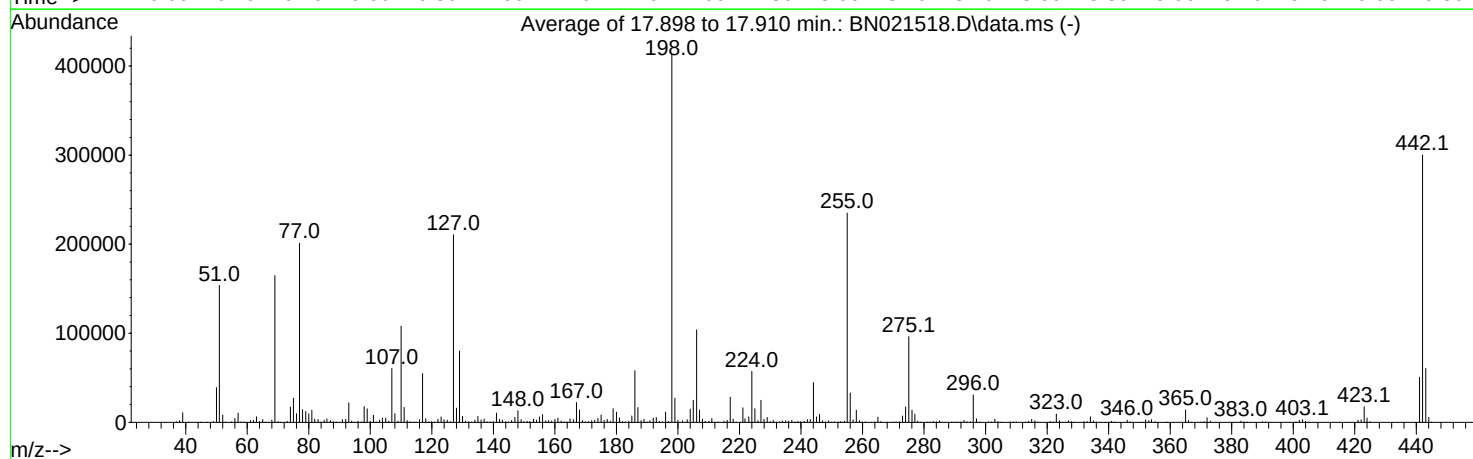


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090122\
 Data File : BN021518.D
 Acq On : 01 Sep 2022 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 00:53:31 2022

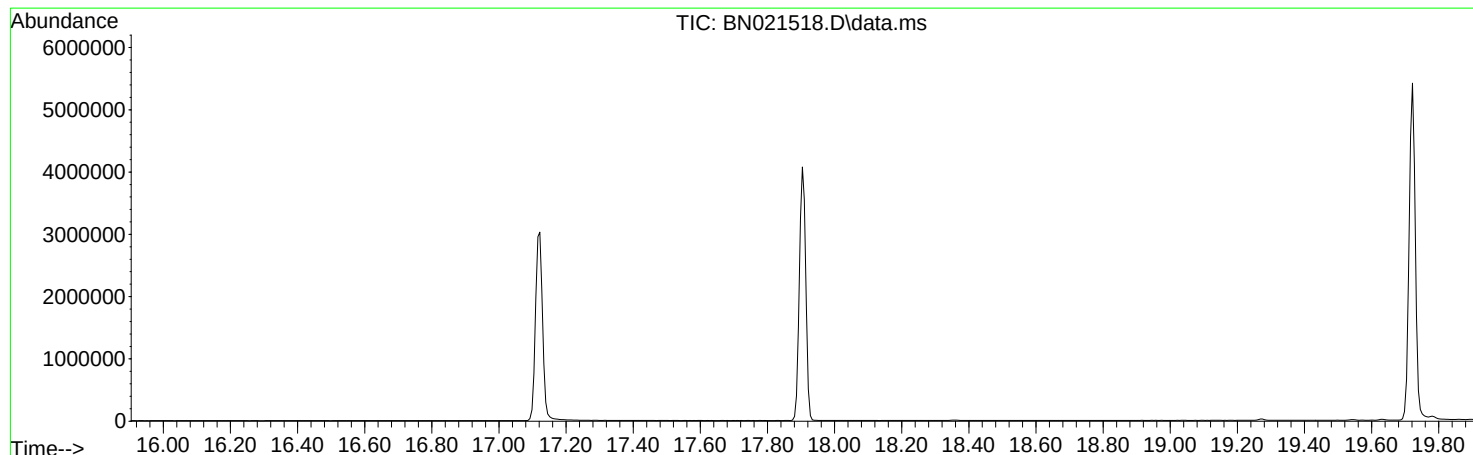




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	153633	PASS
68	69	0.00	2	1.6	2626	PASS
69	198	0.00	100	39.9	164800	PASS
70	69	0.00	2	0.5	851	PASS
127	198	10	80	51.0	210752	PASS
197	198	0.00	2	0.2	667	PASS
198	198	100	100	100.0	413077	PASS
199	198	5	9	6.6	27248	PASS
275	198	10	60	23.3	96261	PASS
365	198	1	100	3.3	13704	PASS
441	198	0.01	100	12.3	50645	PASS
442	442	50	100	100.0	300139	PASS
443	442	15	24	20.2	60488	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090122\
 Data File : BN021518.D
 Acq On : 01 Sep 2022 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 02 06:51:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 02 06:51:31 2022
 Response via : Initial Calibration

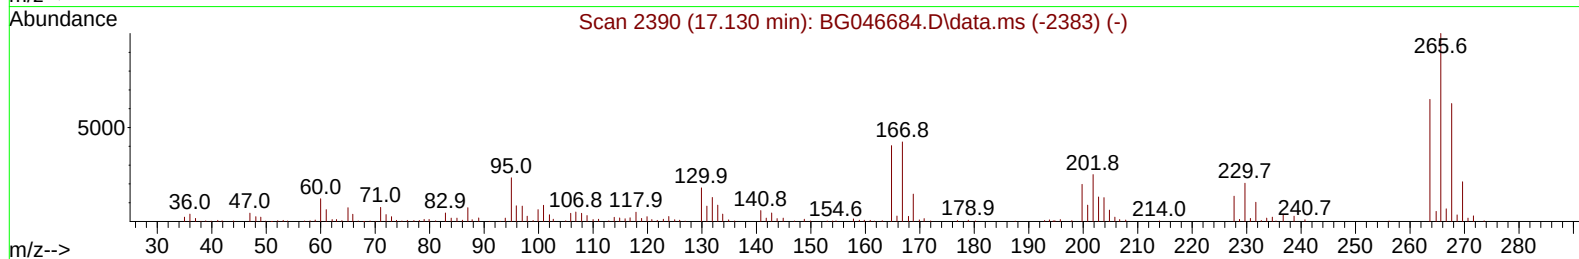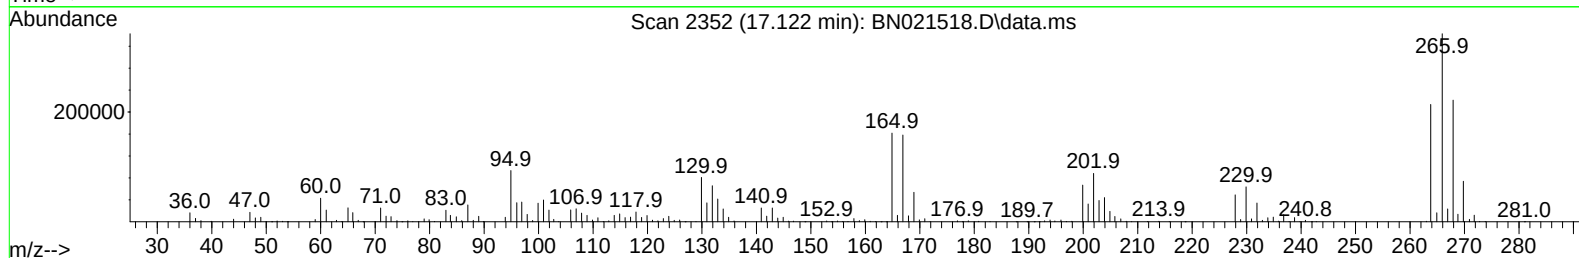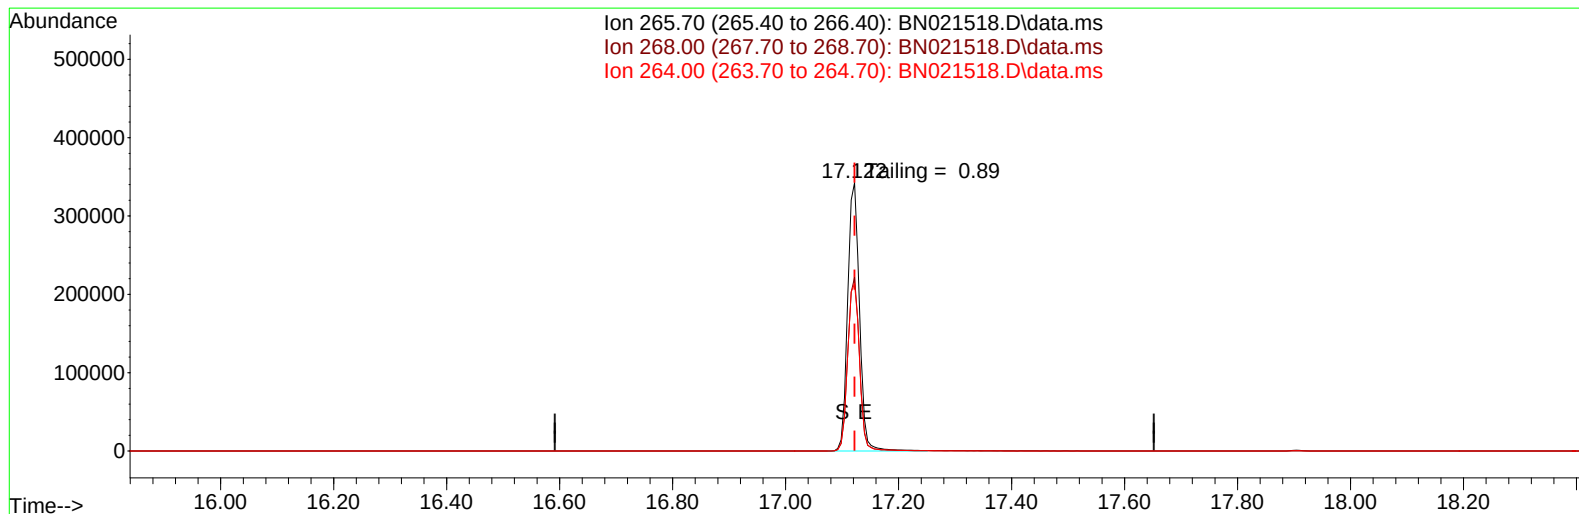

TIC: BN021518.D\data.ms

(70) Pentachlorophenol (C)

17.122min (0.000) 21889.07 ng




response 499536

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.71
264.00	61.60	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090122\
Data File : BN021518.D
Acq On : 01 Sep 2022 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 02 06:51:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 06:51:31 2022
Response via : Initial Calibration

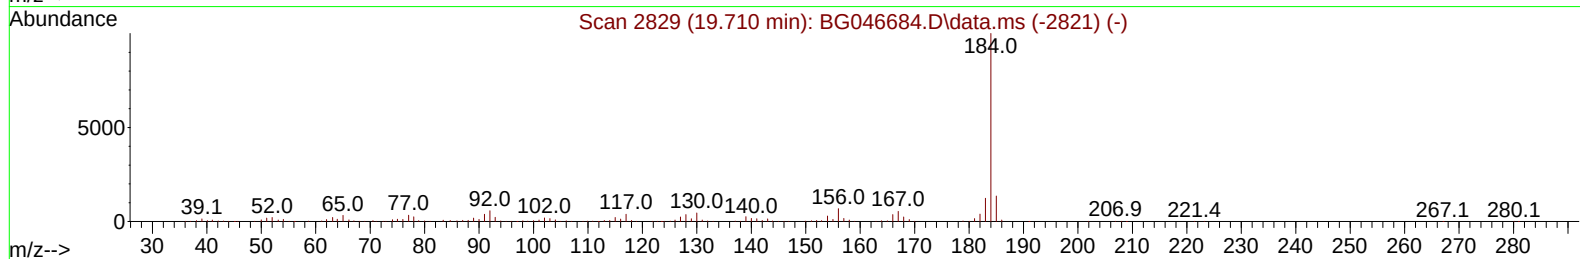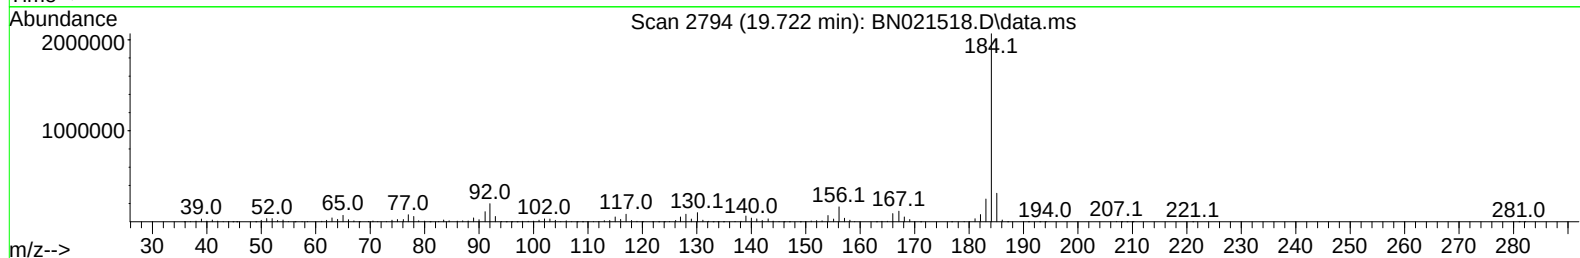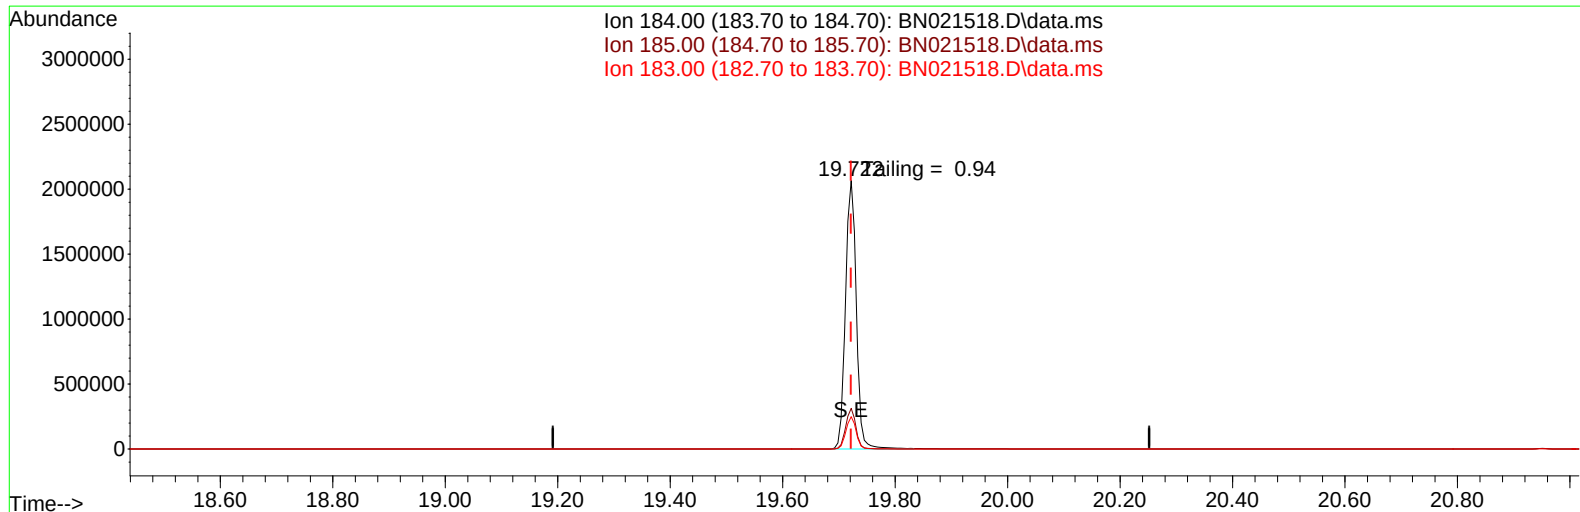

TIC: BN021518.D\data.ms

(77) Benzidine

19.722min (0.000) 0.00 ng

response 2783240

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.15
183.00	13.20	12.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/1/2022	BNA_N	<u>BN021518.D</u>
Compound Name	Response	Retention Time
DDT	1349663	20.951
DDD	18290	20.51
DDE	847	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19137	1368800	1.40

Instrument :
BNA_N
ClientSampleId :
DFTPP