
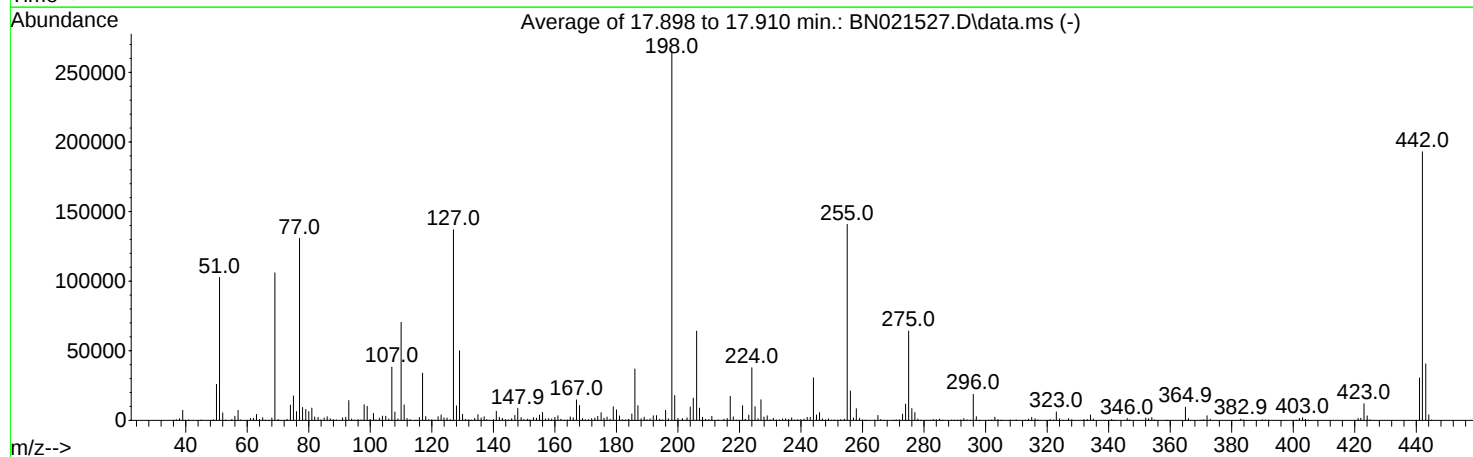


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090122\
 Data File : BN021527.D
 Acq On : 01 Sep 2022 16:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 00:53:31 2022

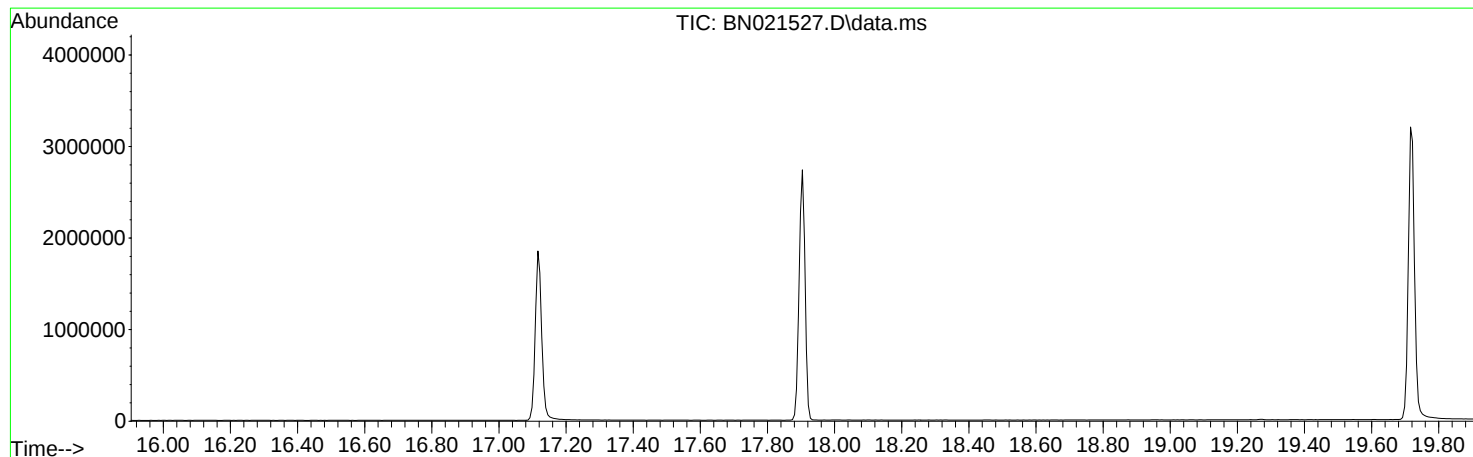




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	102632	PASS
68	69	0.00	2	1.6	1677	PASS
69	198	0.00	100	40.1	105925	PASS
70	69	0.00	2	0.5	515	PASS
127	198	10	80	51.8	136888	PASS
197	198	0.00	2	0.4	1153	PASS
198	198	100	100	100.0	264341	PASS
199	198	5	9	6.7	17782	PASS
275	198	10	60	24.2	64053	PASS
365	198	1	100	3.5	9354	PASS
441	198	0.01	100	11.5	30376	PASS
442	442	50	100	100.0	193024	PASS
443	442	15	24	21.0	40547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090122\
Data File : BN021527.D
Acq On : 01 Sep 2022 16:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 02 06:53:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 06:51:31 2022
Response via : Initial Calibration

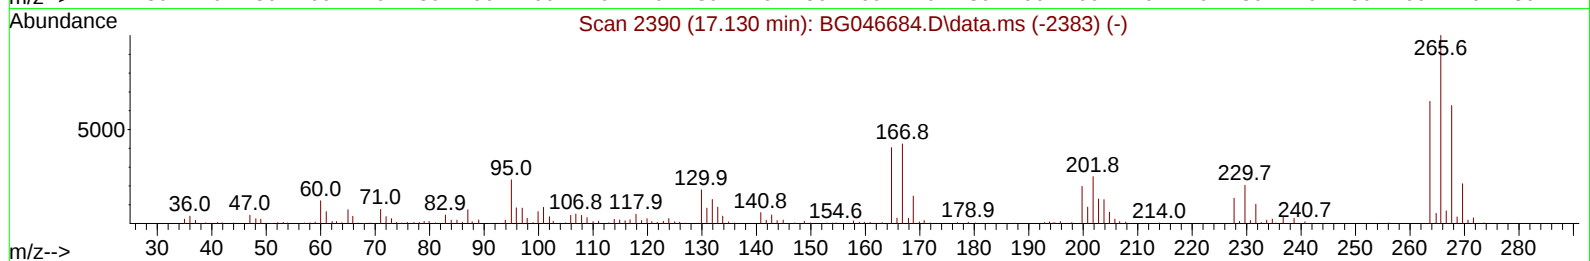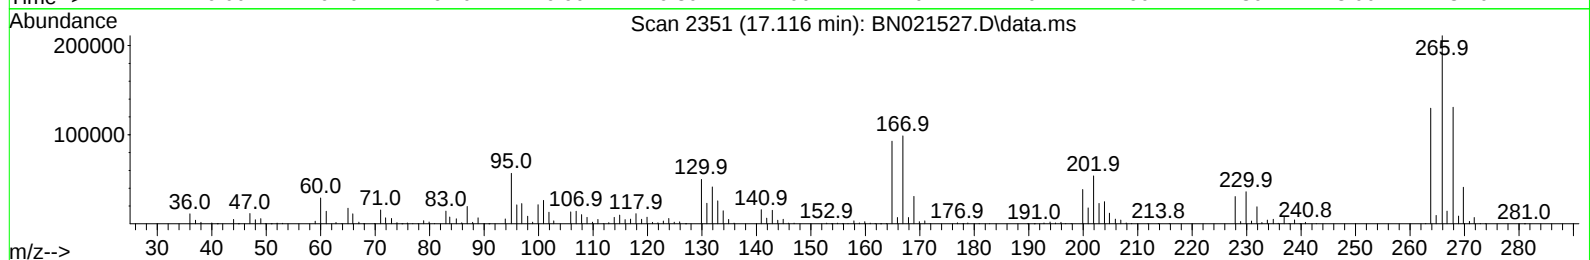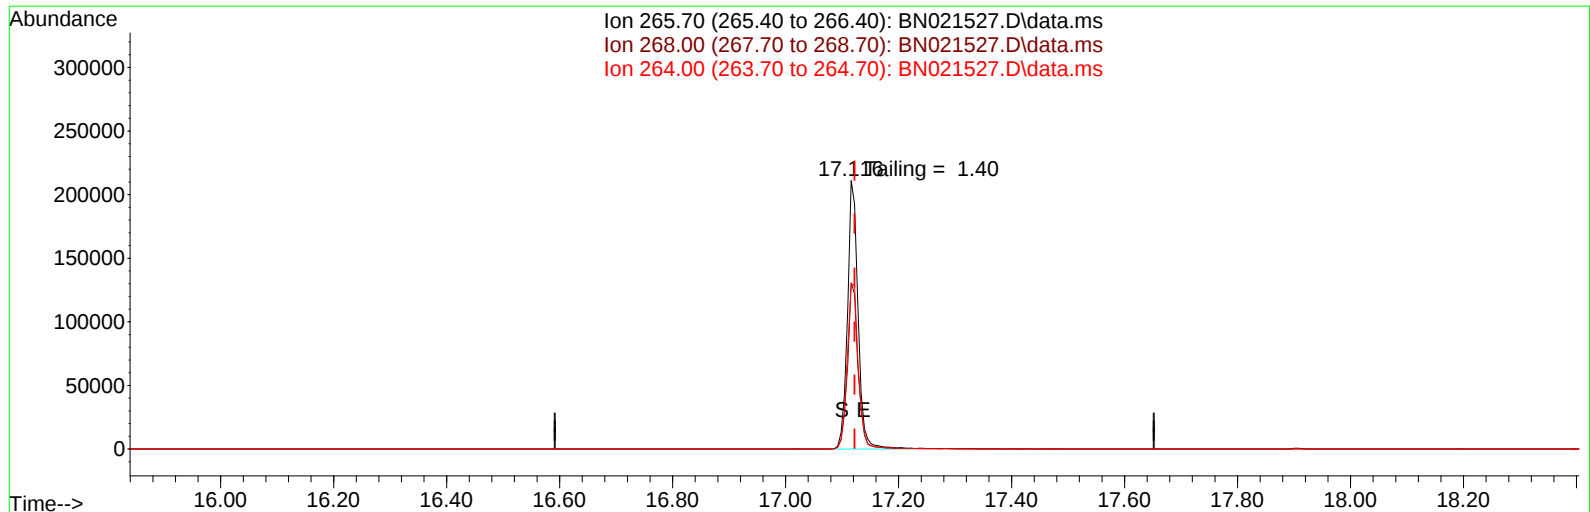

TIC: BN021527.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.006) 20735.15 ng




response 275004

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.96
264.00	61.60	61.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090122\
Data File : BN021527.D
Acq On : 01 Sep 2022 16:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 02 06:53:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 02 06:51:31 2022
Response via : Initial Calibration

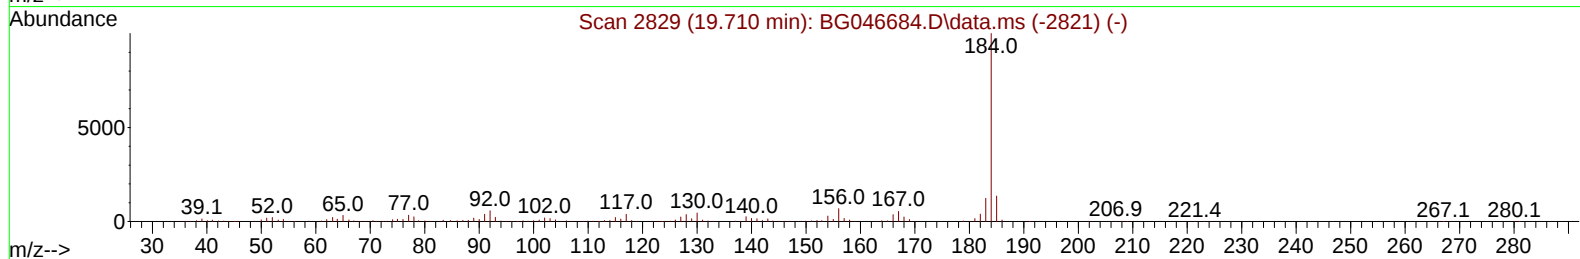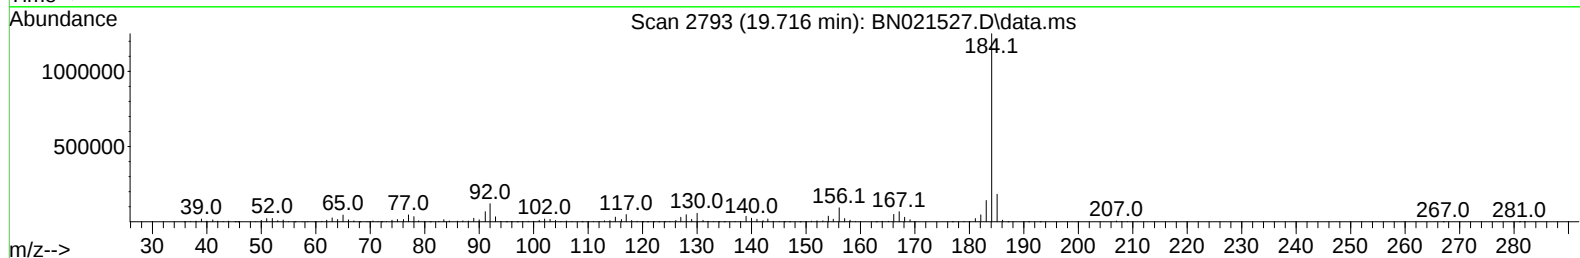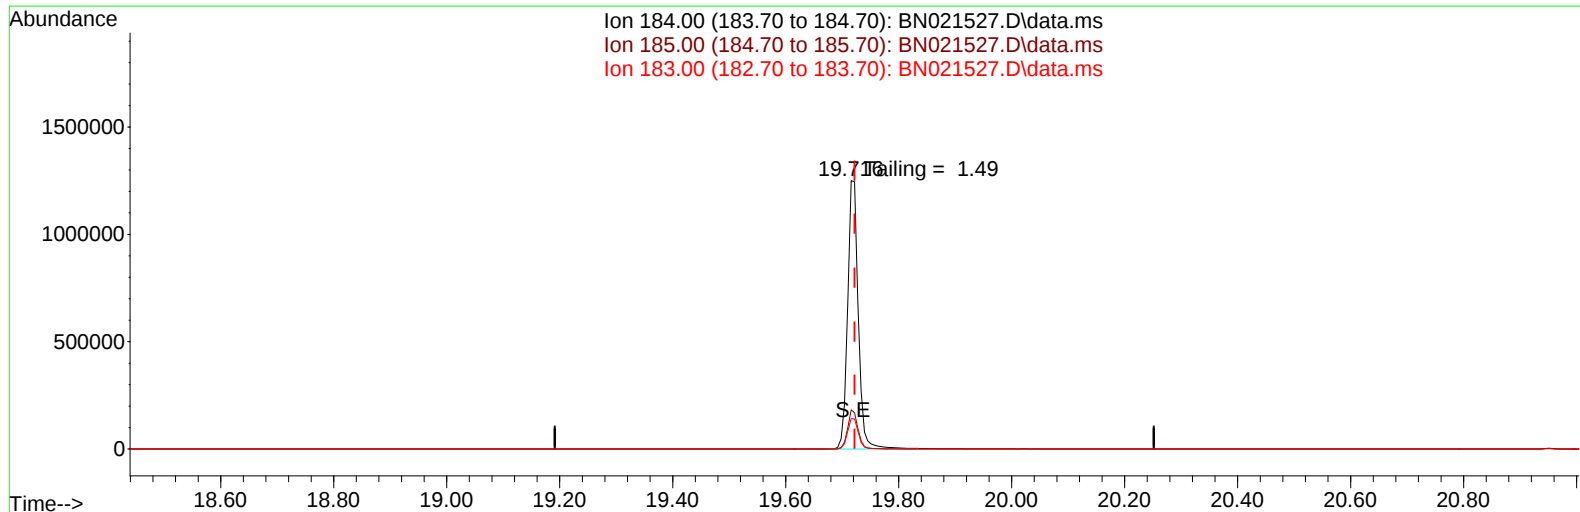

TIC: BN021527.D\data.ms

(77) Benzidine

19.716min (-0.006) 0.00 ng

response 1652228

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.65
183.00	13.20	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/1/2022	BNA_N	<u>BN021527.D</u>
Compound Name	Response	Retention Time
DDT	863617	20.951
DDD	11593	20.51
DDE	838	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12431	876048	1.42

Instrument :
BNA_N
ClientSampleId :
DFTPP