
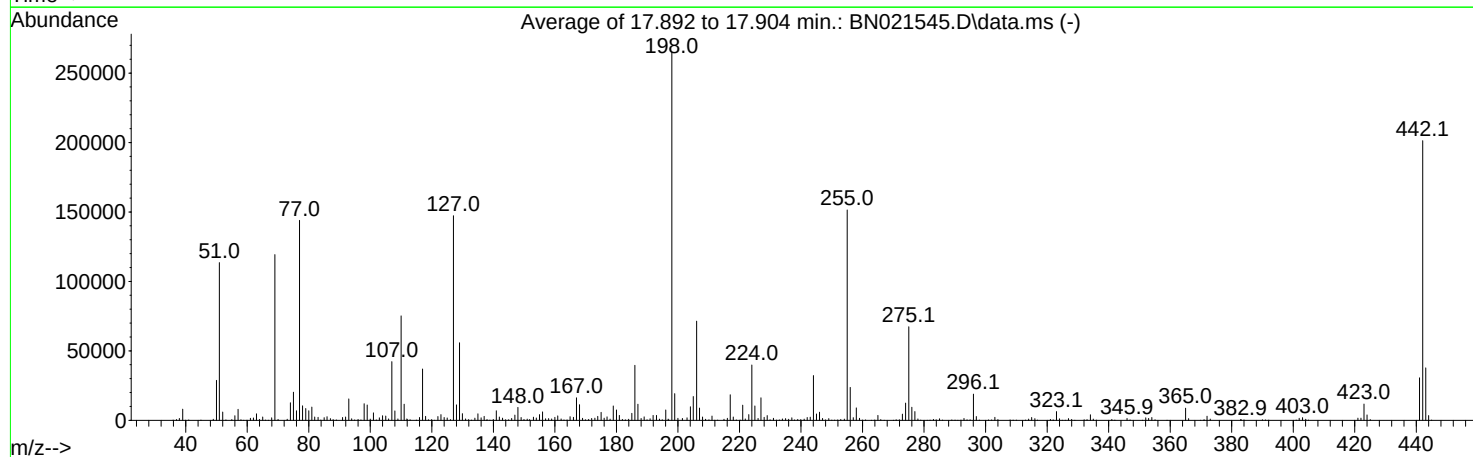


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN090122\  
 Data File : BN021545.D  
 Acq On : 02 Sep 2022 04:28  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN082922.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Sep 02 00:53:31 2022

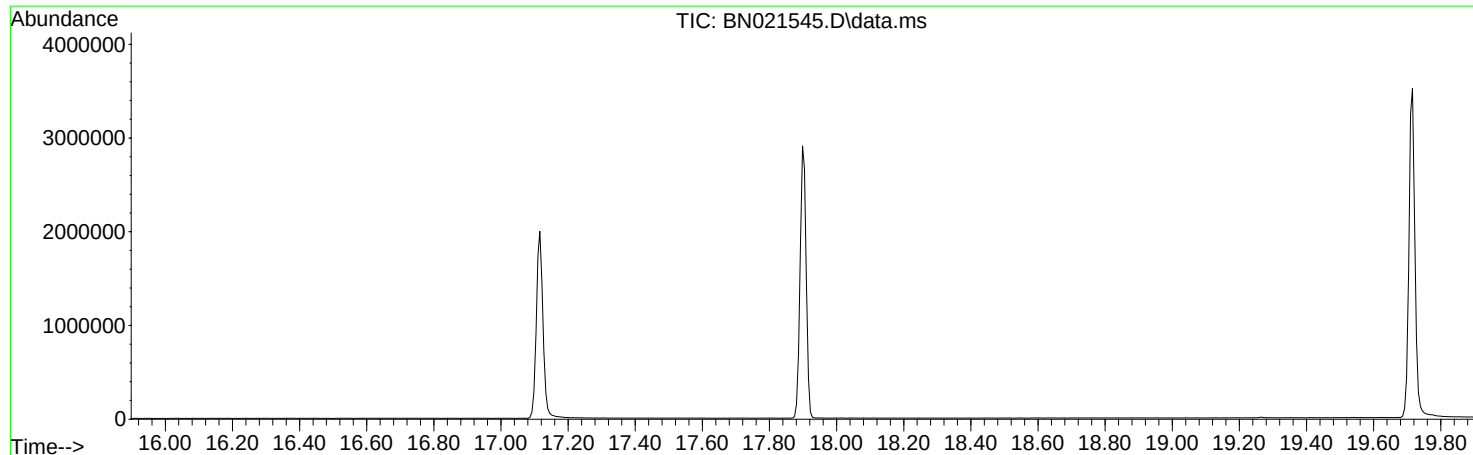




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 42.9         | 113527     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 1801       | PASS                |
| 69             | 198             | 0.00            | 100             | 45.1         | 119368     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 661        | PASS                |
| 127            | 198             | 10              | 80              | 55.6         | 147320     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 859        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 264896     | PASS                |
| 199            | 198             | 5               | 9               | 7.3          | 19205      | PASS                |
| 275            | 198             | 10              | 60              | 25.4         | 67357      | PASS                |
| 365            | 198             | 1               | 100             | 3.3          | 8666       | PASS                |
| 441            | 198             | 0.01            | 100             | 11.5         | 30552      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 201403     | PASS                |
| 443            | 442             | 15              | 24              | 18.7         | 37747      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN090122\  
 Data File : BN021545.D  
 Acq On : 02 Sep 2022 04:28  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Sep 02 06:54:37 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Sep 02 06:51:31 2022  
 Response via : Initial Calibration

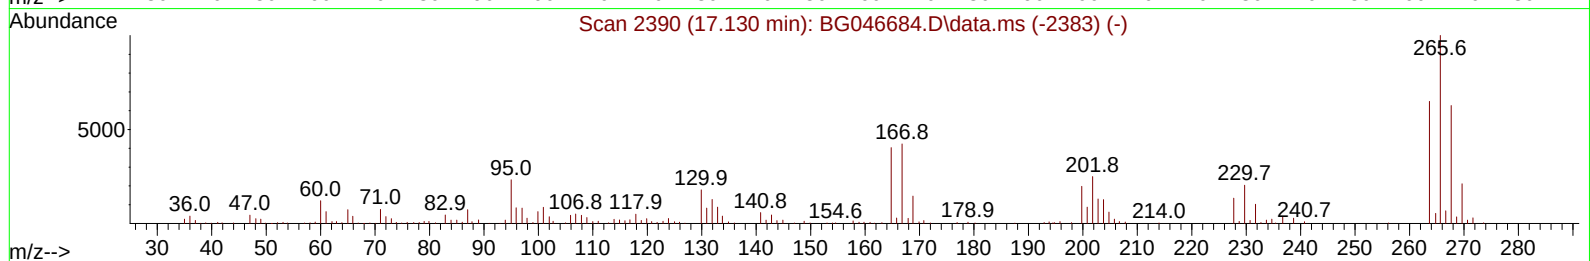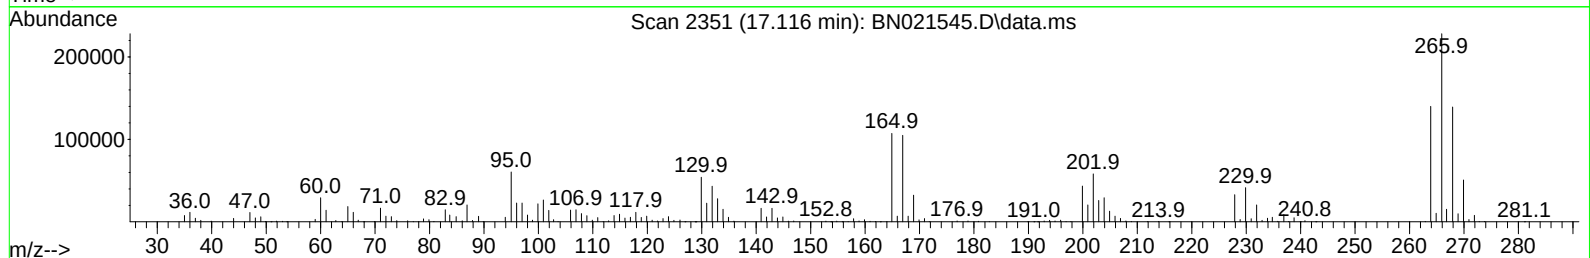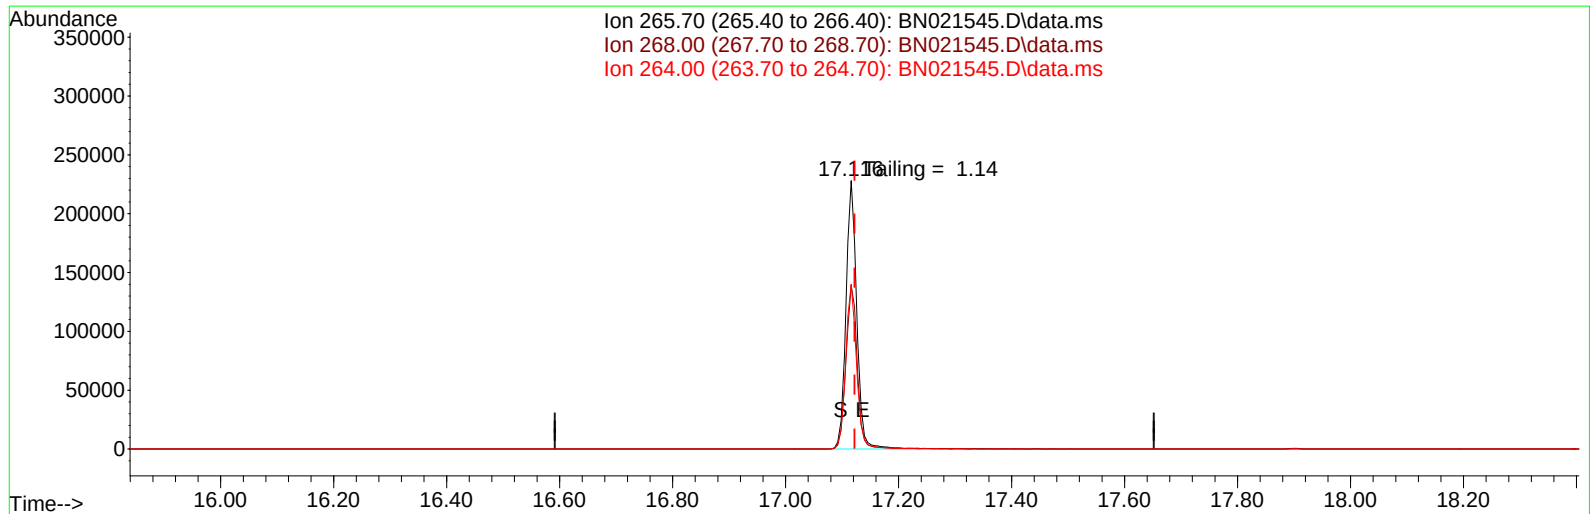

TIC: BN021545.D\data.ms

**(70) Pentachlorophenol (C)**

17.116min (-0.006) 20295.75 ng




response 301350

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 61.03  |
| 264.00 | 61.60  | 61.36  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN090122\  
Data File : BN021545.D  
Acq On : 02 Sep 2022 04:28  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Sep 02 06:54:37 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 02 06:51:31 2022  
Response via : Initial Calibration

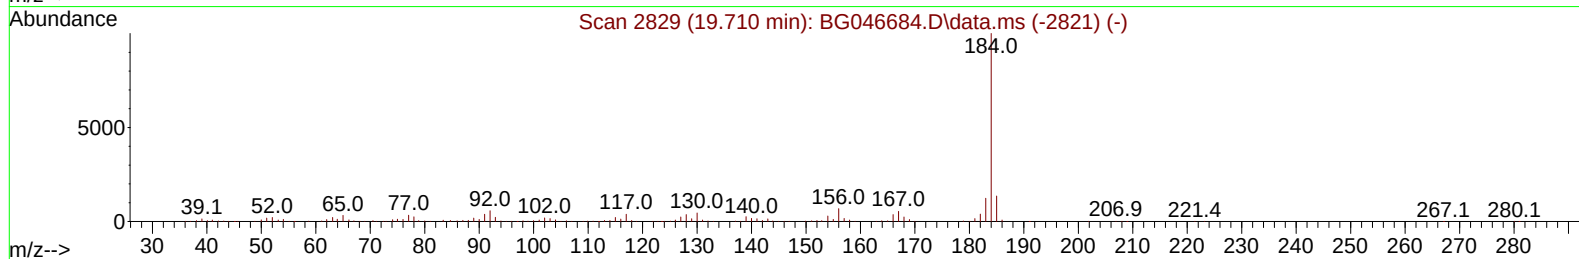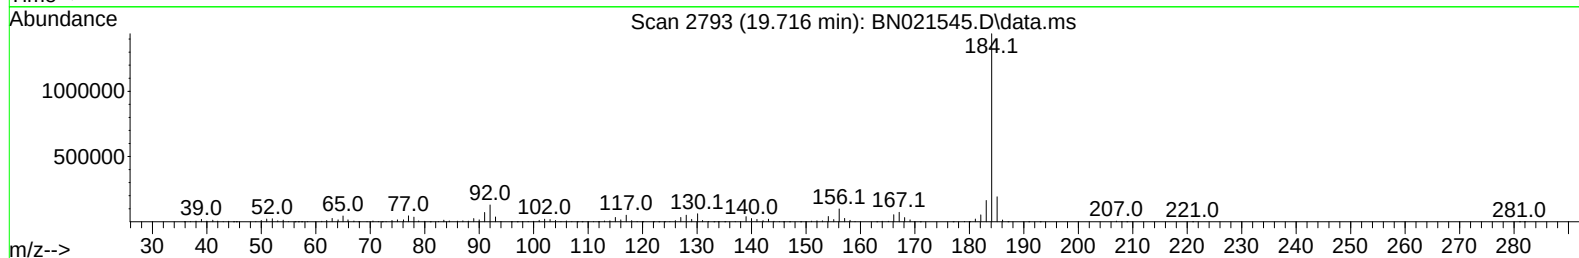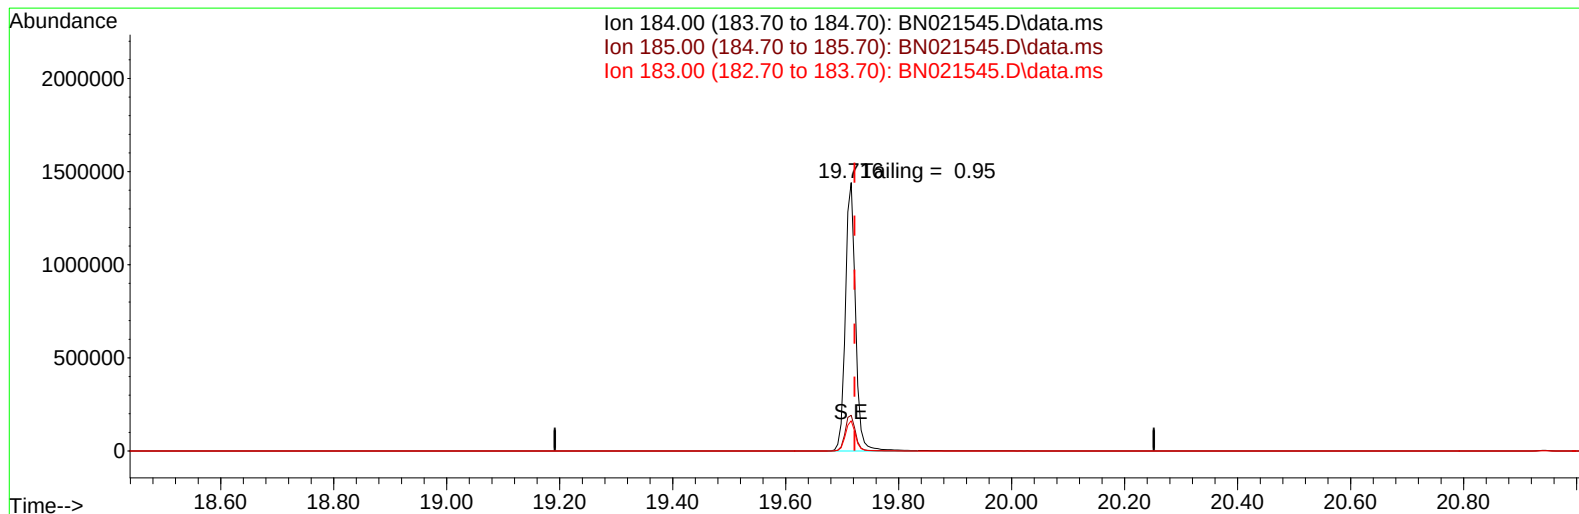

TIC: BN021545.D\data.ms

**(77) Benzidine**

19.716min (-0.006) 0.00 ng

response 1798157

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.29  |
| 183.00 | 13.20  | 11.29  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 9/1/2022      | BNA_N            | <u>BN021545.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 901959           | 20.945             |
| DDD           | 12199            | 20.504             |
| DDE           | 1019             | 19.992             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 13218         | 915177           | 1.44               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP