


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090320\
 Data File : BN011688.D
 Acq On : 03 Sep 2020 08:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 03 12:33:00 2020

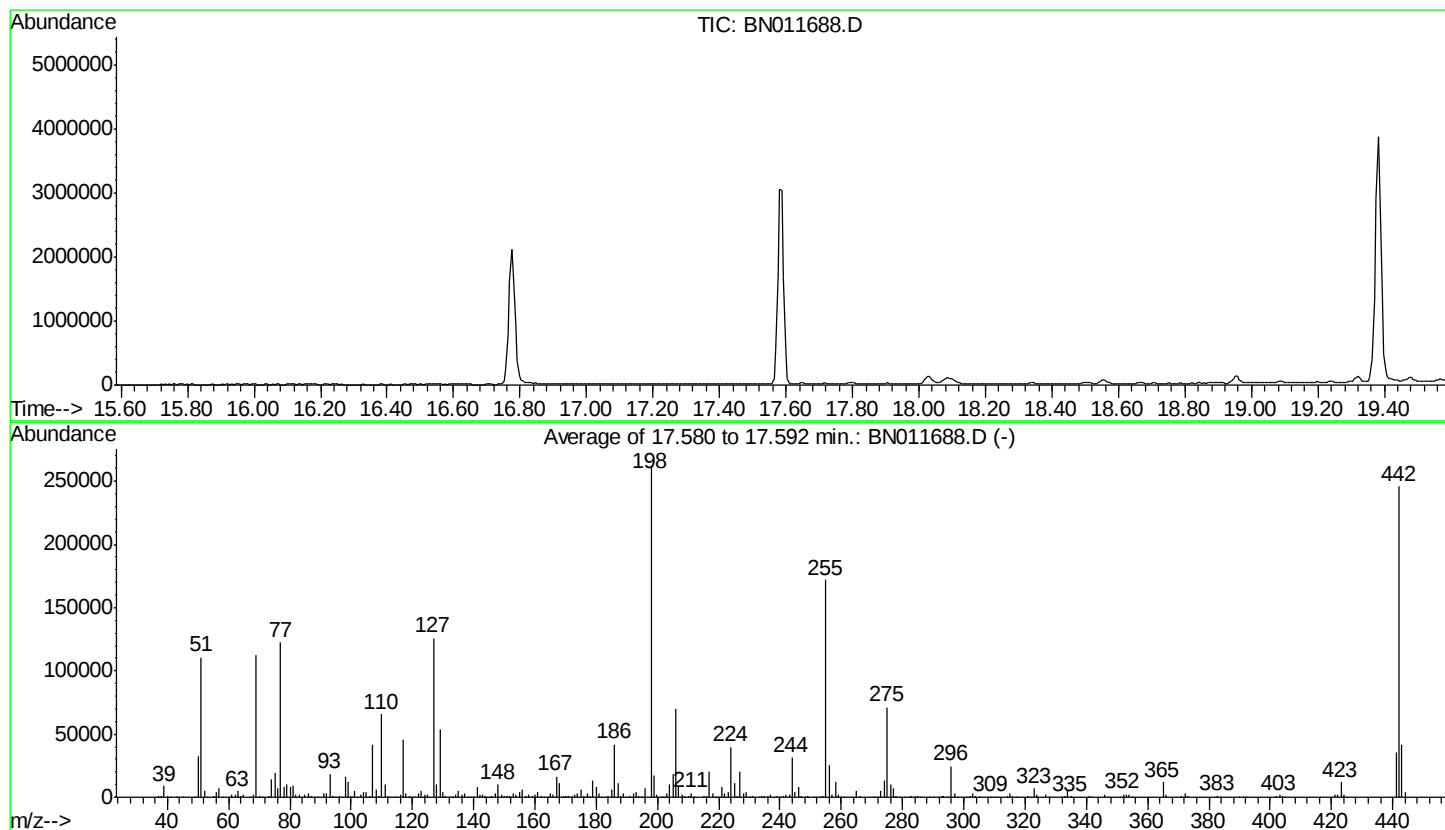

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	110767	PASS
68	69	0.00	2	2.0	2214	PASS
69	198	0.00	100	42.9	112532	PASS
70	69	0.00	2	0.6	695	PASS
127	198	10	80	48.0	126032	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	262314	PASS
199	198	5	9	6.7	17479	PASS
275	198	10	60	27.1	70965	PASS
365	198	1	100	4.5	11798	PASS
441	198	0.01	100	13.4	35125	PASS
442	198	50	100	93.7	245696	PASS
443	442	15	24	16.9	41536	PASS