

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
 Data File : BN033736.D
 Acq On : 03 Sep 2024 12:08
 Operator : MA/JU
 Sample : PB163096BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK096

Quant Time: Sep 04 01:40:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 01:39:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.523	152	4931	0.400	ng/ul	0.00
4) Naphthalene-d8	10.283	136	13503	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.160	164	6878	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.012	188	1106371	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.12
23) Perylene-d12	23.272	264	13814	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.135	96	39035	7.700	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.878	152	6774	0.350	ng/ul	0.00
18) Fluoranthene-d10	18.952	212	12495	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.169	88	239	0.042	ng/ul#	60
26) Benzo(a)pyrene	23.137	252	4768	0.111	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033736.D
Acq On : 03 Sep 2024 12:08
Operator : MA/JU
Sample : PB163096BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK096

Quant Time: Sep 04 01:40:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration




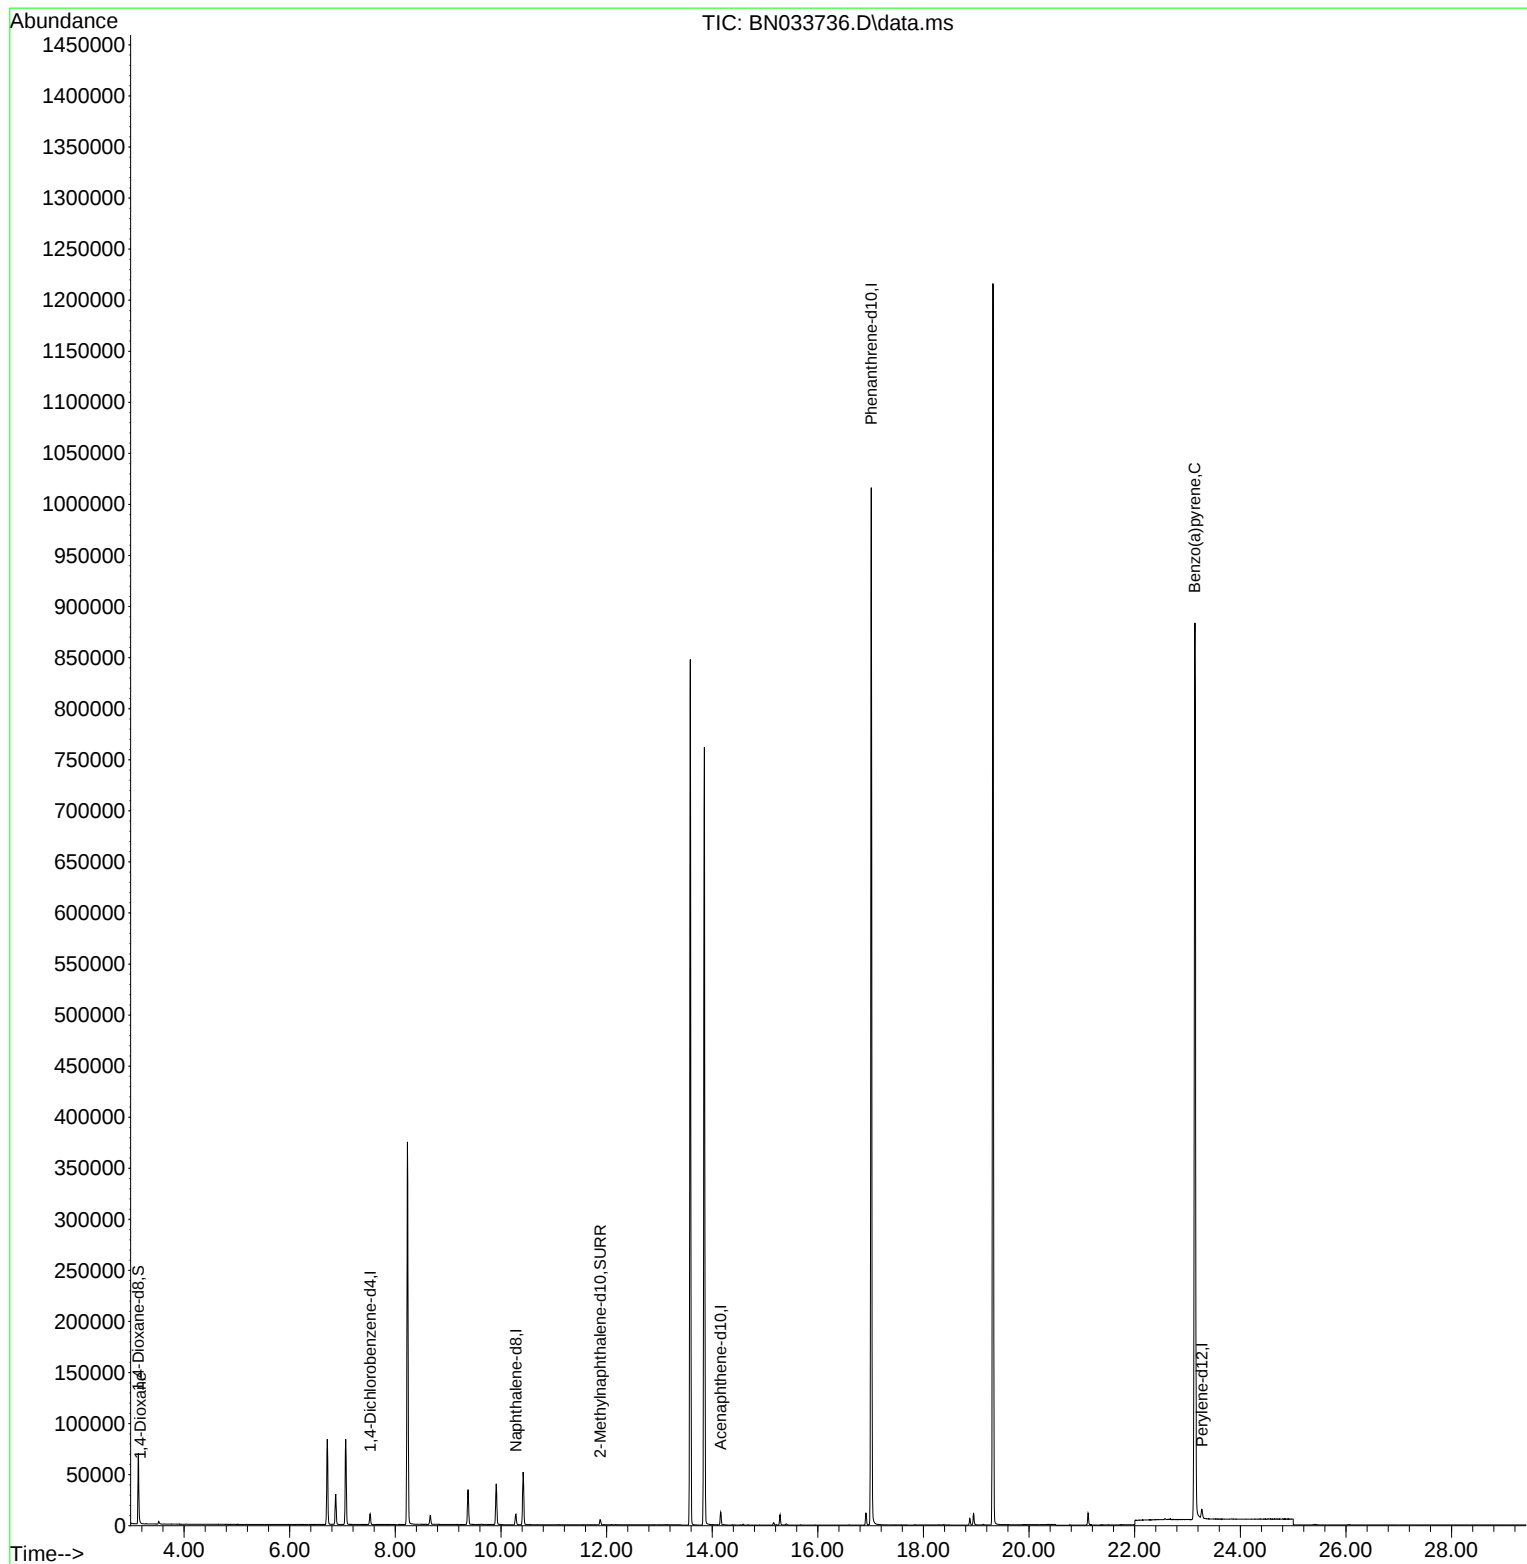


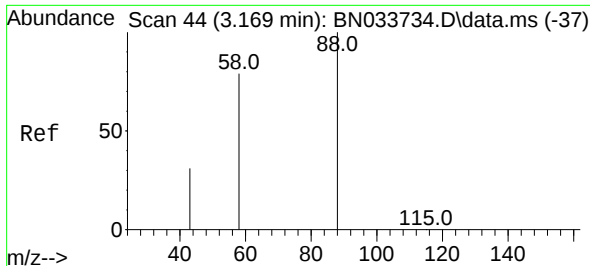

#2
1,4-Dioxane
Concen: 0.042 ng/ul
RT: 3.169 min Scan# 44
Delta R.T. -0.000 min
Lab File: BN033736.D
Acq: 03 Sep 2024 12:08

Instrument :
BNA_N
ClientSampleId :
SBLK096

Tgt Ion: 88 Resp: 239
Ion Ratio Lower Upper
88 100
43 91.2 47.0 70.4#
58 37.5 53.0 79.4#

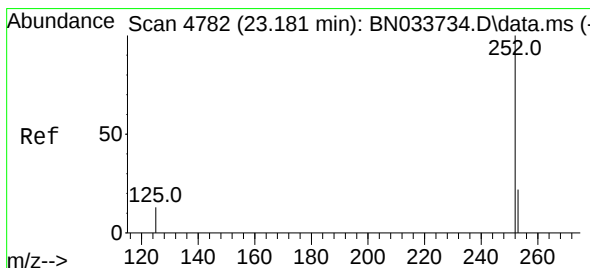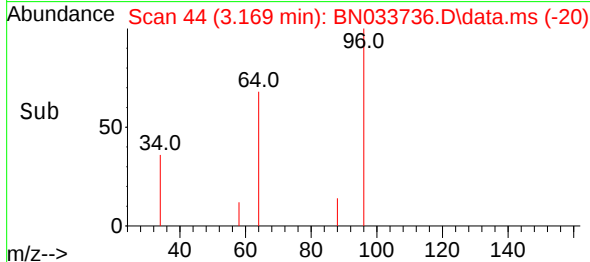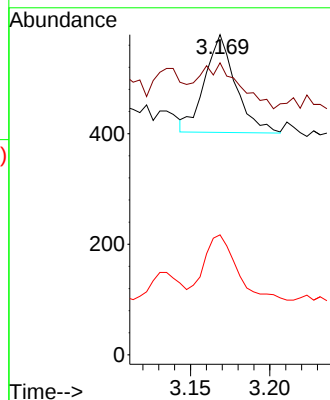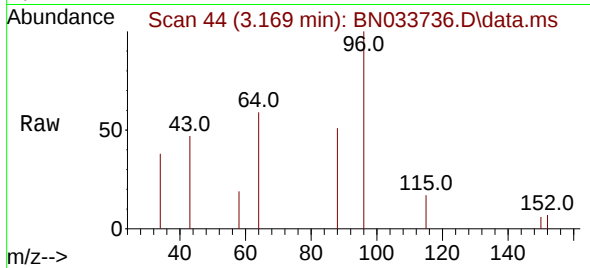

#26
Benzo(a)pyrene
Concen: 0.111 ng/ul
RT: 23.137 min Scan# 4767
Delta R.T. -0.044 min
Lab File: BN033736.D
Acq: 03 Sep 2024 12:08

Tgt Ion: 252 Resp: 4768
Ion Ratio Lower Upper
252 100
253 47.2 22.8 34.2#
125 48.7 18.0 27.0#

