

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033740.D
Acq On : 03 Sep 2024 14:33
Operator : MA/JU
Sample : P3809-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YE3F0

Quant Time: Sep 04 01:41:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.523	152	6473	0.400	ng/ul	0.00
4) Naphthalene-d8	10.283	136	16109	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.160	164	8498	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.012	188	1376095	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.12
23) Perylene-d12	23.275	264	17136	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.135	96	31178	4.685	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.878	152	7803	0.338	ng/ul	0.00
18) Fluoranthene-d10	18.952	212	17804	0.000	ng/ul	0.00
Target Compounds						Qvalue
26) Benzo(a)pyrene	23.140	252	5061	0.095	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033740.D
Acq On : 03 Sep 2024 14:33
Operator : MA/JU
Sample : P3809-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YE3F0

Quant Time: Sep 04 01:41:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

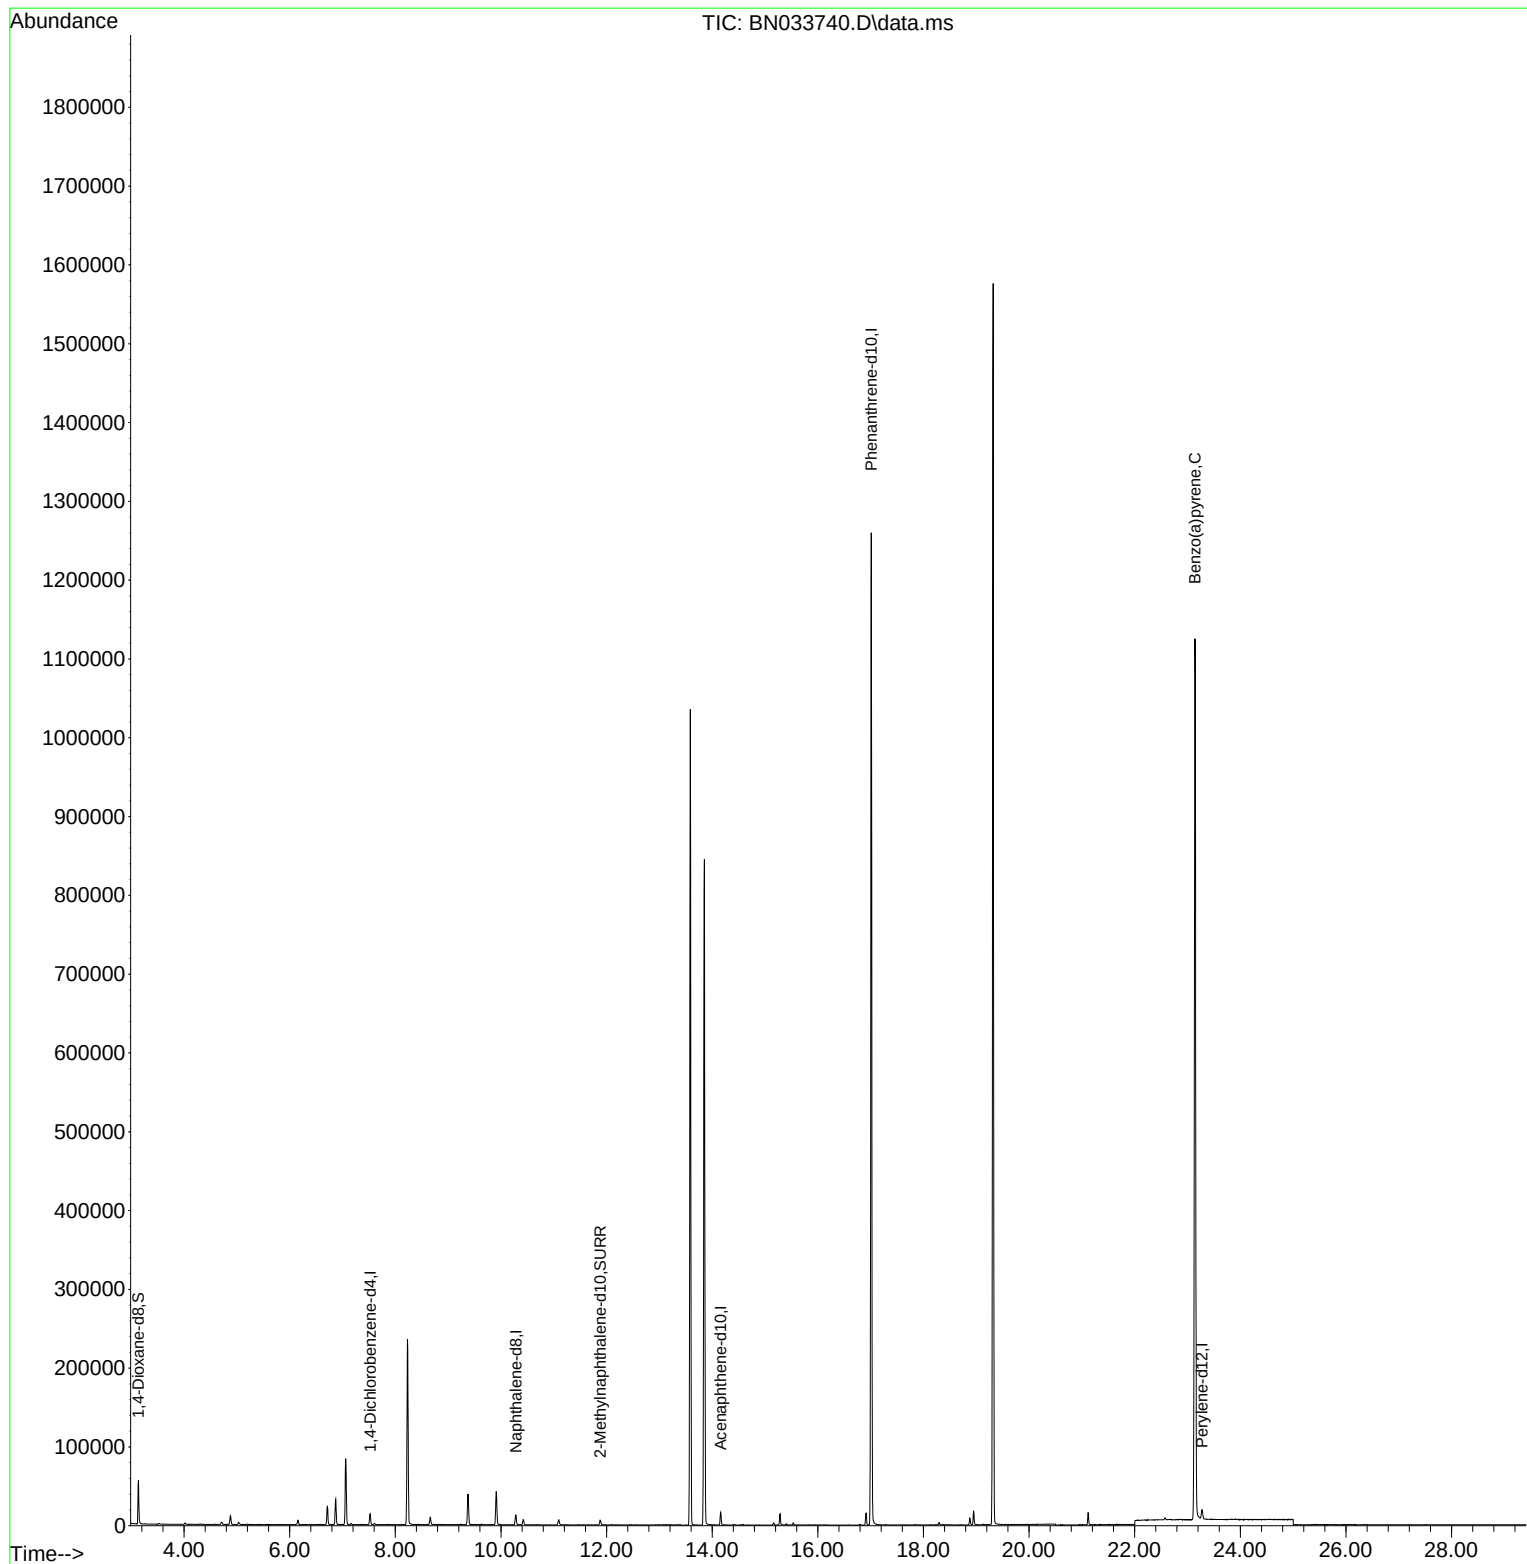

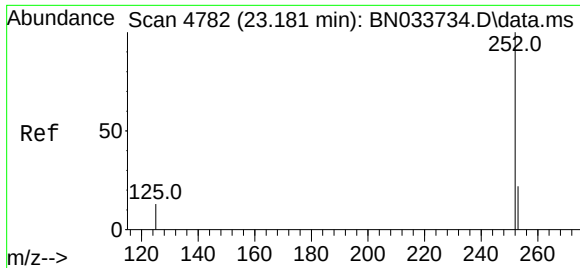

#26

Benzo(a)pyrene

Concen: 0.095 ng/ul

RT: 23.140 min Scan# 41

Delta R.T. -0.041 min

Lab File: BN033740.D


Acq: 03 Sep 2024 14:33

Instrument :

BNA_N

ClientSampleId :

YE3F0

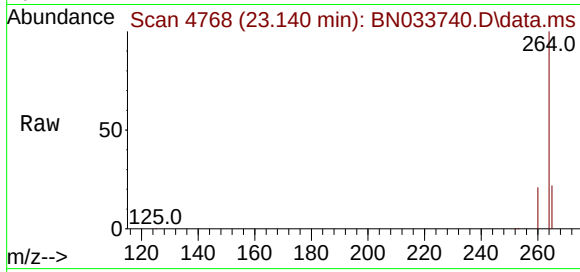

Tgt Ion:252 Resp: 5061

Ion Ratio Lower Upper

252 100

253 46.1 22.8 34.2#

125 49.0 18.0 27.0#

