

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
 Data File : BN033741.D
 Acq On : 03 Sep 2024 15:09
 Operator : MA/JU
 Sample : P3809-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YE3F1

Quant Time: Sep 04 01:41:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 01:39:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.523	152	6432	0.400	ng/ul	0.00
4) Naphthalene-d8	10.283	136	15412	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.160	164	7993	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.012	188	1304947	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.12
23) Perylene-d12	23.278	264	16919	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.135	96	29723	4.495	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.878	152	7468	0.338	ng/ul	0.00
18) Fluoranthene-d10	18.952	212	17076	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.164	166	2414	0.082	ng/ul#	17
26) Benzo(a)pyrene	23.143	252	5079	0.096	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033741.D
Acq On : 03 Sep 2024 15:09
Operator : MA/JU
Sample : P3809-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YE3F1

Quant Time: Sep 04 01:41:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

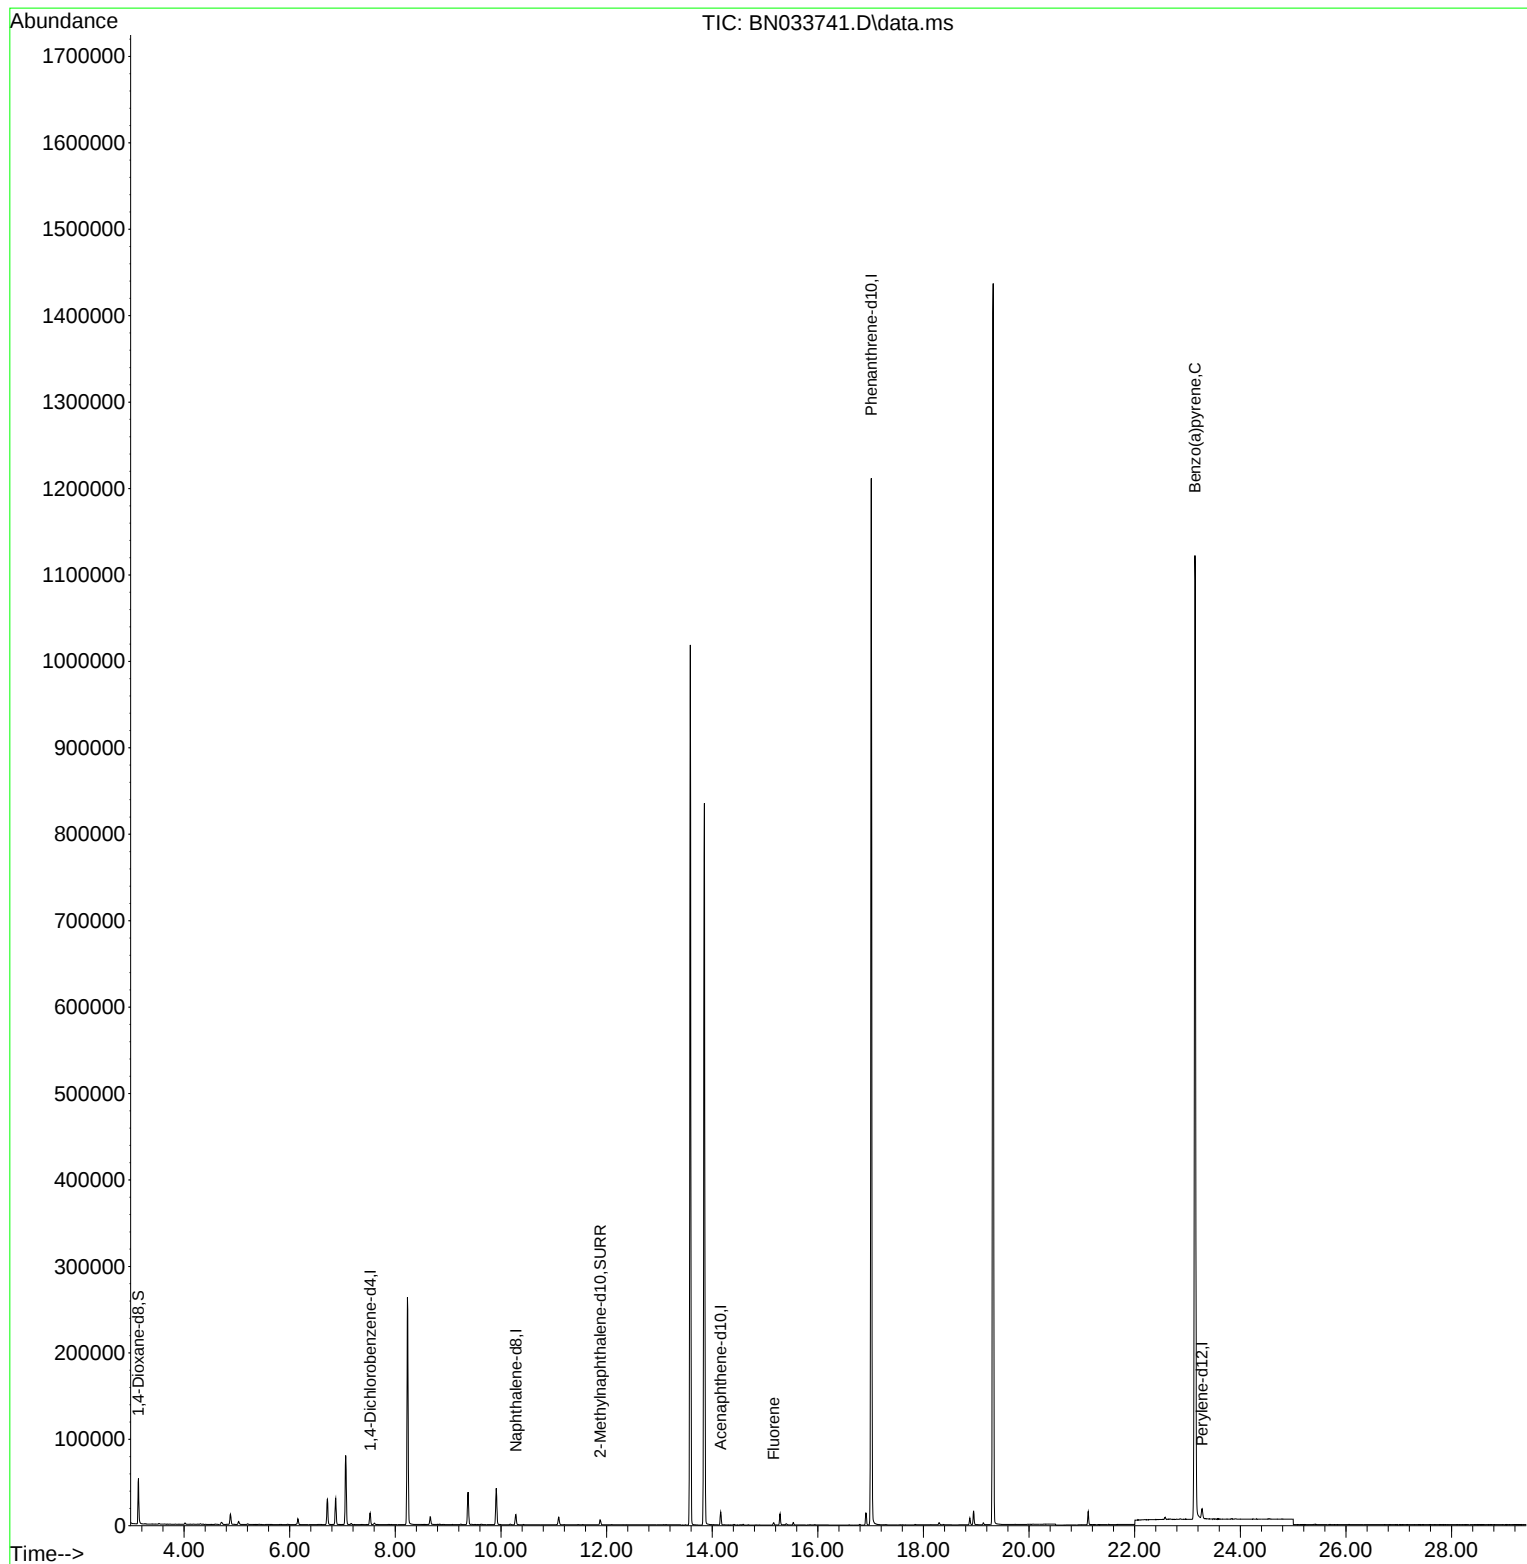

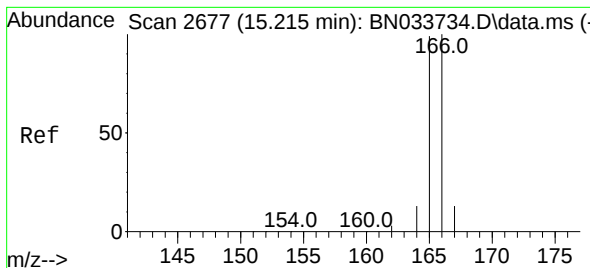

#12

Fluorene

Concen: 0.082 ng/ul

RT: 15.164 min Scan# 2

Delta R.T. -0.051 min

Lab File: BN033741.D

Acq: 03 Sep 2024 15:09

Instrument :

BNA_N

ClientSampleId :

YE3F1





Tgt Ion:166 Resp: 2414

Ion Ratio Lower Upper

166 100

165 11.6 79.1 118.7#

167 35.0 11.4 17.0#

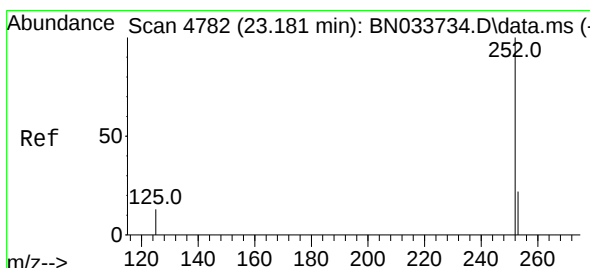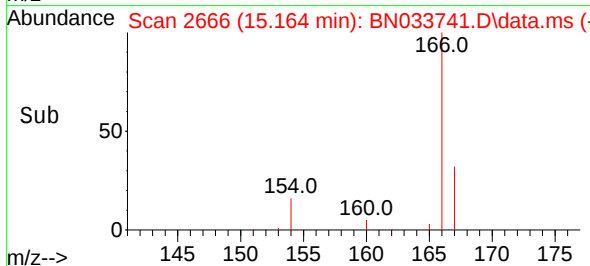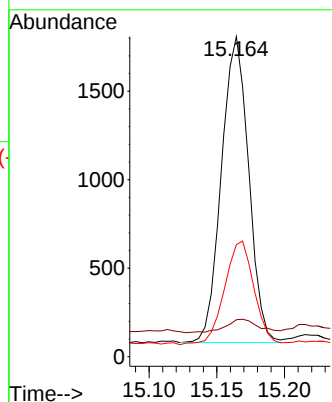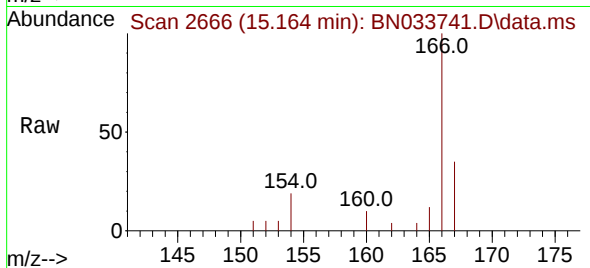

#26

Benzo(a)pyrene

Concen: 0.096 ng/ul

RT: 23.143 min Scan# 4769

Delta R.T. -0.038 min

Lab File: BN033741.D

Acq: 03 Sep 2024 15:09

Tgt Ion:252 Resp: 5079

Ion Ratio Lower Upper

252 100

253 46.4 22.8 34.2#

125 47.8 18.0 27.0#

