

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
 Data File : BN033742.D
 Acq On : 03 Sep 2024 15:45
 Operator : MA/JU
 Sample : P3809--08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YE3E3

Quant Time: Sep 04 01:41:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 01:39:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.523	152	6246	0.400	ng/ul	0.00
4) Naphthalene-d8	10.283	136	17222	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.160	164	9135	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.011	188	1592984	0.400	ng/ul	0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.12
23) Perylene-d12	23.277	264	20225	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.135	96	36538	5.690	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.877	152	9080	0.367	ng/ul	0.00
18) Fluoranthene-d10	18.952	212	21018	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.164	88	55014	7.721	ng/ul#	75
26) Benzo(a)pyrene	23.146	252	6395	0.101	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033742.D
Acq On : 03 Sep 2024 15:45
Operator : MA/JU
Sample : P3809--08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YE3E3

Quant Time: Sep 04 01:41:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

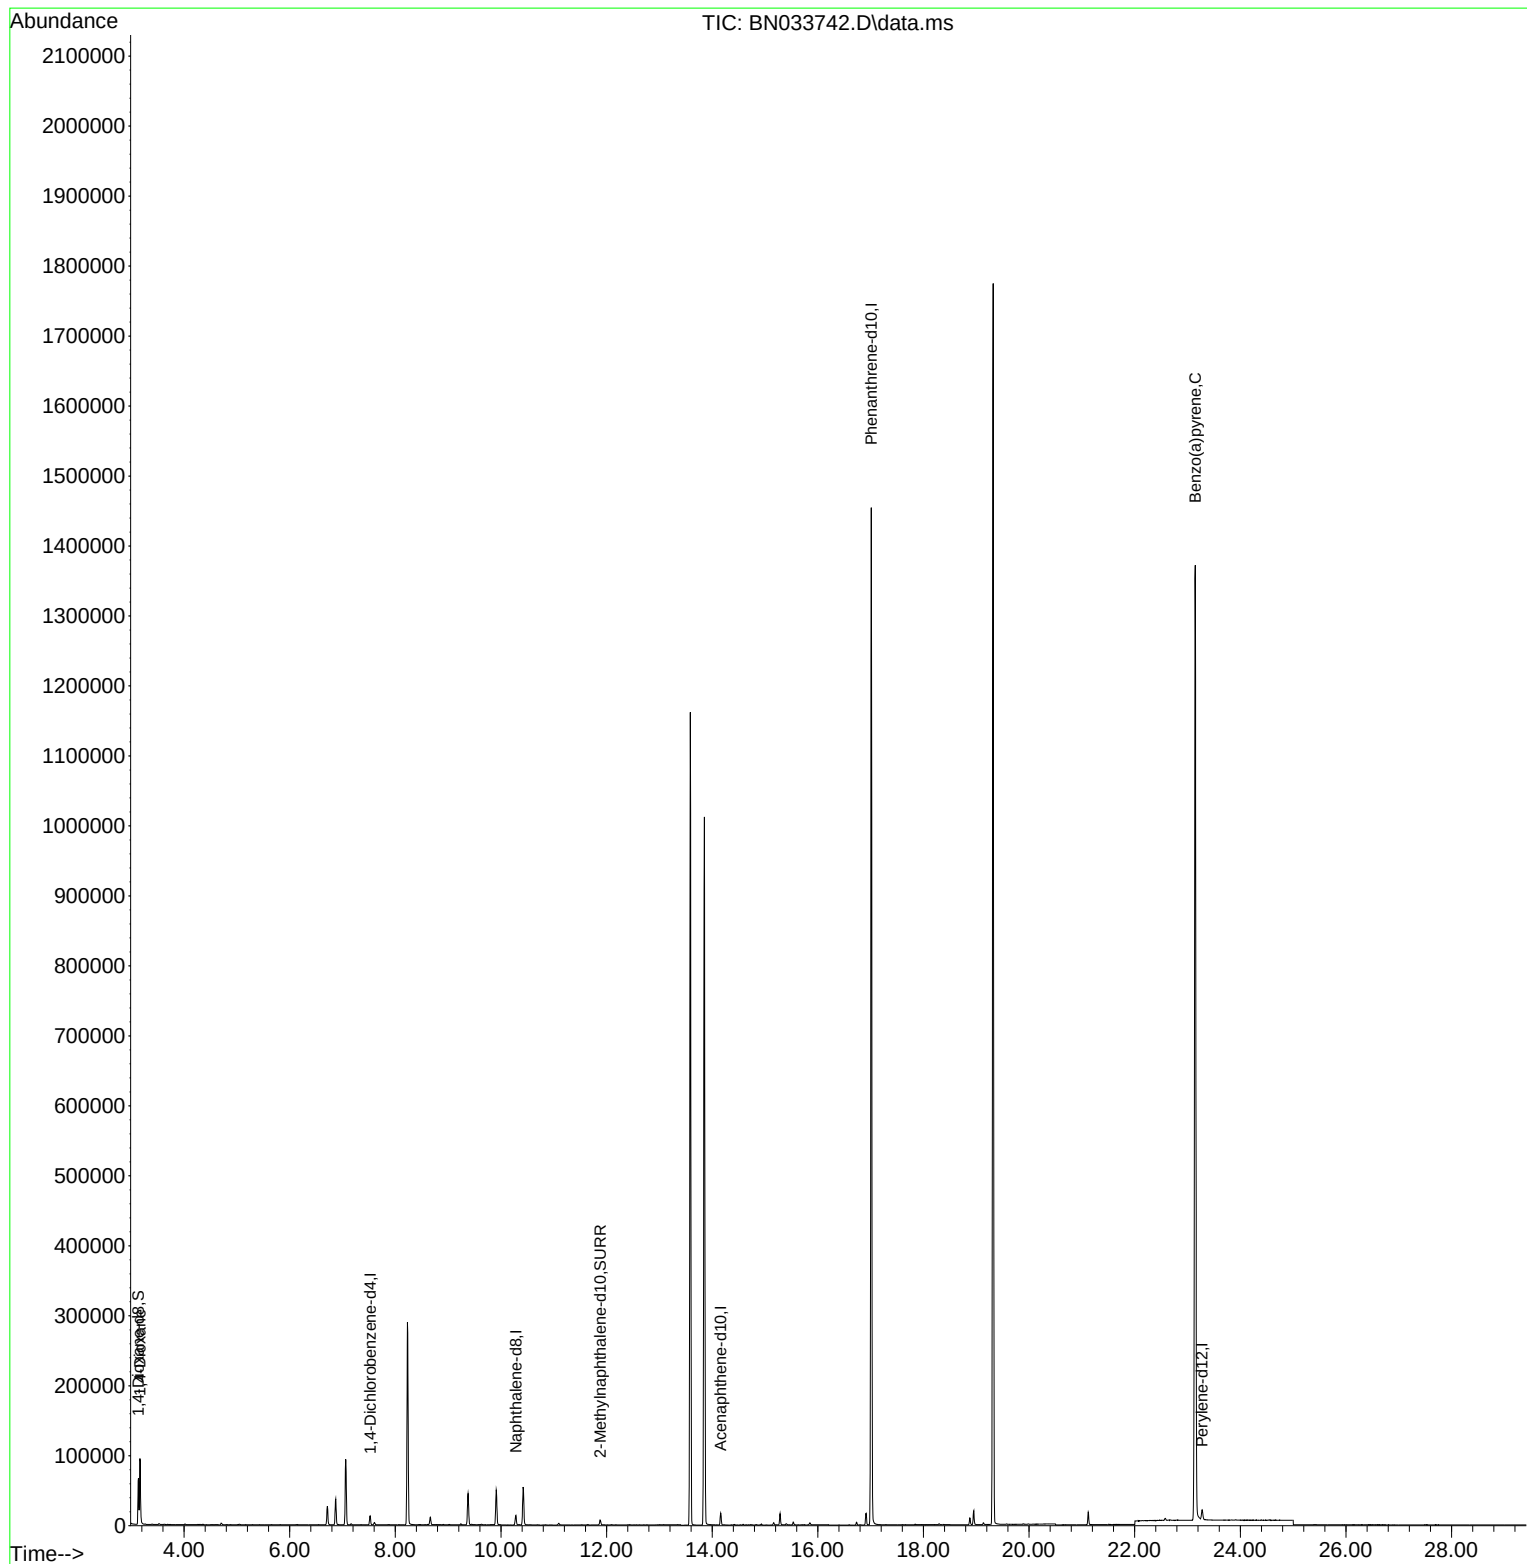

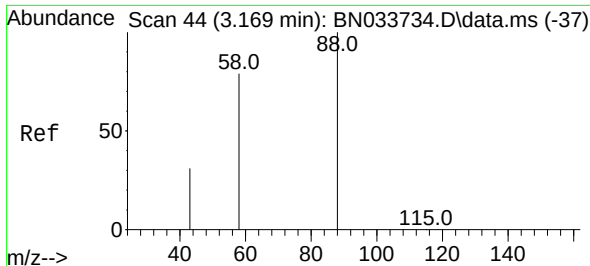

#2

1,4-Dioxane

Concen: 7.721 ng/ul

RT: 3.164 min Scan# 41

Delta R.T. -0.004 min

Lab File: BN033742.D

Acq: 03 Sep 2024 15:45

Instrument :

BNA_N

ClientSampleId :

YE3E3





Tgt Ion: 88 Resp: 55014

Ion Ratio Lower Upper

88 100

43 33.5 47.0 70.4#

58 79.5 53.0 79.4#

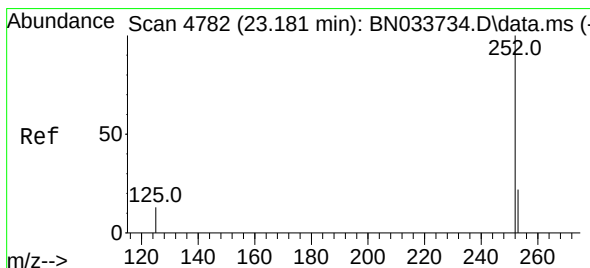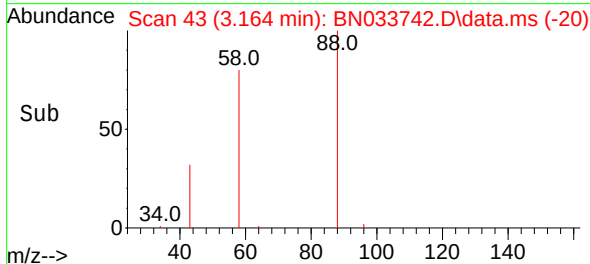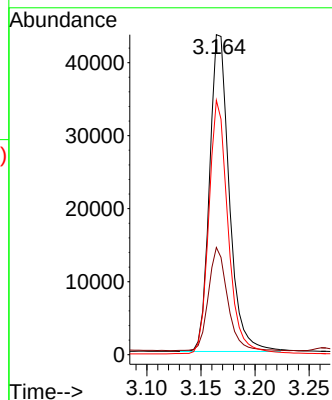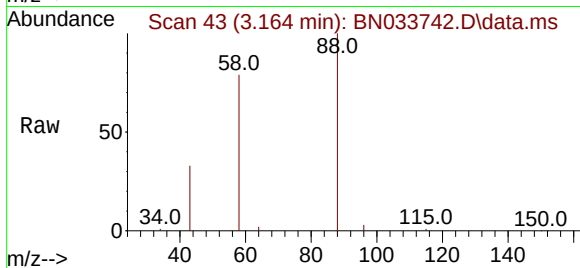

#26

Benzo(a)pyrene

Concen: 0.101 ng/ul

RT: 23.146 min Scan# 4770

Delta R.T. -0.035 min

Lab File: BN033742.D

Acq: 03 Sep 2024 15:45

Tgt Ion: 252 Resp: 6395

Ion Ratio Lower Upper

252 100

253 42.8 22.8 34.2#

125 44.3 18.0 27.0#

