




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033735.D
Acq On : 03 Sep 2024 11:32
Operator : MA/JU
Sample : PB163093BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/06/2024

Quant Time: Sep 04 01:47:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

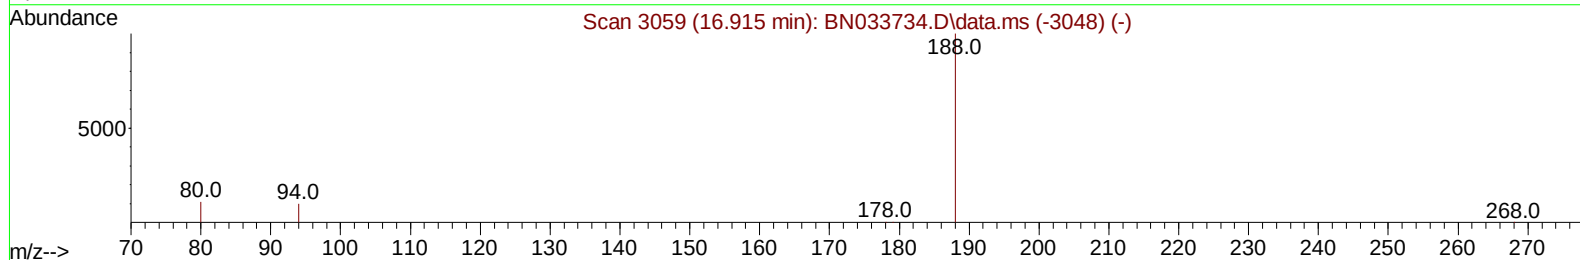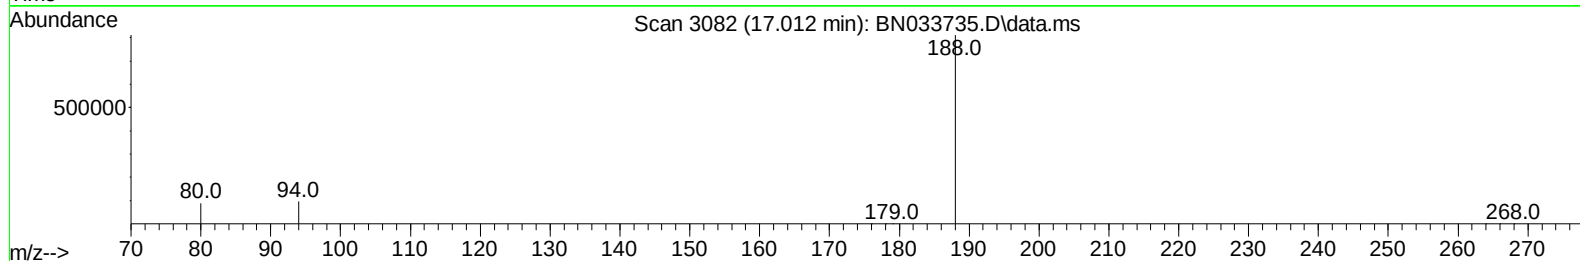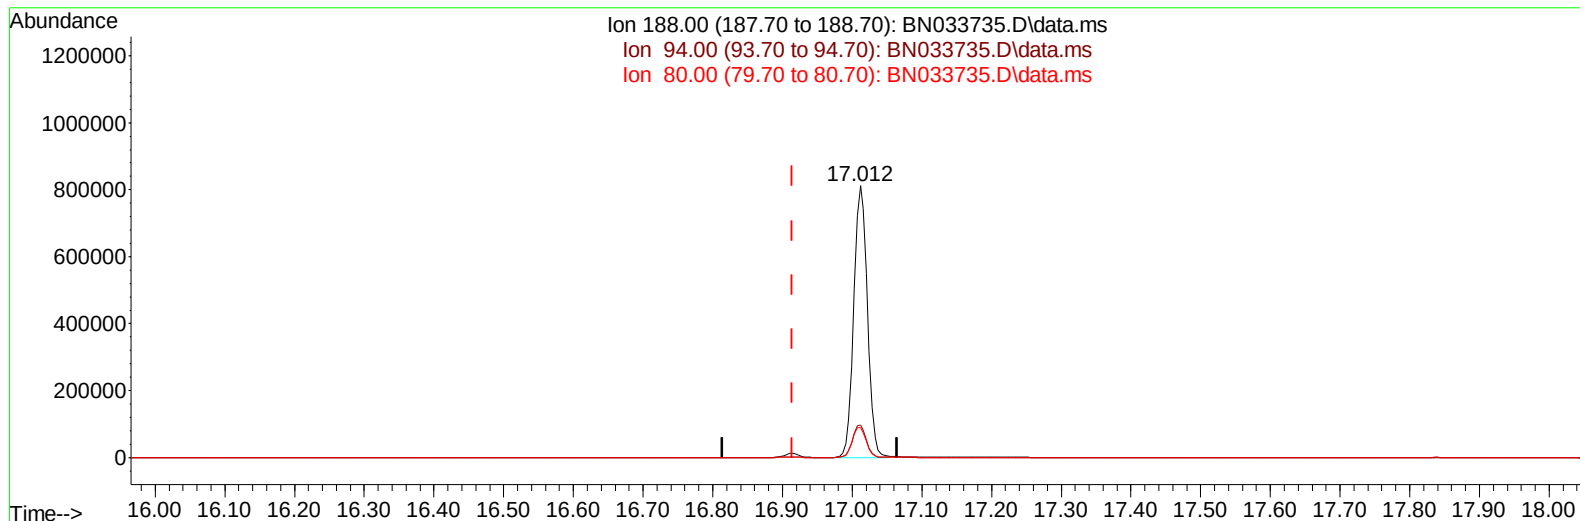

TIC: BN033735.D\data.ms

(13) Phenanthrene-d10 (I)

17.012min (+ 0.097) 0.40 ng/u1

response 1100127

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	11.87
80.00	11.50	11.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033735.D
Acq On : 03 Sep 2024 11:32
Operator : MA/JU
Sample : PB163093BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Manual IntegrationsAPPROVED

Quant Time: Sep 04 01:47:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/06/2024

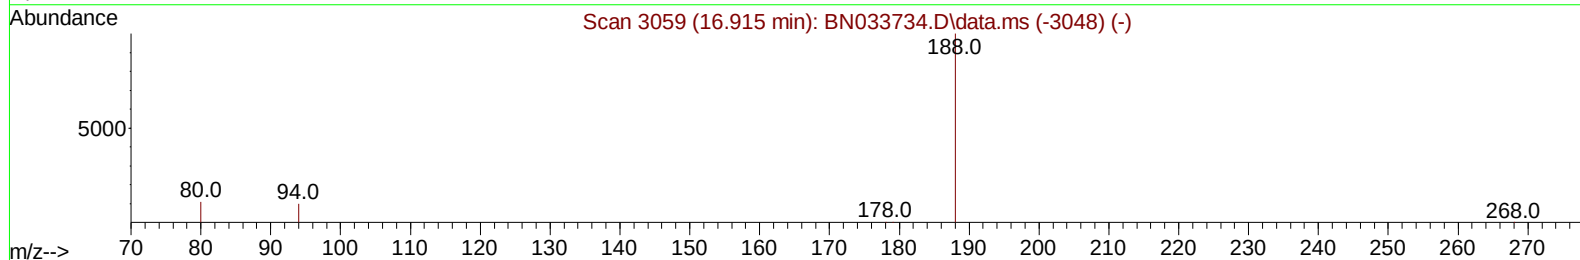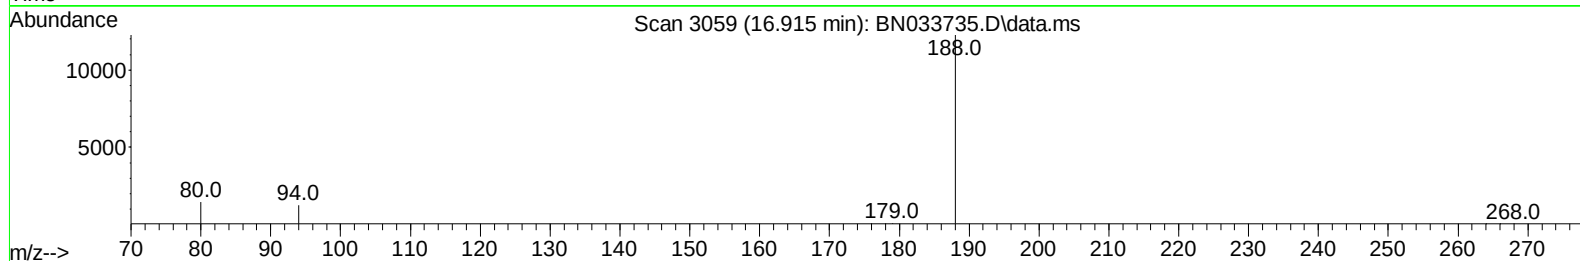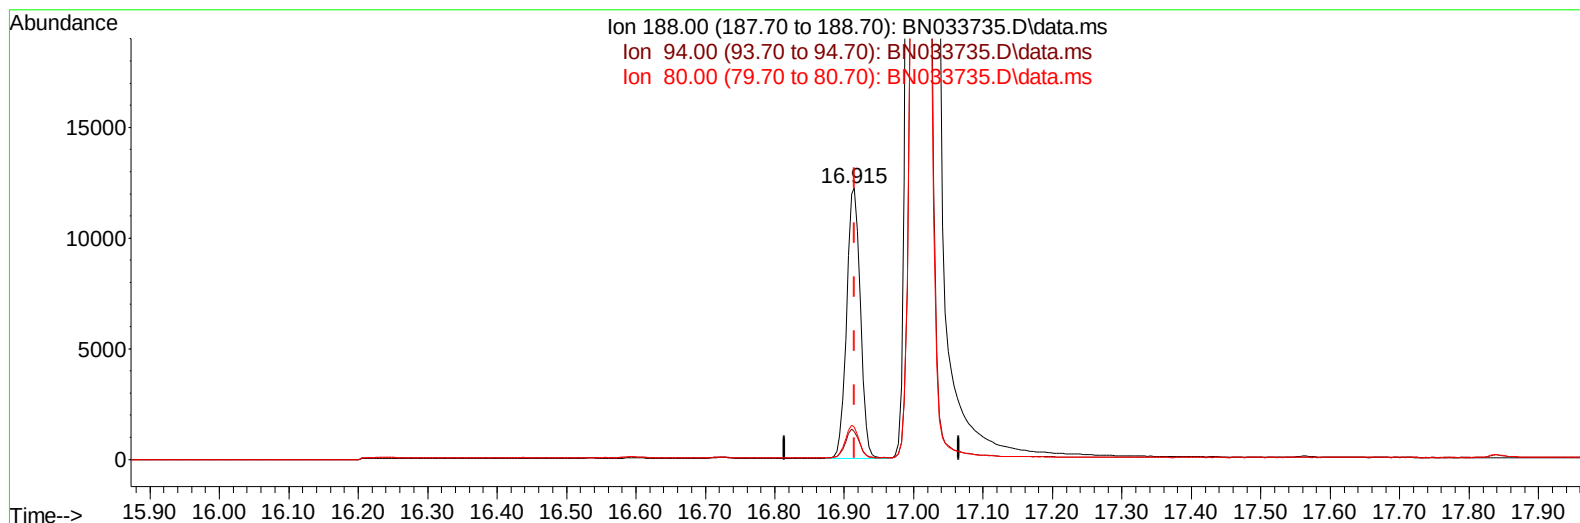

TIC: BN033735.D\data.ms

(13) Phenanthrene-d10 (I)

16.915min (0.000) 0.40 ng/ul m

response 16657

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	10.35
80.00	11.50	11.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033735.D
Acq On : 03 Sep 2024 11:32
Operator : MA/JU
Sample : PB163093BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Manual IntegrationsAPPROVED

Quant Time: Sep 04 01:47:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/06/2024

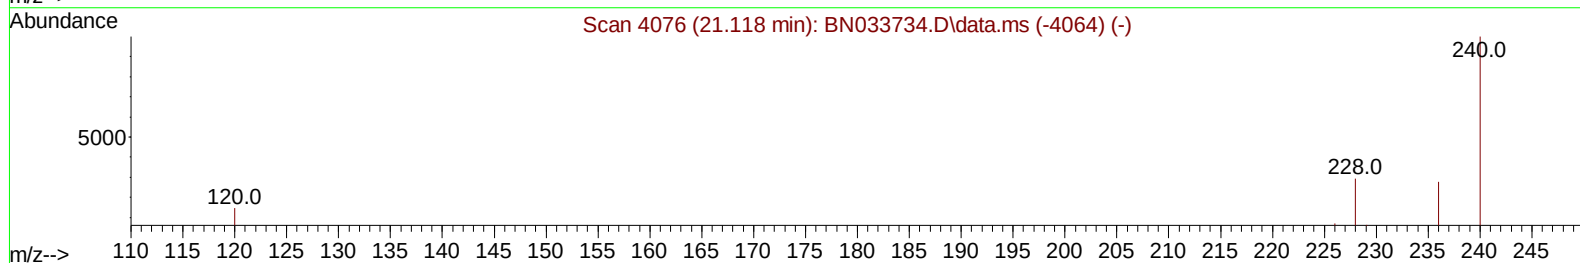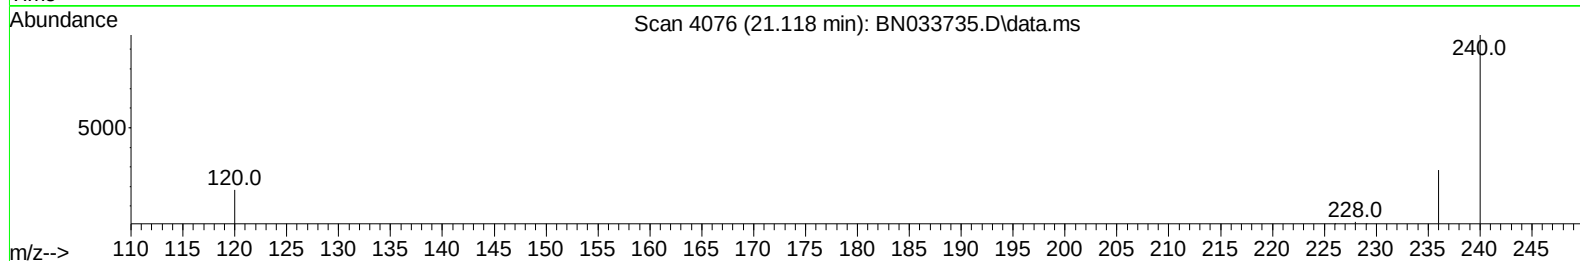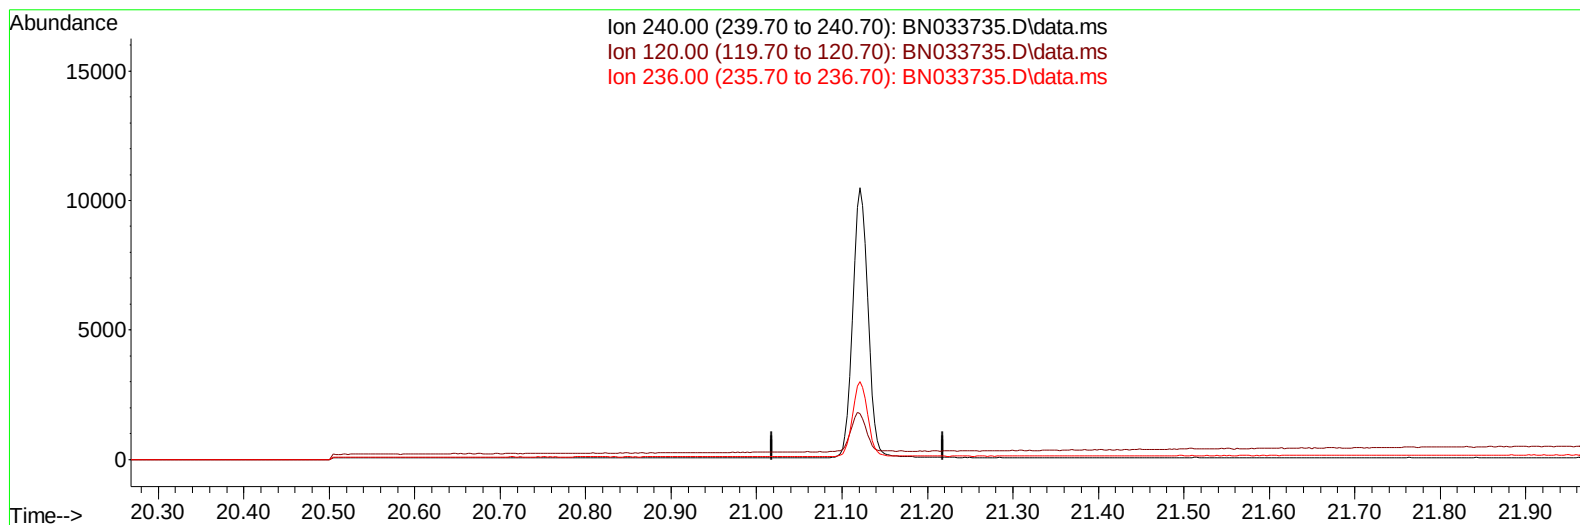

TIC: BN033735.D\data.ms

(17) Chrysene-d12

21.118min (-21.118) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.40	0.00#
236.00	28.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033735.D
Acq On : 03 Sep 2024 11:32
Operator : MA/JU
Sample : PB163093BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/06/2024

Quant Time: Sep 04 01:47:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

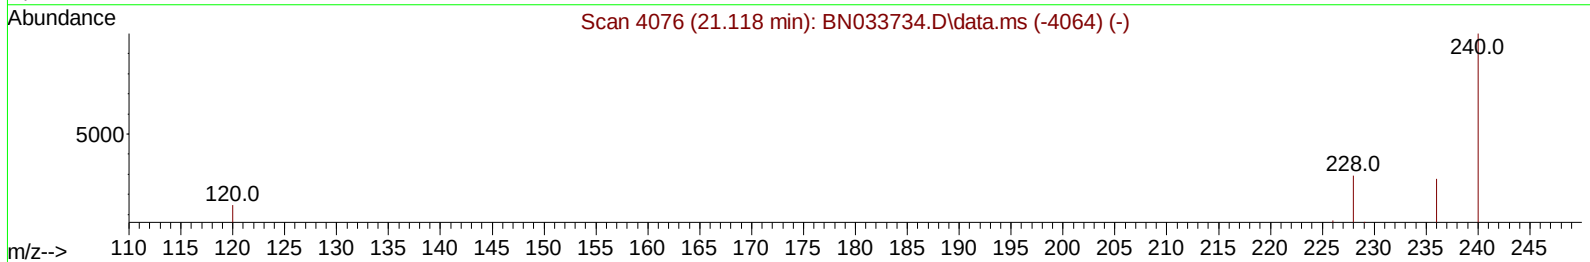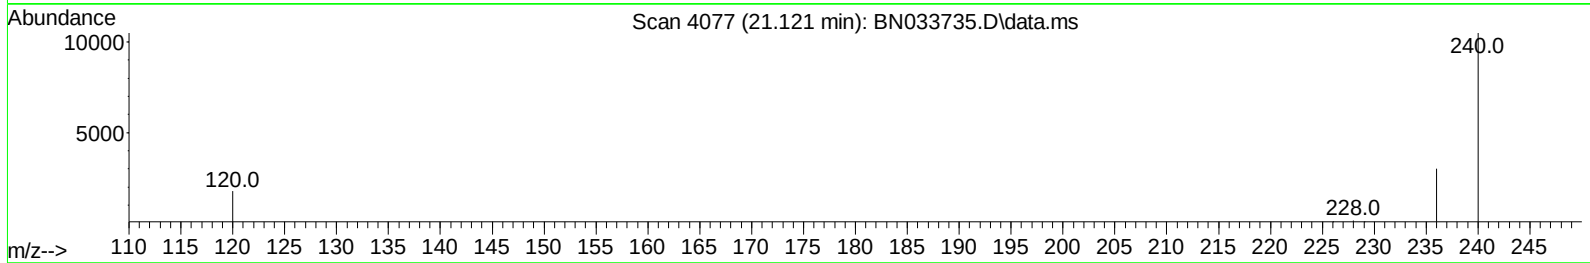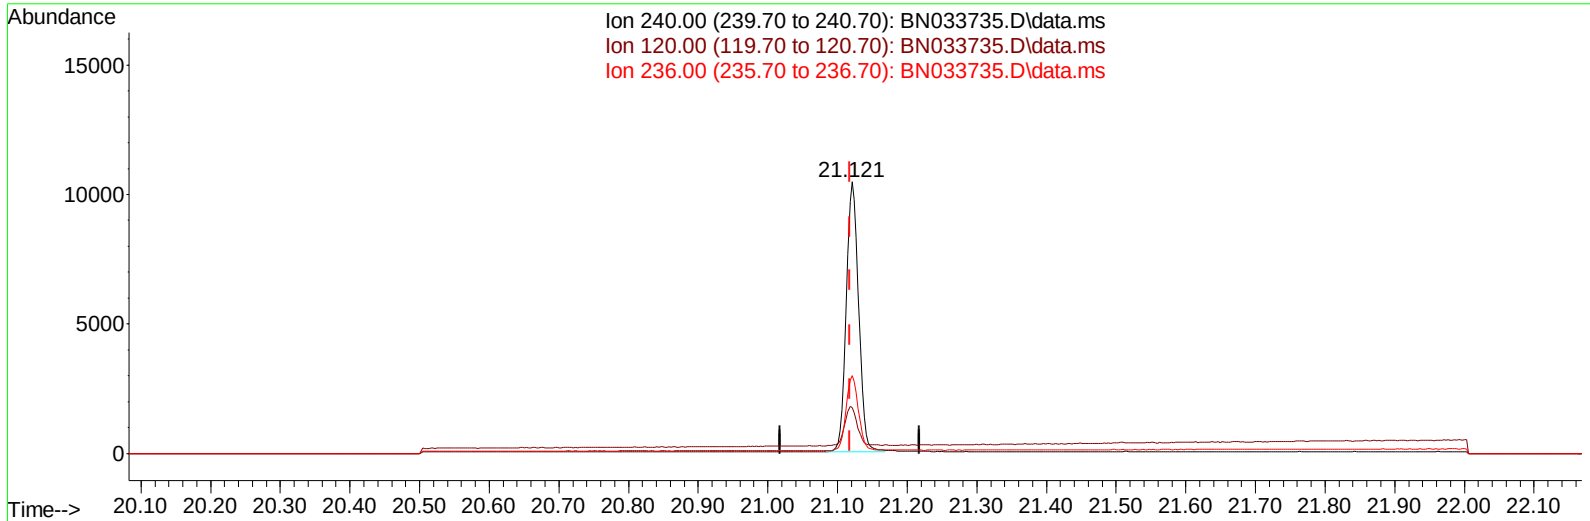

TIC: BN033735.D\data.ms

(17) Chrysene-d12

21.121min (+ 0.003) 0.40 ng/ul m

response 12793

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.40	16.88
236.00	28.30	28.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033735.D
Acq On : 03 Sep 2024 11:32
Operator : MA/JU
Sample : PB163093BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/06/2024

Quant Time: Sep 04 01:47:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

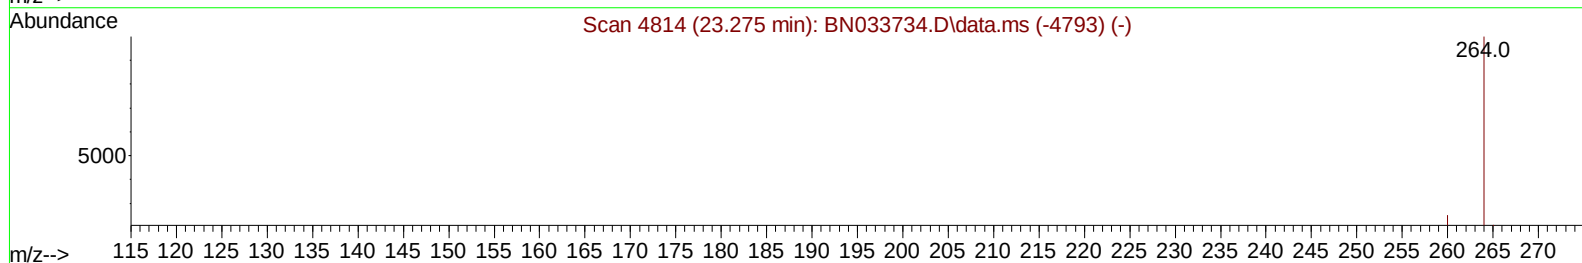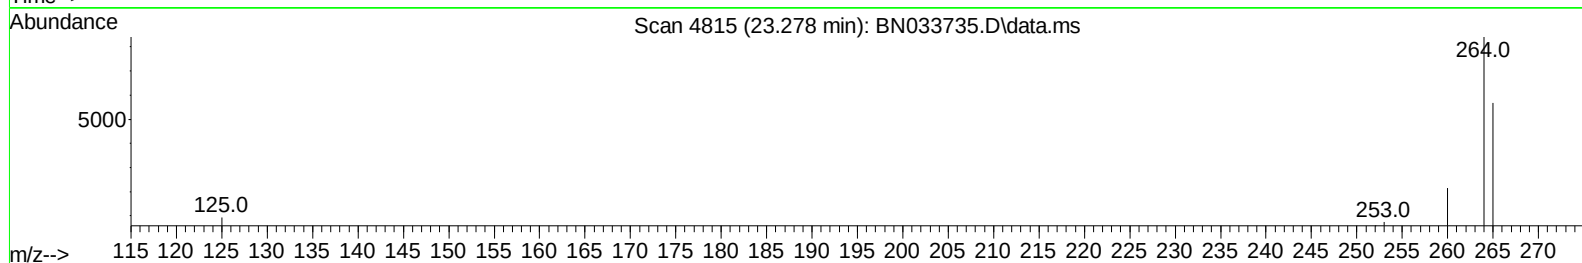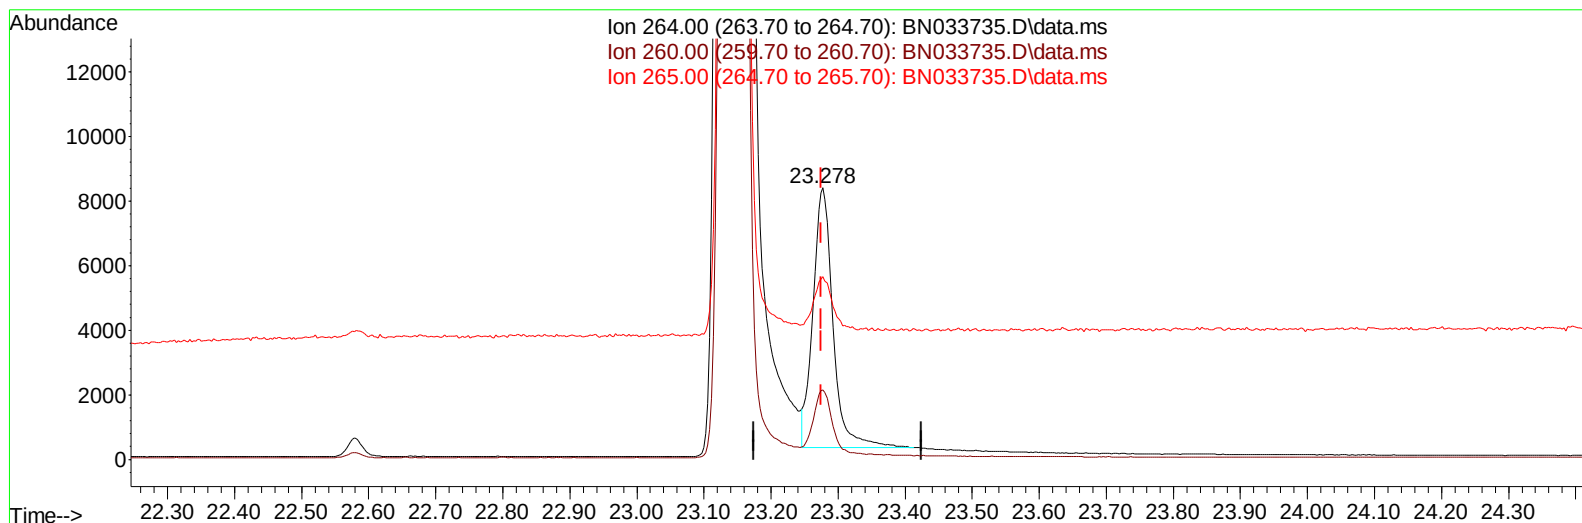

TIC: BN033735.D\data.ms

(23) Perylene-d12 (I)

23.278min (+ 0.003) 0.40 ng/u1

response 16607

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.68
265.00	73.30	67.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
 Data File : BN033735.D
 Acq On : 03 Sep 2024 11:32
 Operator : MA/JU
 Sample : PB163093BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK093

Manual IntegrationsAPPROVED

Quant Time: Sep 04 01:47:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 01:39:37 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/04/2024
 Supervised By :mohammad ahmed 09/06/2024

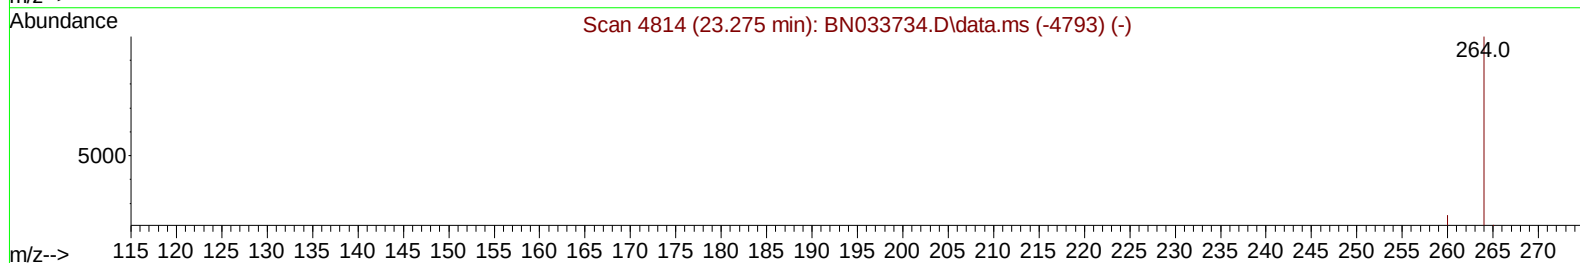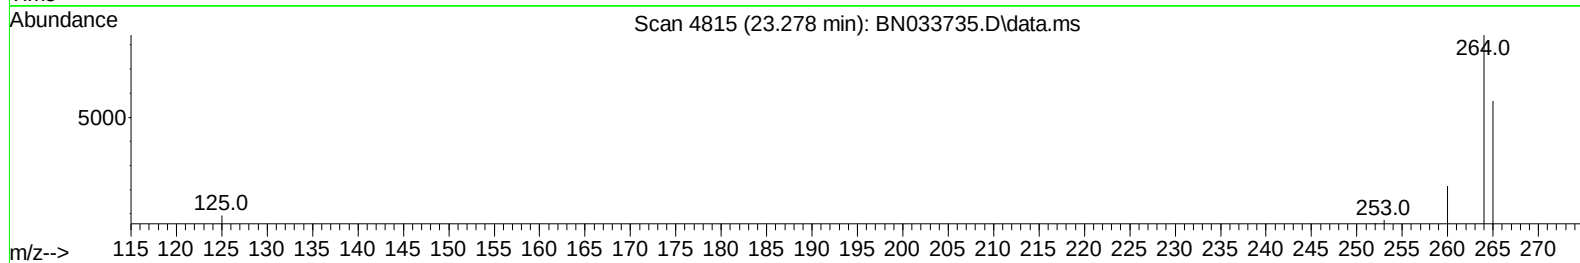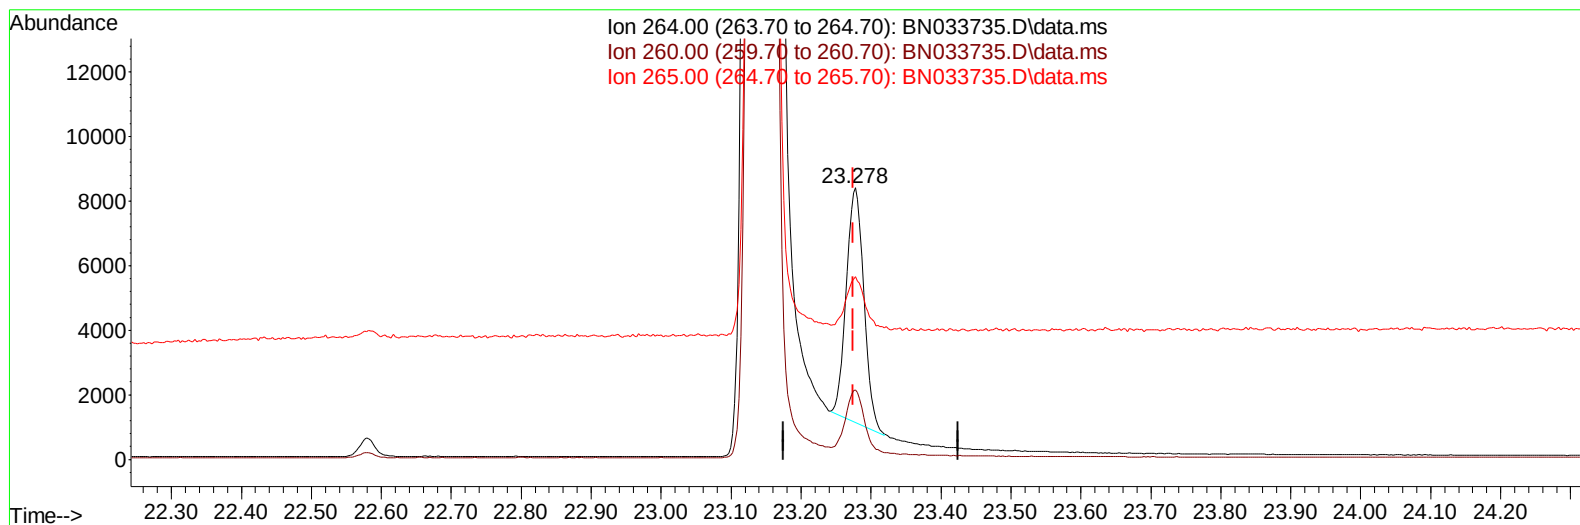

TIC: BN033735.D\data.ms

(23) Perylene-d12 (I)

23.278min (+ 0.003) 0.40 ng/ul m

response 12632

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.68
265.00	73.30	67.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
 Data File : BN033735.D
 Acq On : 03 Sep 2024 11:32
 Operator : MA/JU
 Sample : PB163093BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK093

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
 Supervised By :mohammad ahmed 09/06/2024

Quant Time: Sep 04 01:47:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 01:39:37 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.523	152		6002	0.400	ng/ul	0.00
4) Naphthalene-d8	10.283	136		16540	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.161	164		8444	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.915	188		16657m	0.400	ng/ul	0.00
17) Chrysene-d12	21.121	240		12793m	0.400	ng/ul	0.00
23) Perylene-d12	23.278	264		12632m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.135	96		38553	6.248	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.878	152		6744	0.284	ng/ul	0.00
18) Fluoranthene-d10	18.952	212		12513	0.328	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033735.D
Acq On : 03 Sep 2024 11:32
Operator : MA/JU
Sample : PB163093BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Manual IntegrationsAPPROVED

Quant Time: Sep 04 01:47:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/06/2024

