

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
 Data File : BN033742.D
 Acq On : 03 Sep 2024 15:45
 Operator : MA/JU
 Sample : P3809-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YE3E3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
 Supervised By :mohammad ahmed 09/06/2024

Quant Time: Sep 04 01:41:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 01:39:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.523	152	6246	0.400	ng/ul	0.00
4) Naphthalene-d8	10.283	136	17222	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.160	164	9135	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.914	188	19086m	0.400	ng/ul	0.00
17) Chrysene-d12	21.121	240	15611m	0.400	ng/ul	0.00
23) Perylene-d12	23.277	264	15521m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.135	96	36538	5.690	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.877	152	9080	0.367	ng/ul	0.00
18) Fluoranthene-d10	18.952	212	21018	0.452	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.164	88	55014	7.721	ng/ul#	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090324\
Data File : BN033742.D
Acq On : 03 Sep 2024 15:45
Operator : MA/JU
Sample : P3809-08
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YE3E3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
Supervised By :mohammad ahmed 09/06/2024


Quant Time: Sep 04 01:41:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 01:39:37 2024
Response via : Initial Calibration

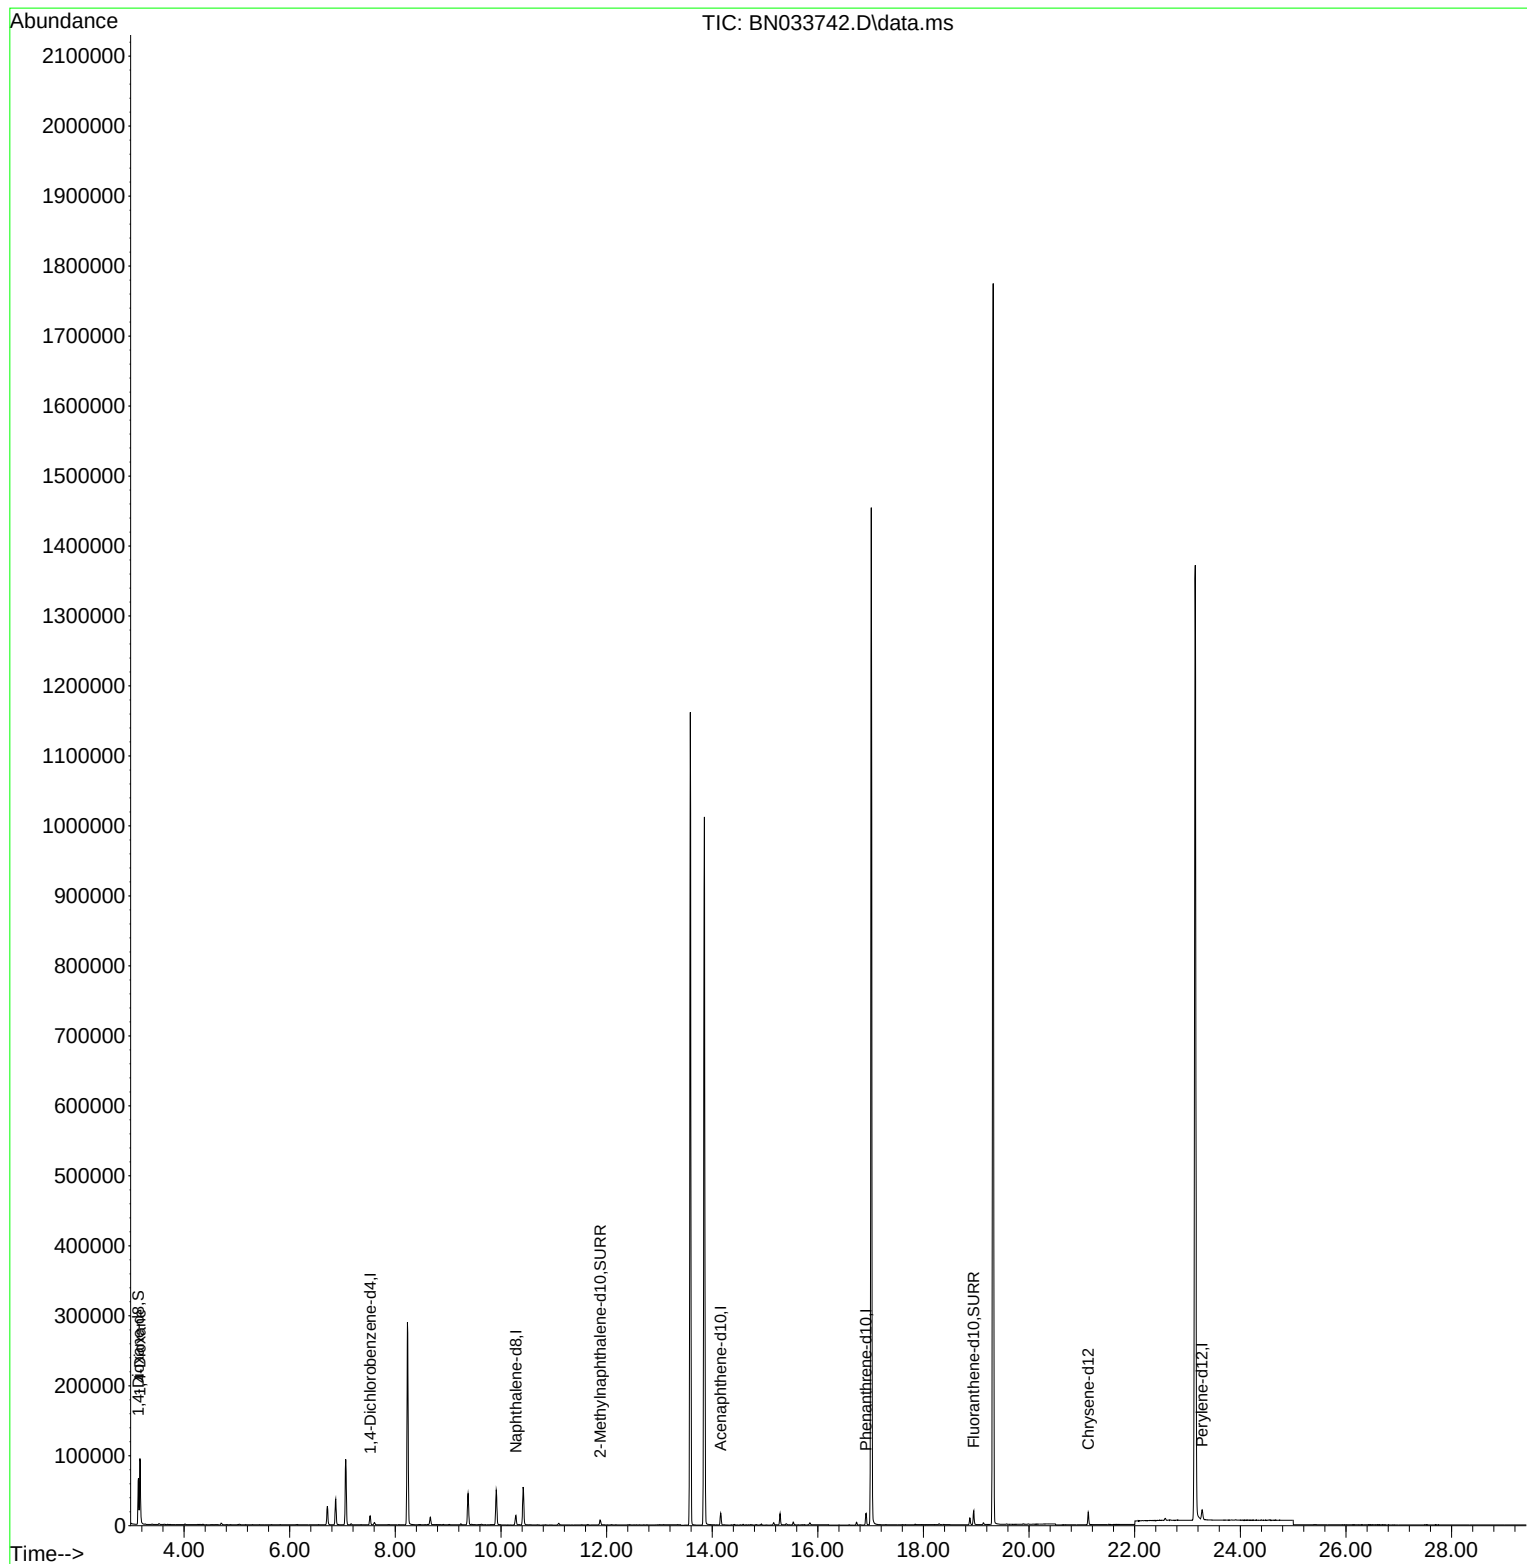

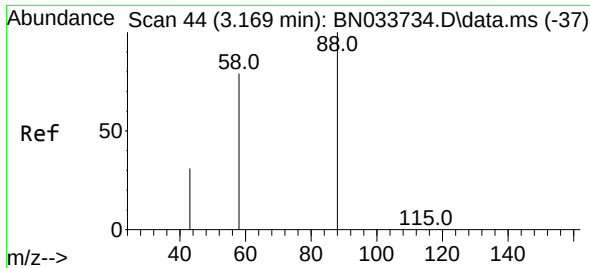

#2
 1,4-Dioxane
 Concen: 7.721 ng/ul
 RT: 3.164 min Scan# 41
 Delta R.T. -0.004 min
 Lab File: BN033742.D
 Acq: 03 Sep 2024 15:45

Instrument :
 BNA_N
 ClientSampleId :
 YE3E3

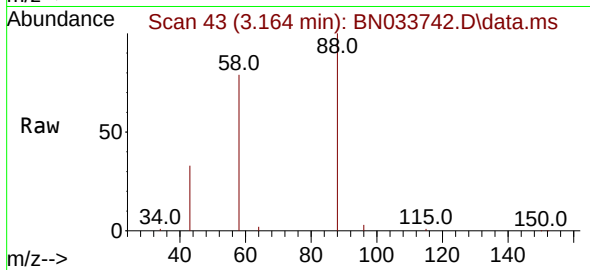

Tgt Ion: 88 Resp: 55014
 Ion Ratio Lower Upper
 88 100
 43 33.5 47.0 70.4
 58 79.5 53.0 79.4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/04/2024
 Supervised By :mohammad ahmed 09/06/2024

