
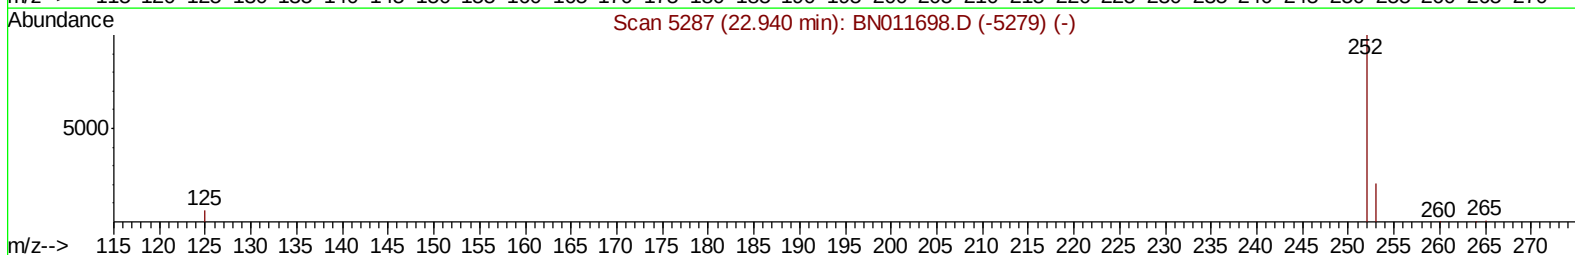
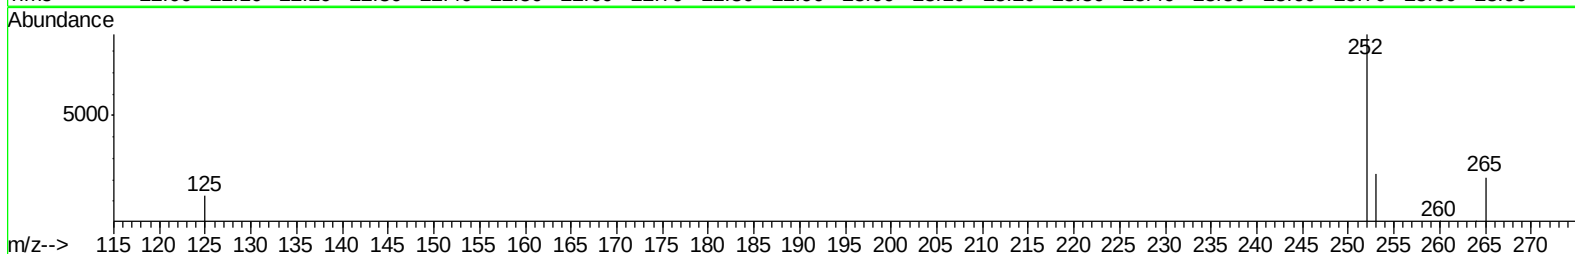


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011709.D
Acq On : 04 Sep 2020 19:20
Operator : CG/JU
Sample : L3840-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Sep 05 01:49:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 01:37:48 2020
Response via : Initial Calibration

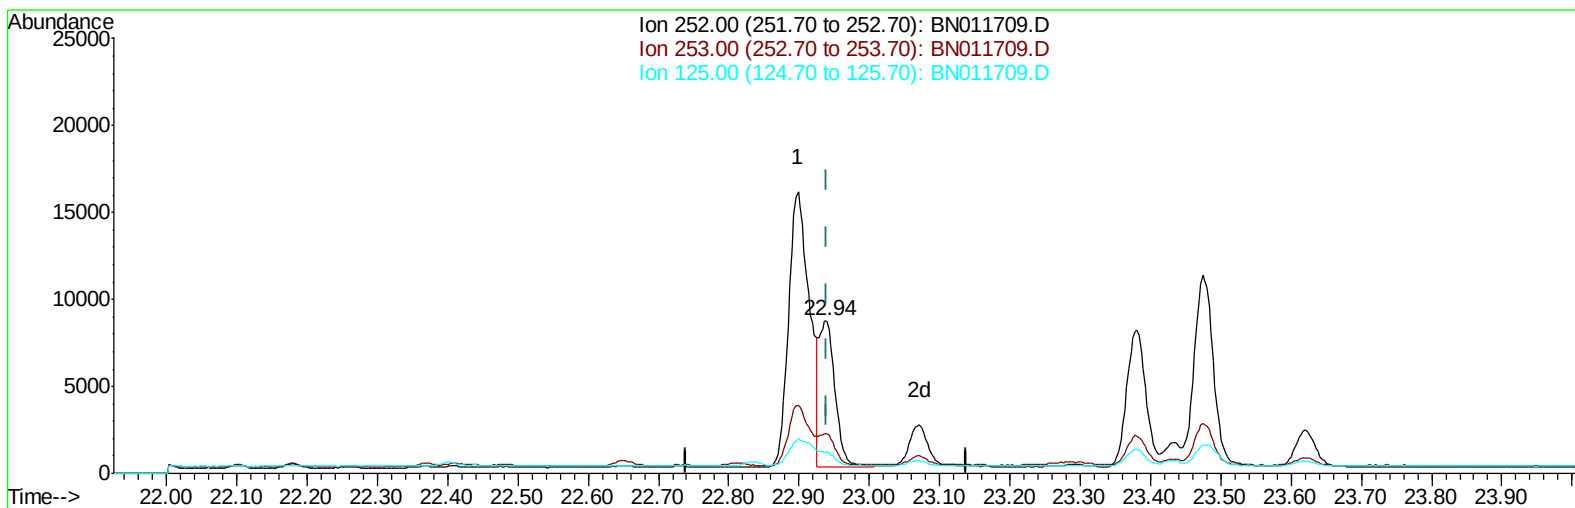

TIC: BN011709.D

(22) Benzo(k)fluoranthene

22.940min (-0.000) 0.27ng/ul m

response 13453

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	26.21
125.00	11.40	14.19#
0.00	0.00	0.00