
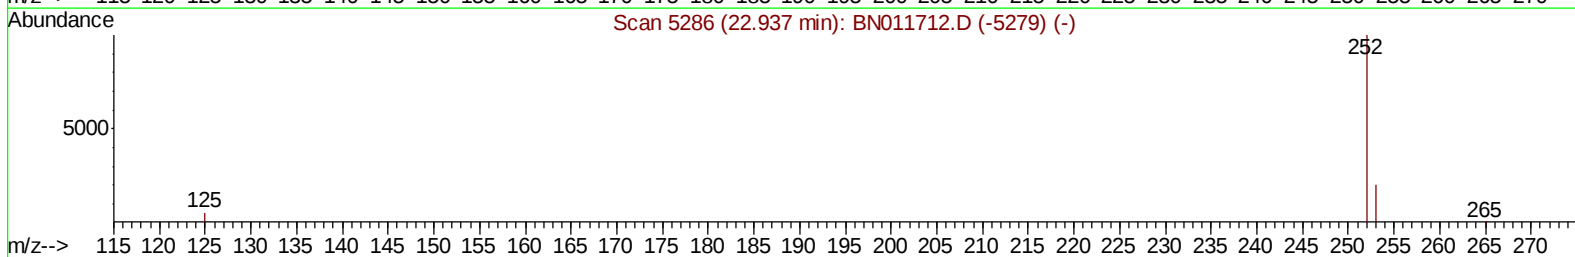
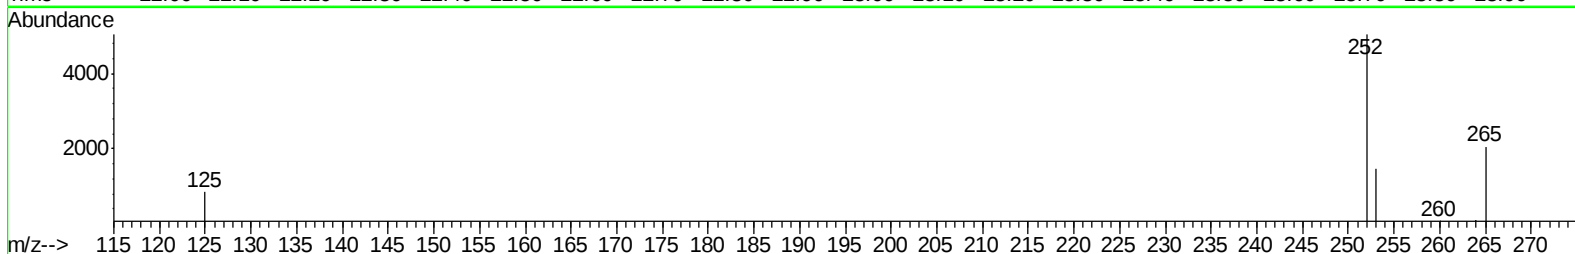


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011710.D
Acq On : 04 Sep 2020 19:57
Operator : CG/JU
Sample : L3840-04RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Sep 05 02:16:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 01:53:42 2020
Response via : Initial Calibration

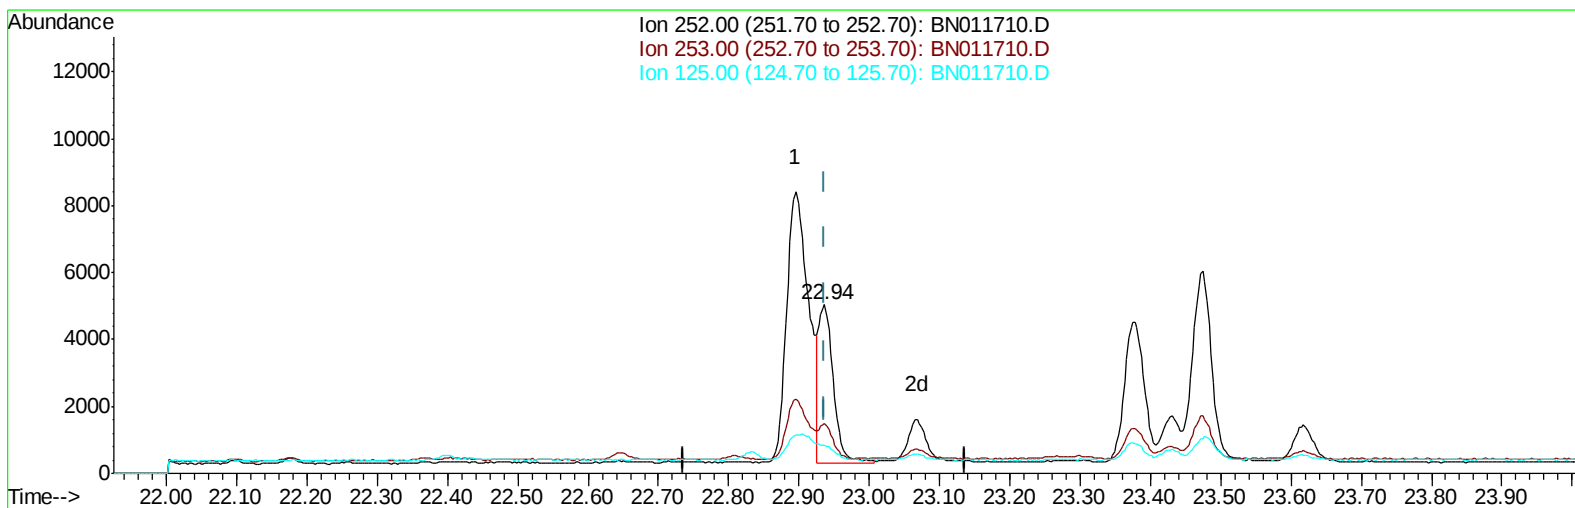

TIC: BN011710.D

(22) Benzo(k)fluoranthene

22.937min (+0.000) 0.13ng/ul m

response 6946

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	29.31
125.00	11.40	16.65#
0.00	0.00	0.00