
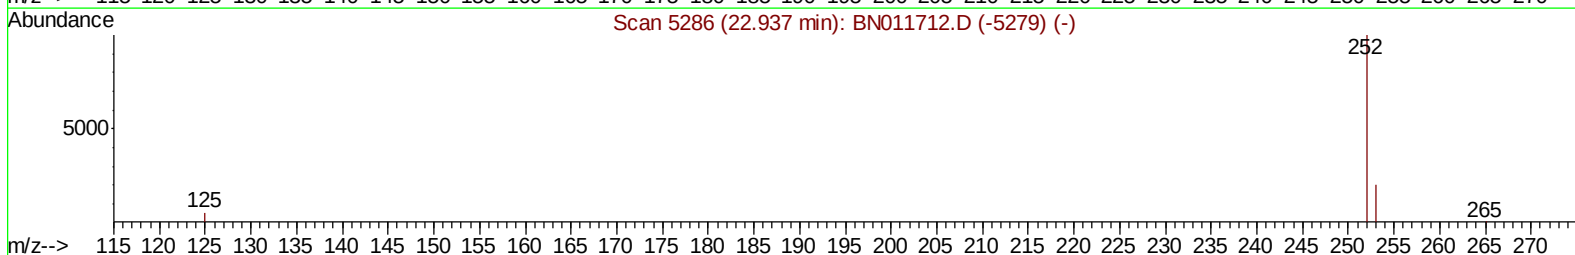
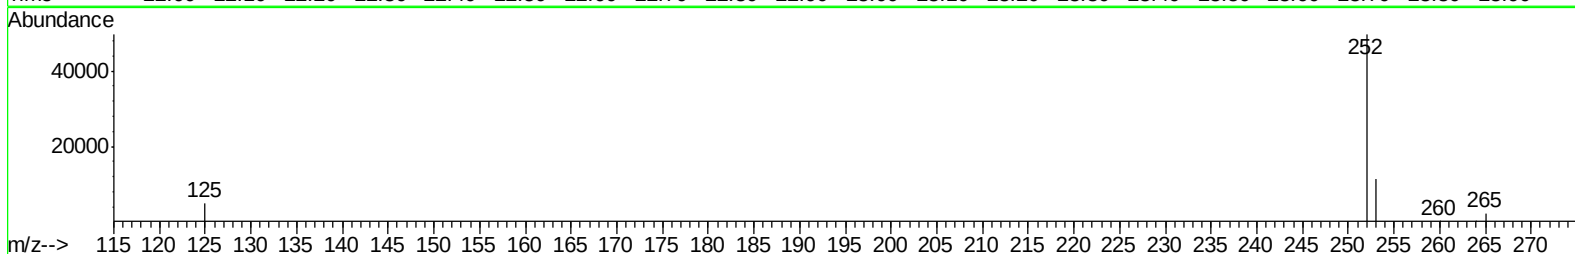


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011713.D
Acq On : 04 Sep 2020 22:59
Operator : CG/JU
Sample : L3840-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Sep 05 02:00:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 01:53:42 2020
Response via : Initial Calibration

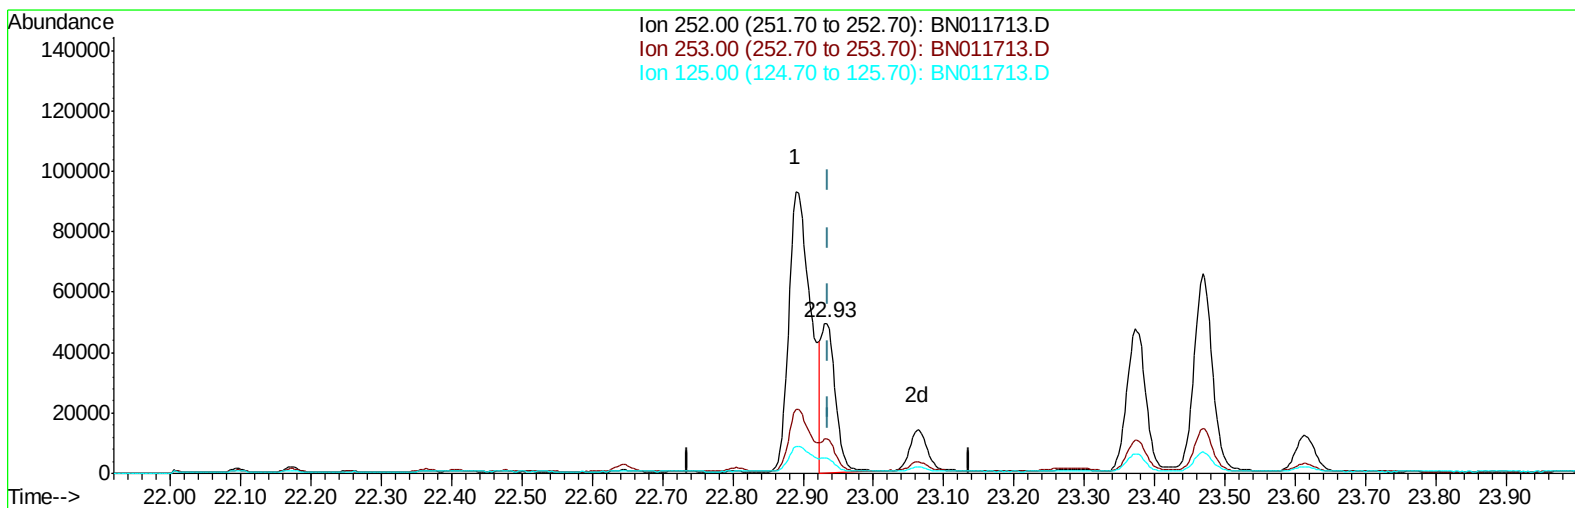

TIC: BN011713.D

(22) Benzo(k)fluoranthene

22.934min (-0.003) 1.56ng/ul m

response 72103

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	23.13
125.00	11.40	10.15
0.00	0.00	0.00