
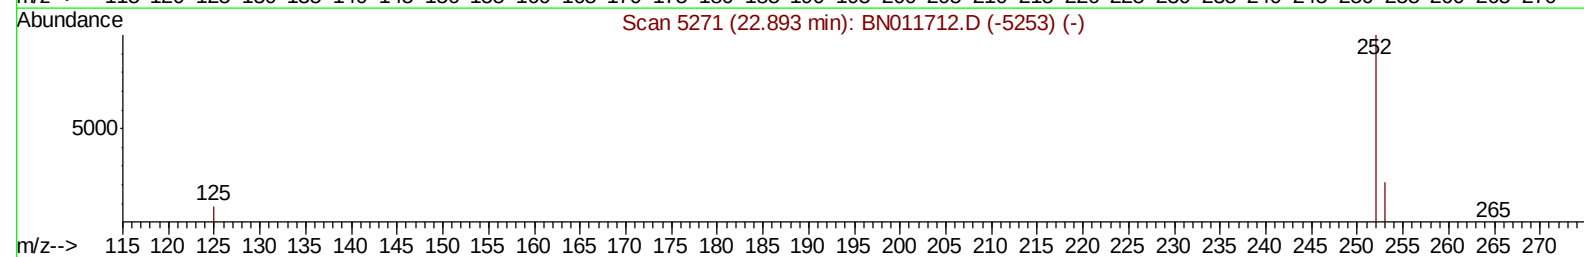
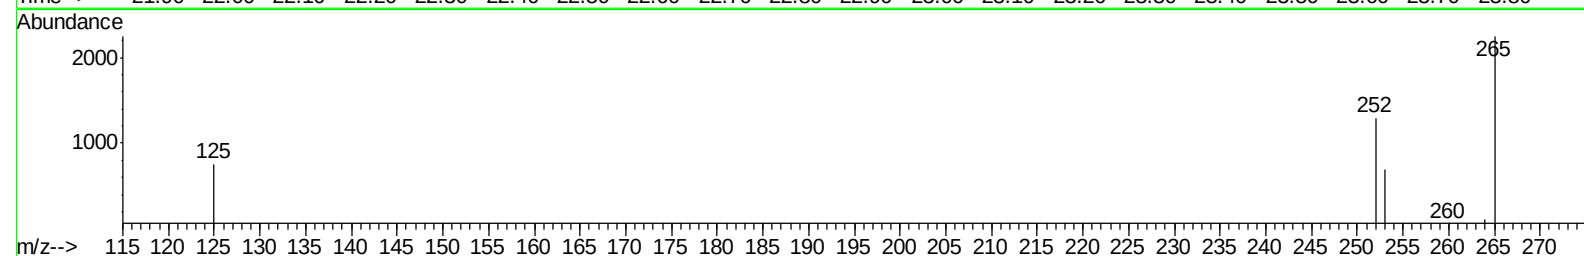


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011714.D
Acq On : 04 Sep 2020 23:34
Operator : CG/JU
Sample : L3840-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Sep 05 02:03:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 01:53:42 2020
Response via : Initial Calibration

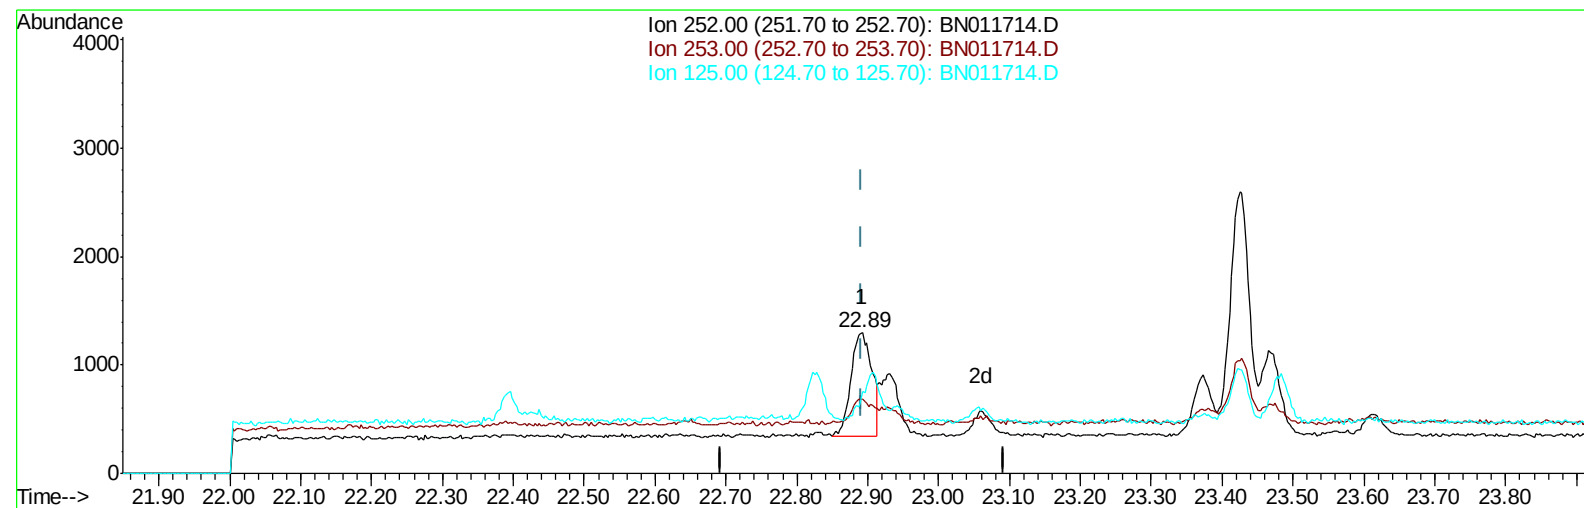

TIC: BN011714.D

(21) Benzo(b)fluoranthene

22.893min (-0.000) 0.04ng/ul m

response 1979

Ion	Exp%	Act%
252.00	100	100
253.00	27.40	53.08
125.00	11.10	58.17#
0.00	0.00	0.00