
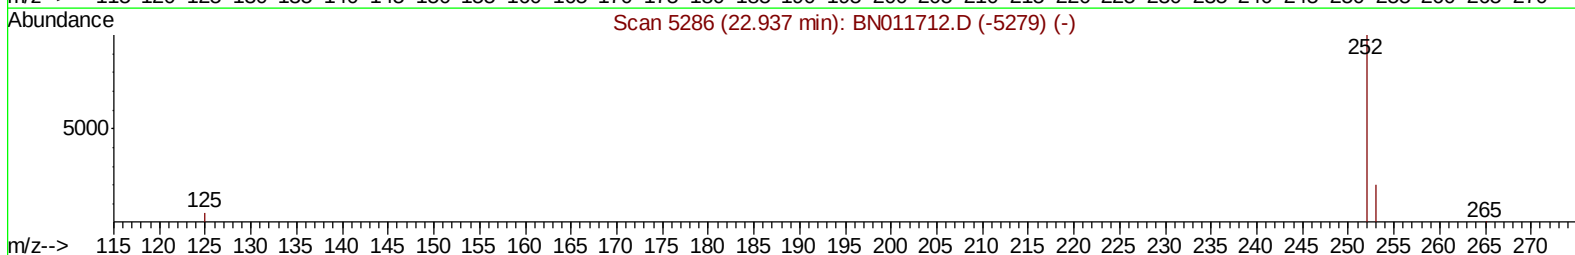
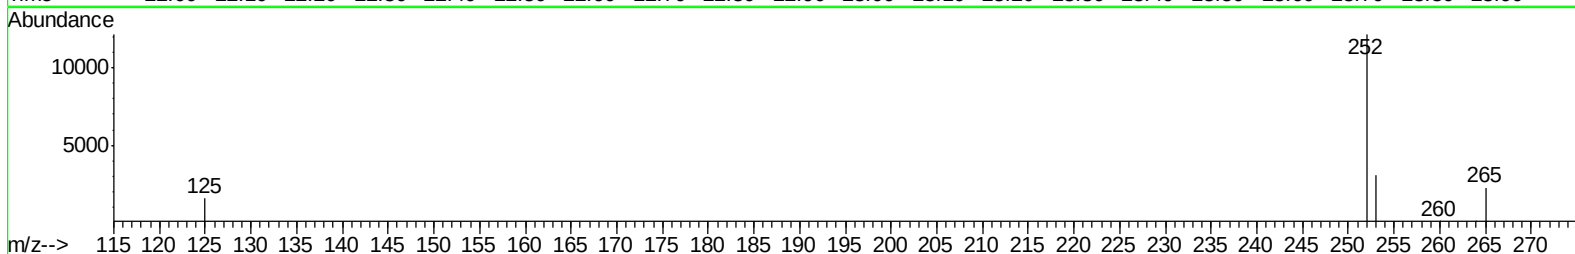


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011715.D
Acq On : 05 Sep 2020 00:11
Operator : CG/JU
Sample : L3840-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Sep 05 02:06:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 01:53:42 2020
Response via : Initial Calibration

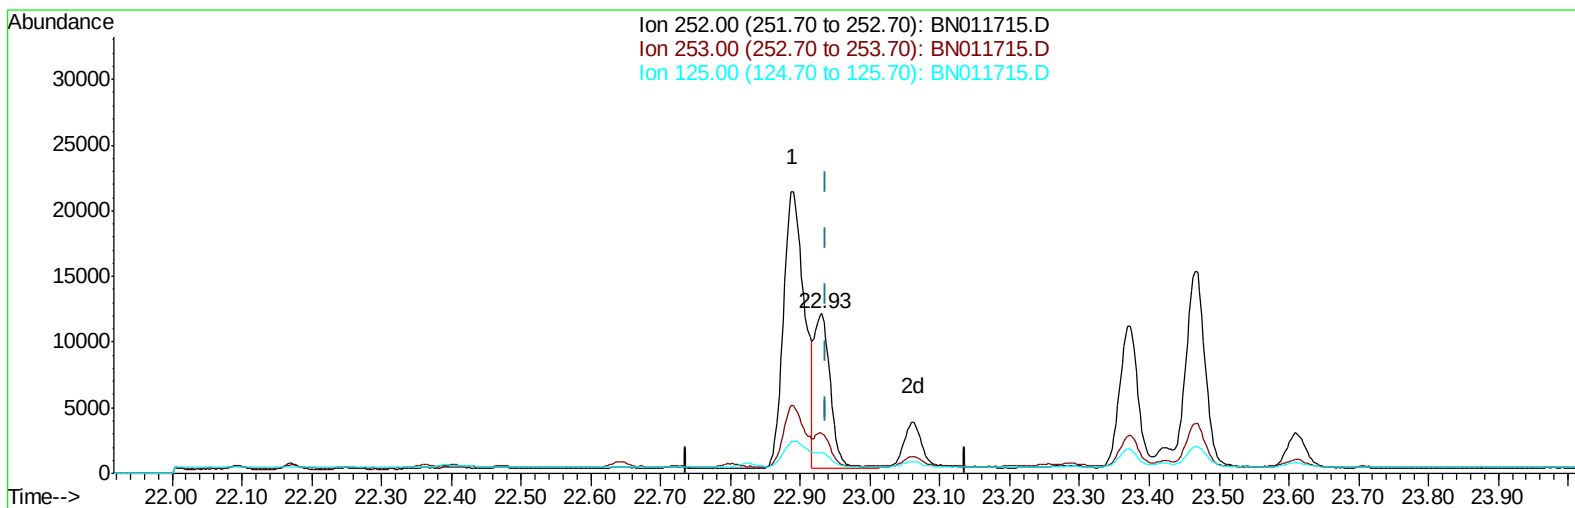

TIC: BN011715.D

(22) Benzo(k)fluoranthene

22.931min (-0.006) 0.32ng/ul m

response 18778

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	25.24
125.00	11.40	12.74
0.00	0.00	0.00