
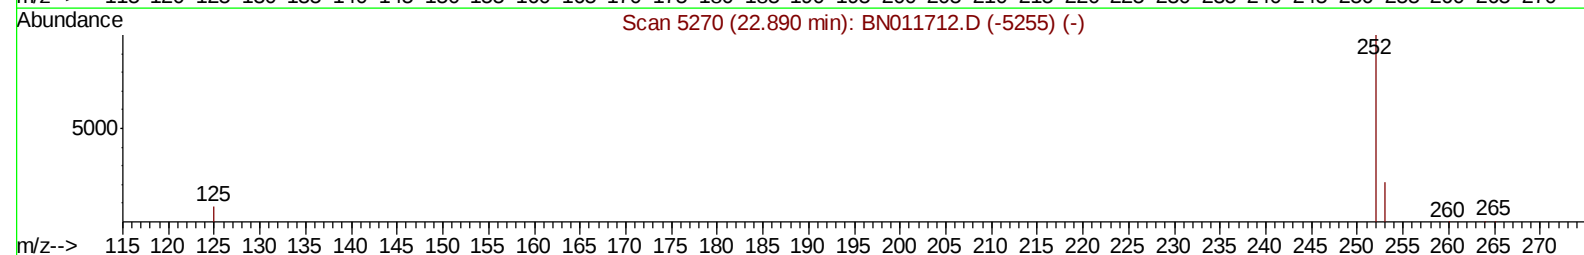
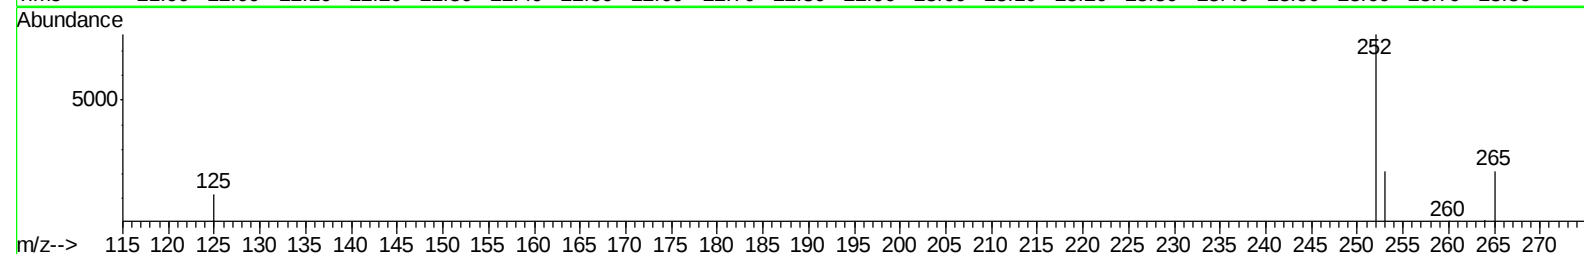


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011717.D
Acq On : 05 Sep 2020 01:23
Operator : CG/JU
Sample : L3840-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Sep 05 06:05:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

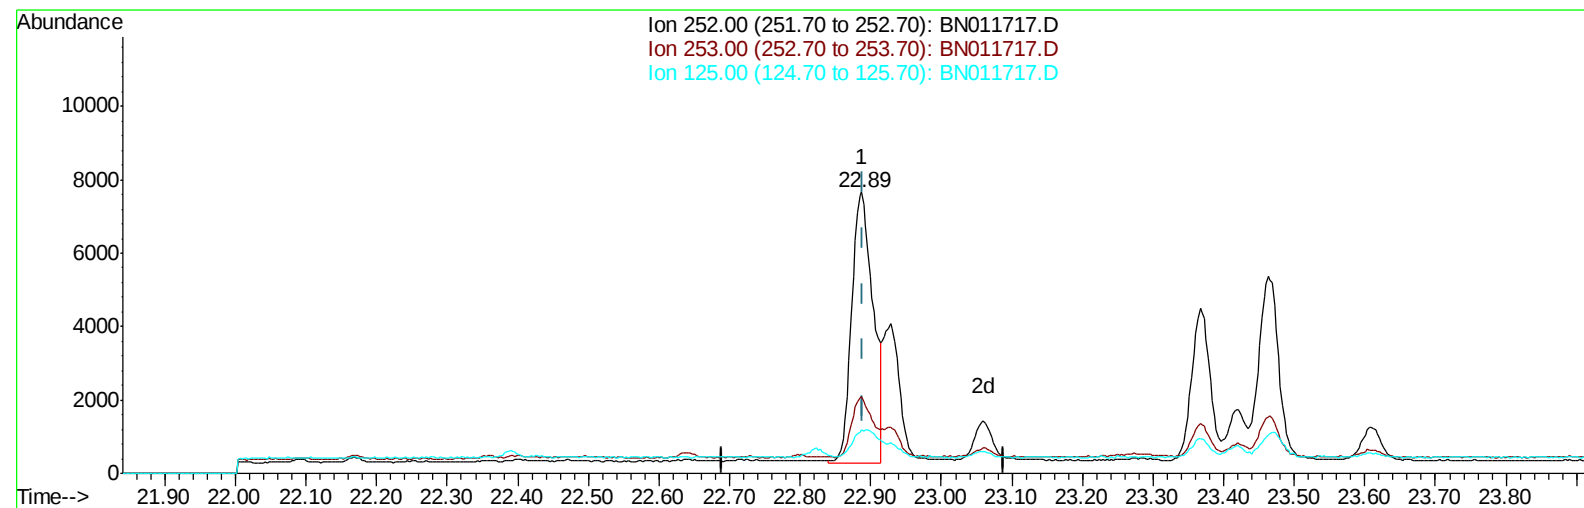

TIC: BN011717.D

(21) Benzo(b)fluoranthene

22.887min (-0.003) 0.34ng/ul m

response 15277

Ion	Exp%	Act%
252.00	100	100
253.00	27.40	27.25
125.00	11.10	15.25
0.00	0.00	0.00