
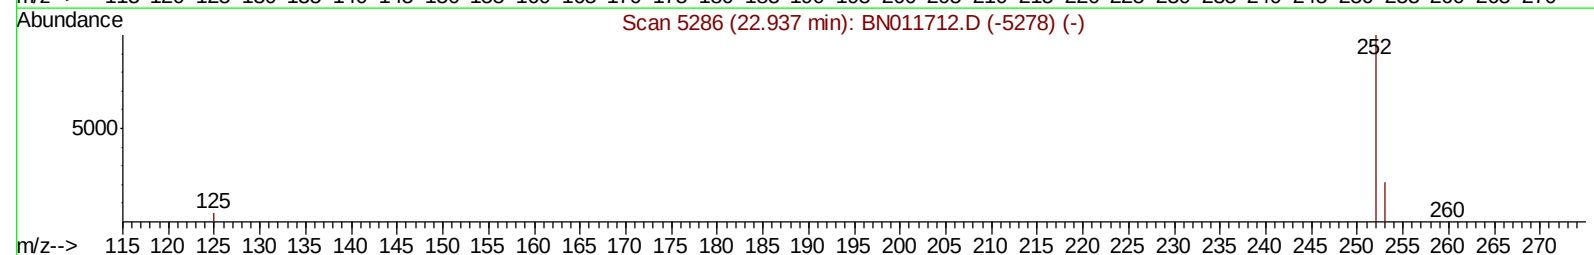
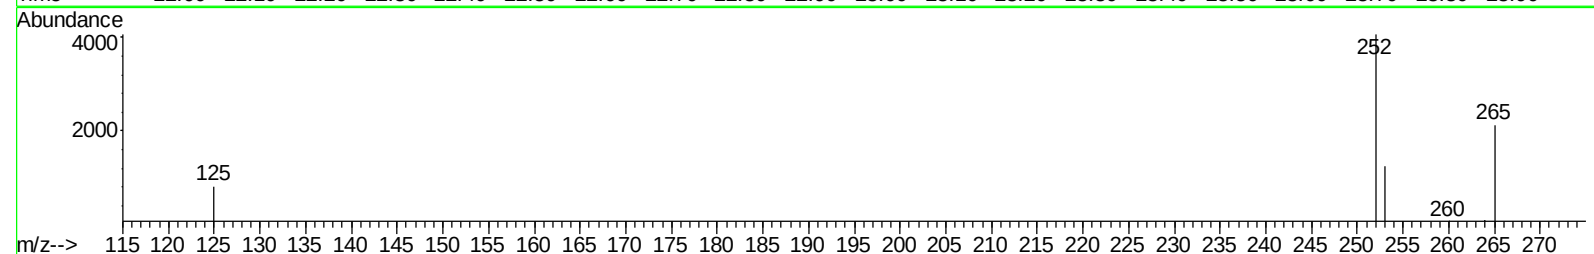


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011717.D
Acq On : 05 Sep 2020 01:23
Operator : CG/JU
Sample : L3840-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Sep 05 06:05:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

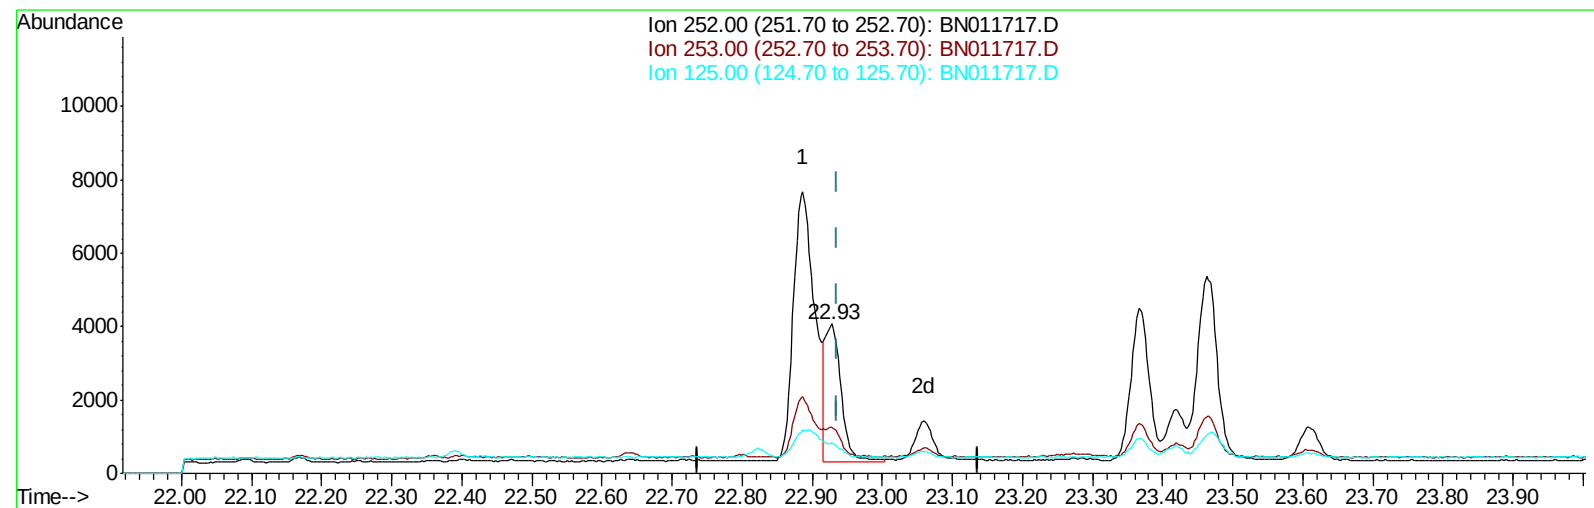

TIC: BN011717.D

(22) Benzo(k)fluoranthene

22.928min (-0.009) 0.12ng/ul m

response 5795

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	30.97
125.00	11.40	20.20#
0.00	0.00	0.00