
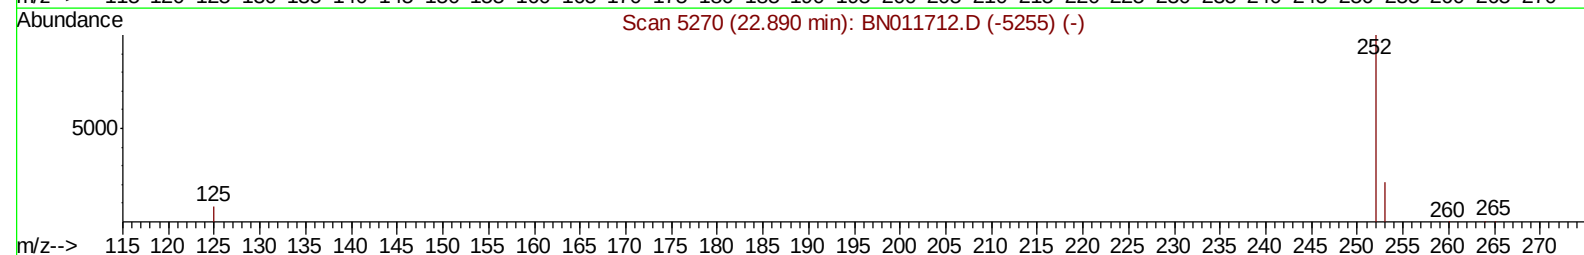
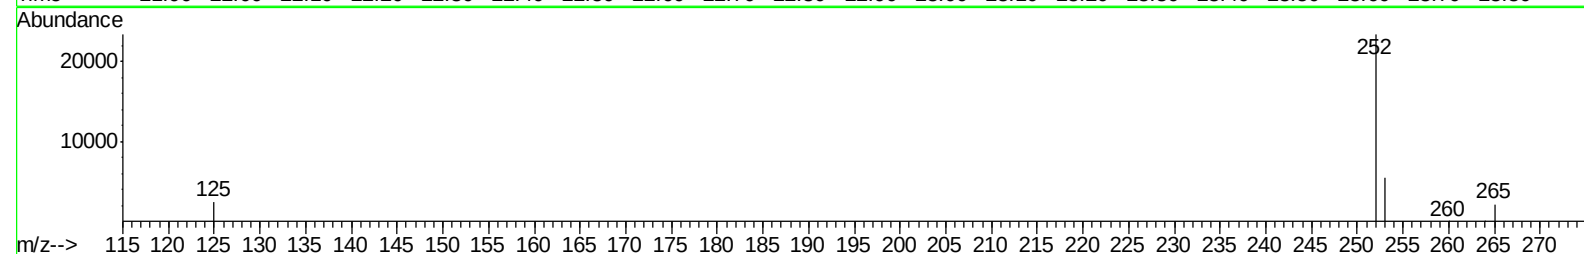


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011719.D
Acq On : 05 Sep 2020 02:36
Operator : CG/JU
Sample : L3840-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Sep 05 06:01:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

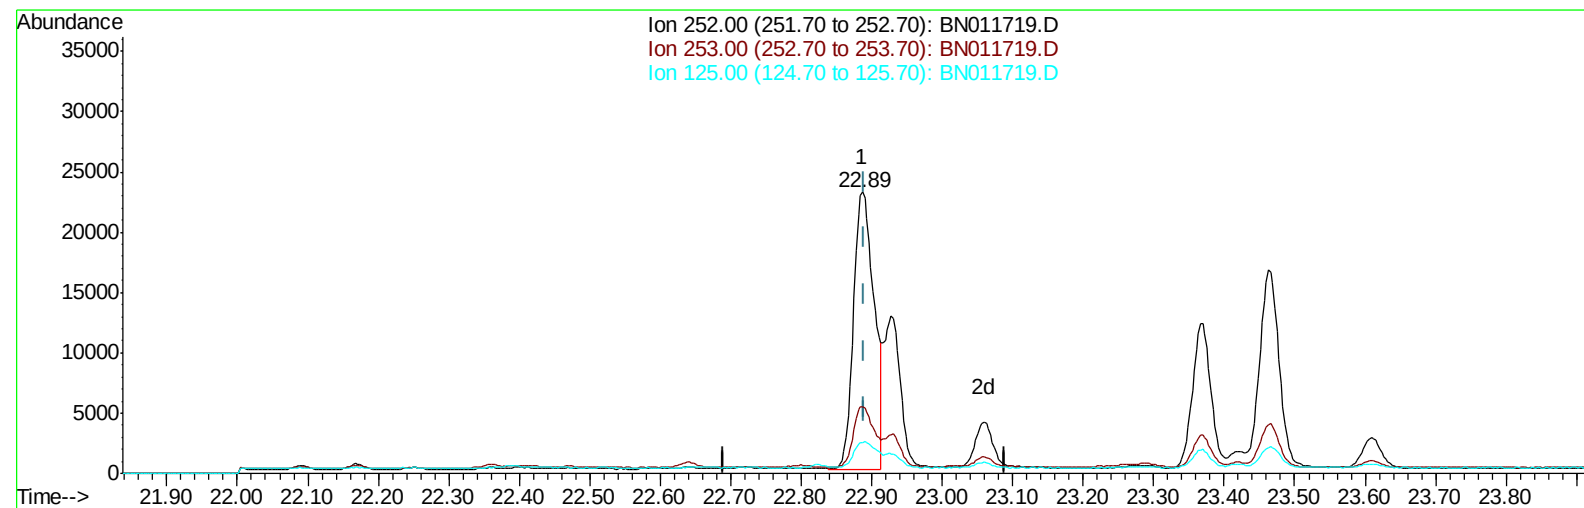

TIC: BN011719.D

(21) Benzo(b)fluoranthene

22.887min (-0.003) 0.91ng/ul m

response 46694

Ion	Exp%	Act%
252.00	100	100
253.00	27.40	23.76
125.00	11.10	10.77
0.00	0.00	0.00