
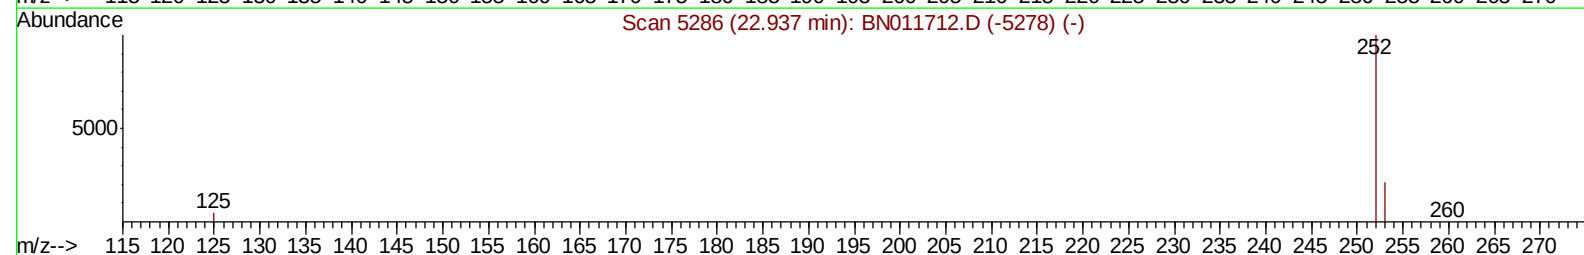
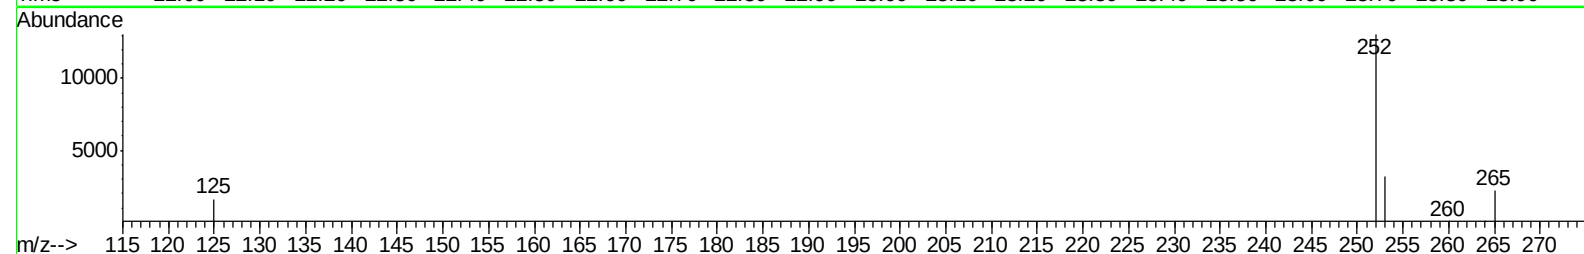


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011719.D
 Acq On : 05 Sep 2020 02:36
 Operator : CG/JU
 Sample : L3840-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Sep 05 06:01:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

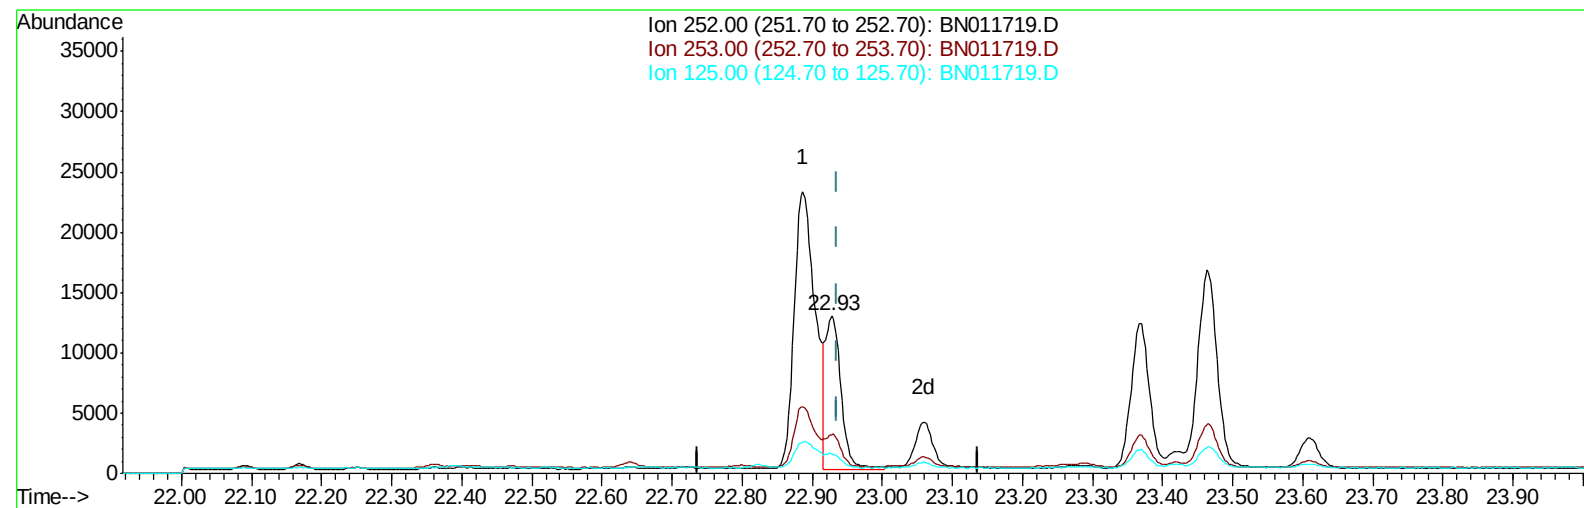

TIC: BN011719.D

(22) Benzo(k)fluoranthene

22.928min (-0.009) 0.34ng/ul m

response 19022

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	24.67
125.00	11.40	12.46
0.00	0.00	0.00