
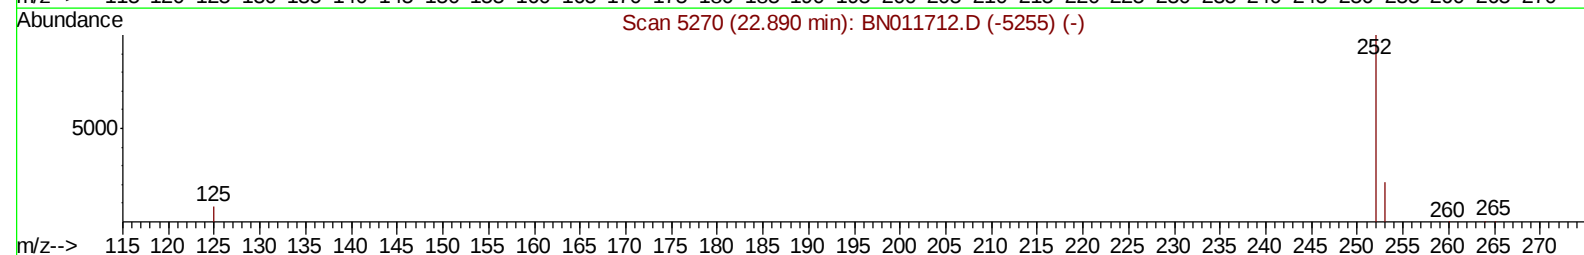
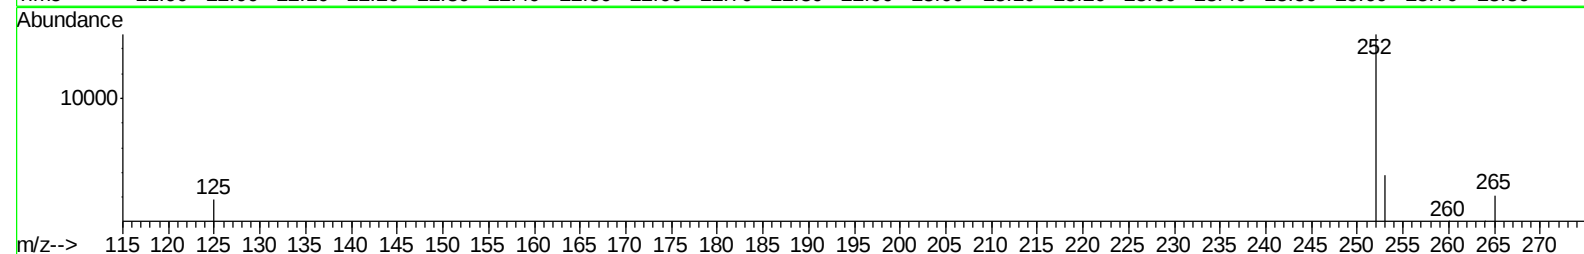


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\  
 Data File : BN011720.D  
 Acq On : 05 Sep 2020 03:12  
 Operator : CG/JU  
 Sample : L3843-04  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 05 06:01:52 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Sep 05 05:40:34 2020  
 Response via : Initial Calibration

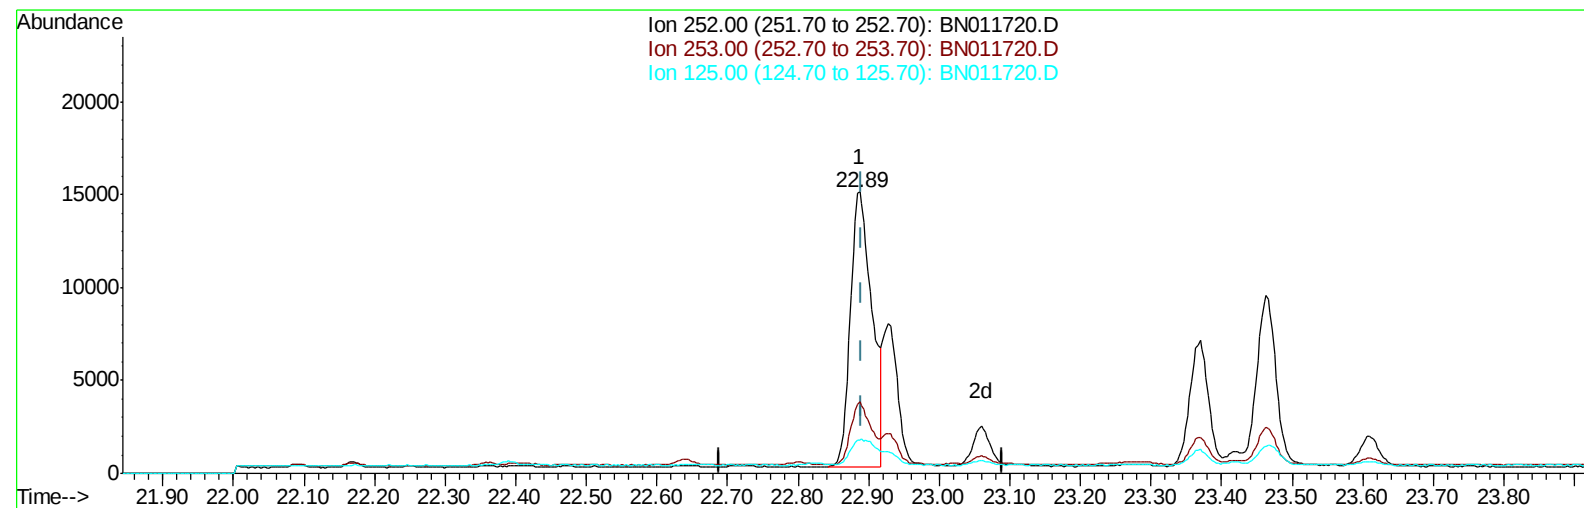

TIC: BN011720.D

(21) Benzo(b)fluoranthene

22.887min (-0.003) 0.60ng/ul m

response 31168

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 27.40 | 25.30 |
| 125.00 | 11.10 | 11.98 |
| 0.00   | 0.00  | 0.00  |