
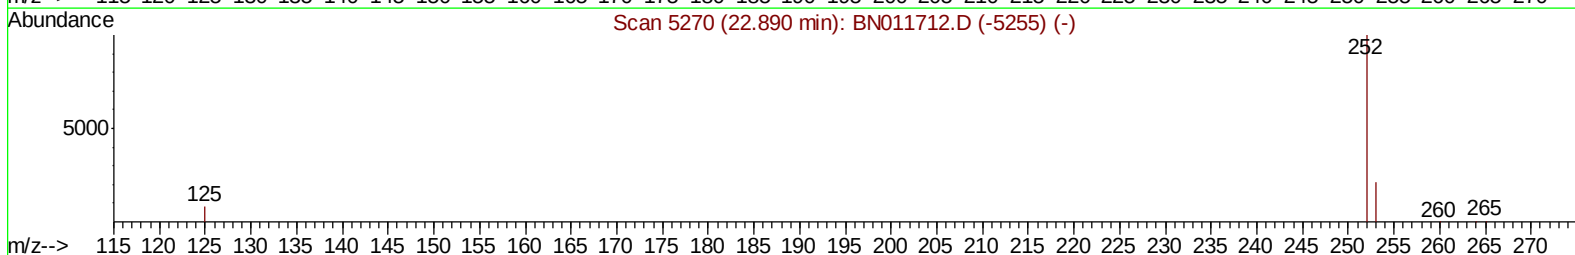
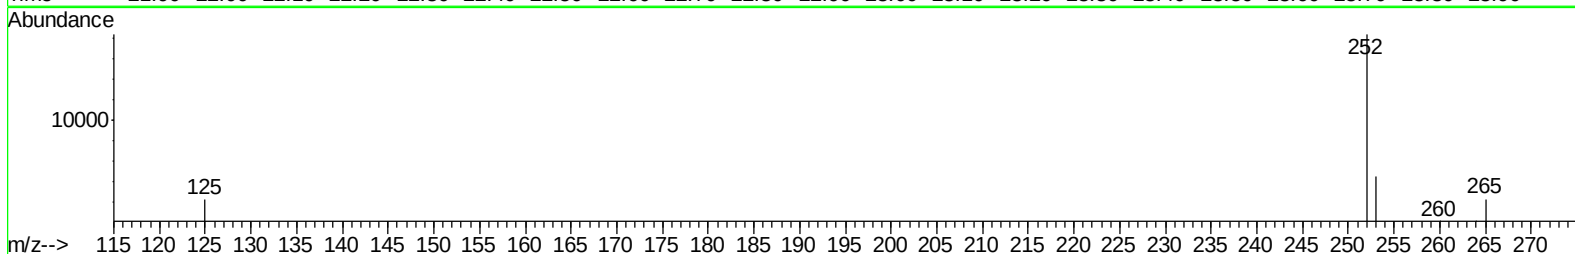


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\  
Data File : BN011721.D  
Acq On : 05 Sep 2020 03:48  
Operator : CG/JU  
Sample : L3843-01  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Sep 05 06:27:26 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Sep 05 05:40:34 2020  
Response via : Initial Calibration

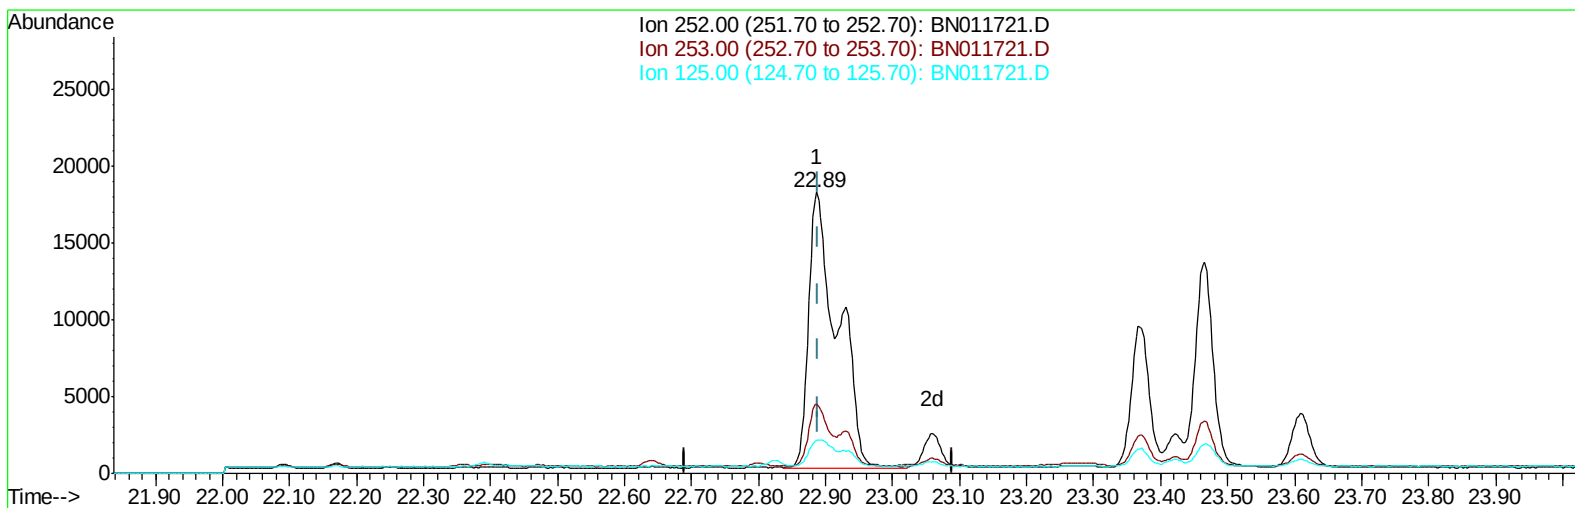

TIC: BN011721.D

(21) Benzo(b)fluoranthene

22.887min (-0.003) 22.00ng/ul

response 54401

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 27.40 | 24.50 |
| 125.00 | 11.10 | 11.83 |
| 0.00   | 0.00  | 0.00  |