
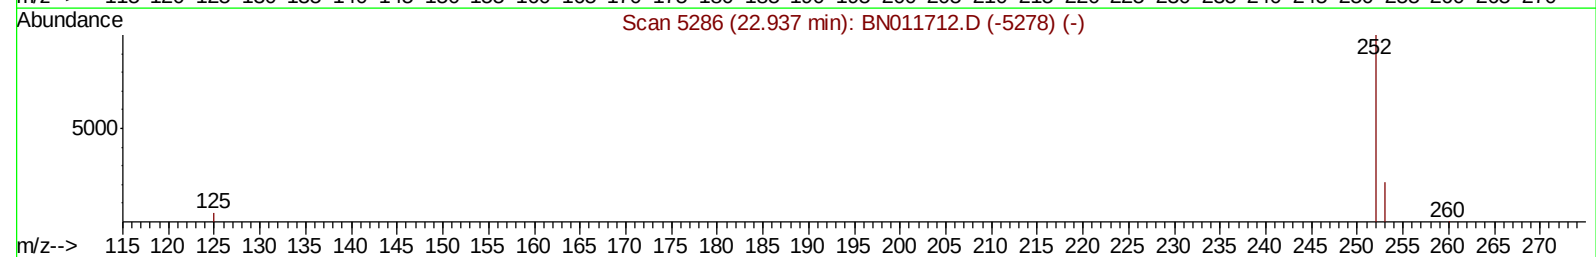
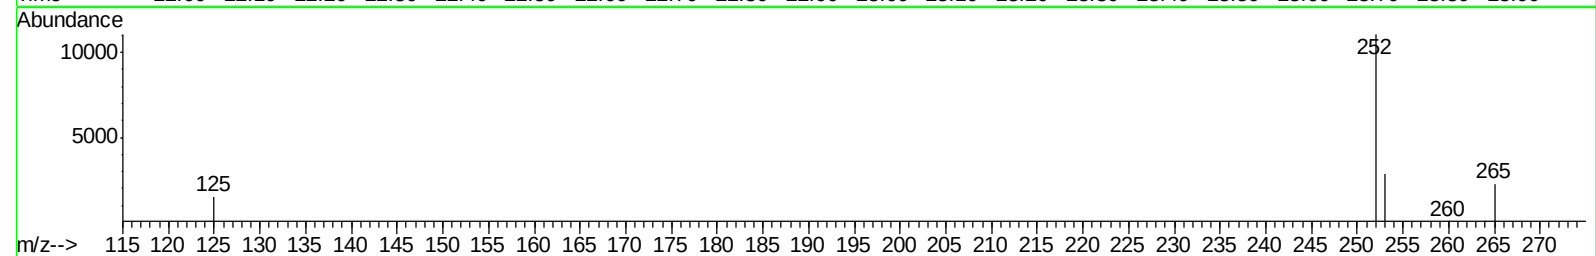


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011722.D
Acq On : 05 Sep 2020 04:24
Operator : CG/JU
Sample : L3843-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 05 06:32:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

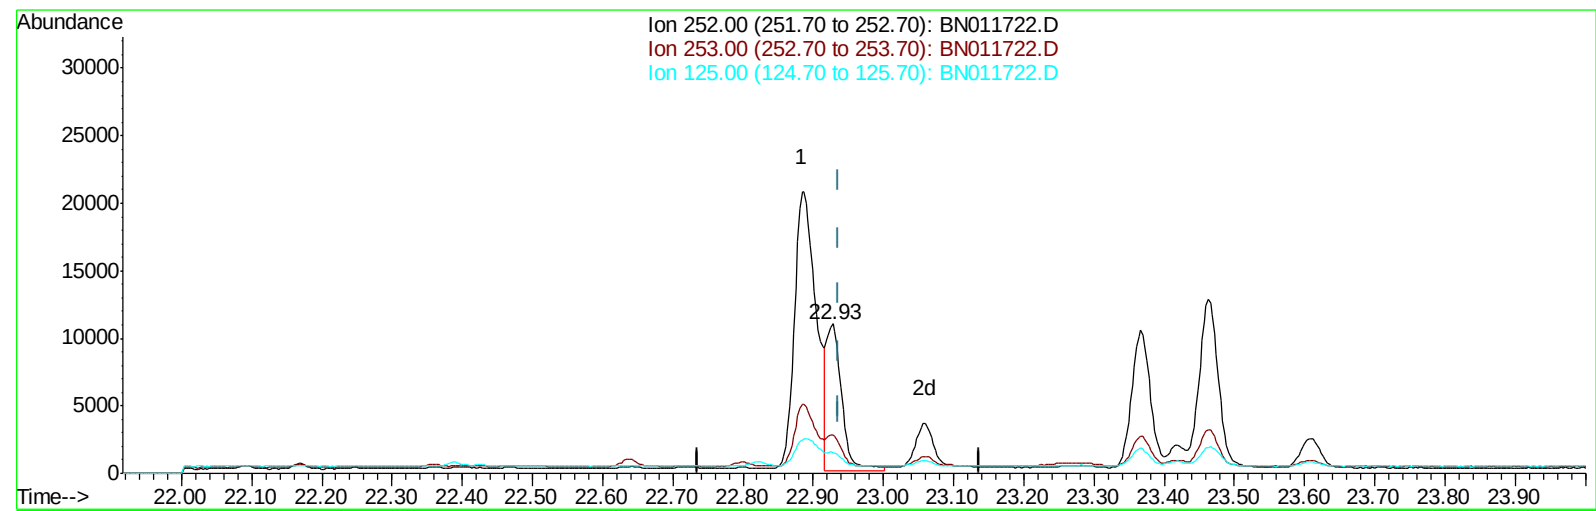

TIC: BN011722.D

(22) Benzo(k)fluoranthene

22.928min (-0.009) 7.08ng/ul m

response 16334

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	25.93
125.00	11.40	13.86#
0.00	0.00	0.00