
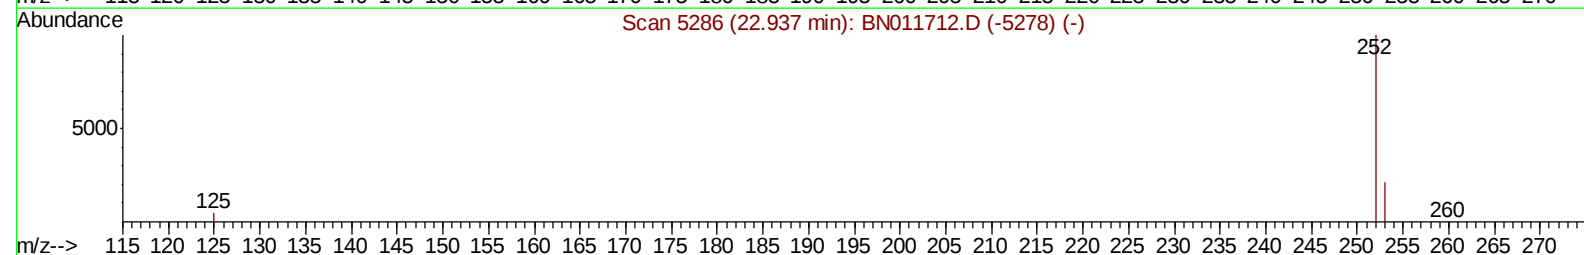
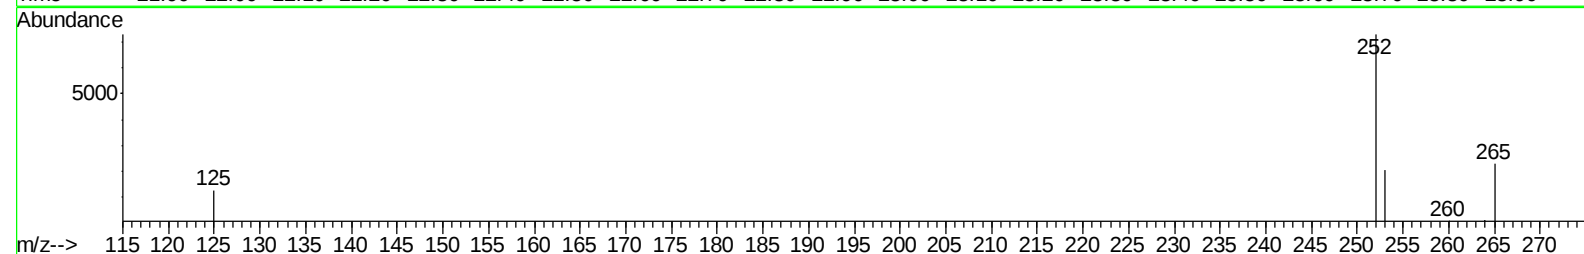


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011723.D
 Acq On : 05 Sep 2020 05:00
 Operator : CG/JU
 Sample : L3843-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 05 06:35:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

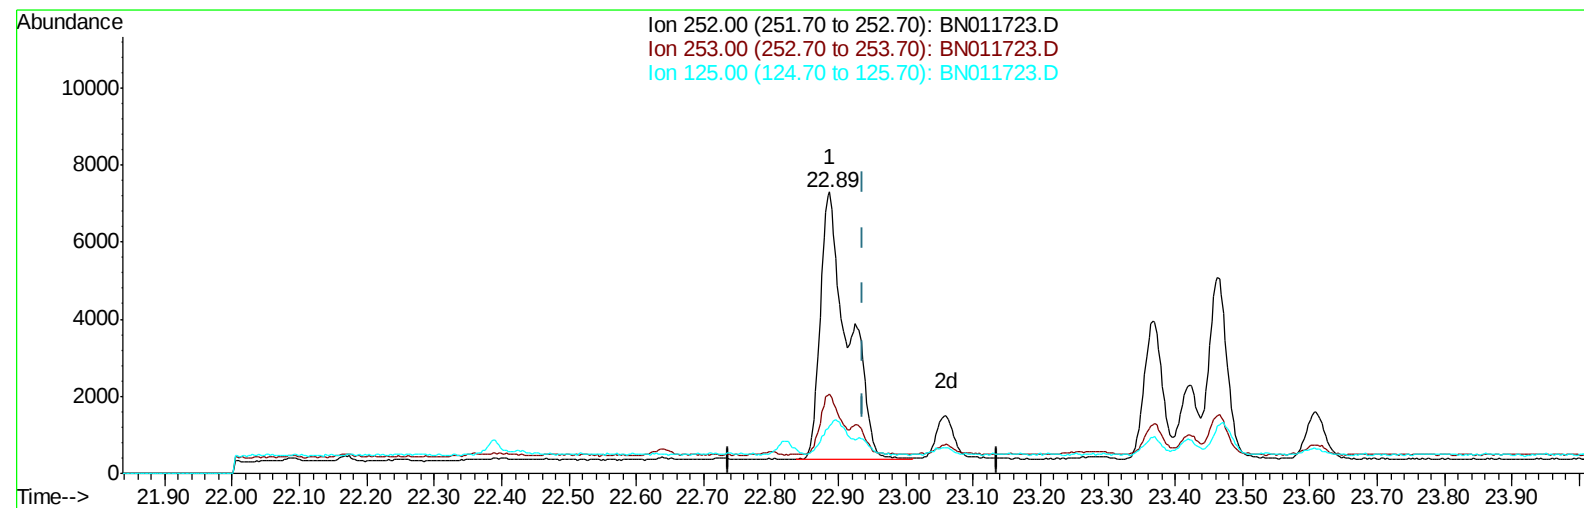

TIC: BN011723.D

(22) Benzo(k)fluoranthene

22.887min (-0.050) 12.70ng/ul

response 19829

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	28.30
125.00	11.40	17.03#
0.00	0.00	0.00