
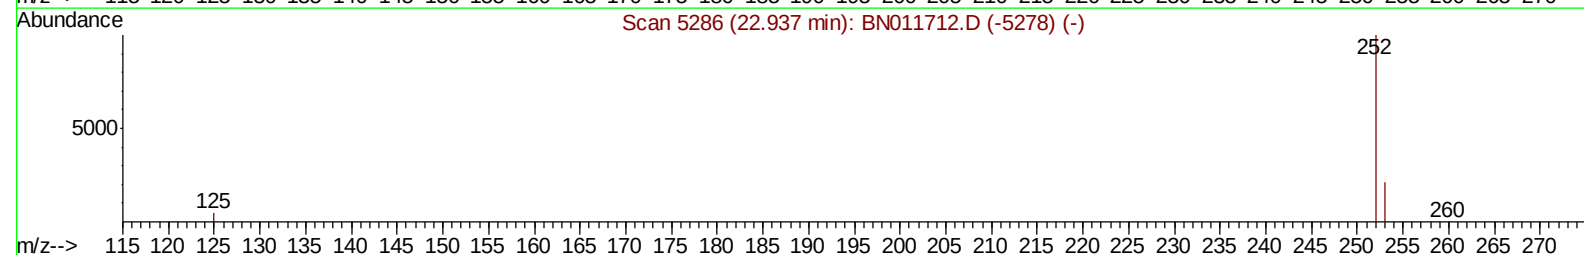
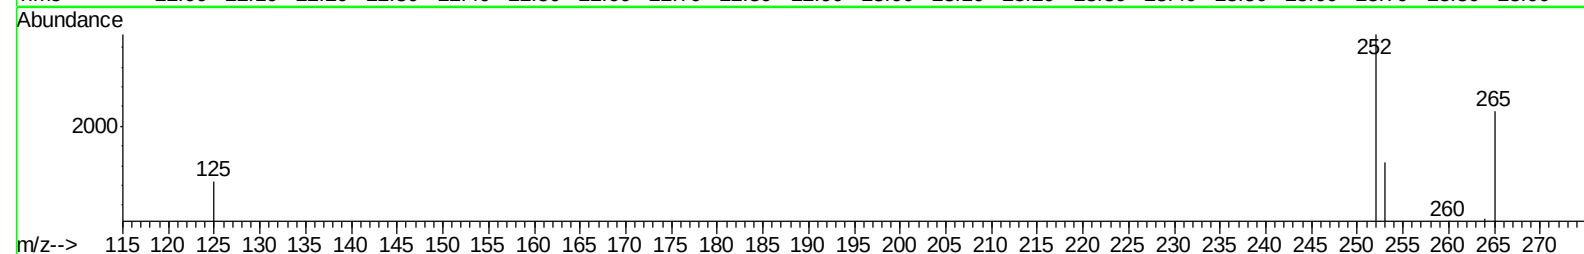


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011723.D
Acq On : 05 Sep 2020 05:00
Operator : CG/JU
Sample : L3843-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 05 06:35:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

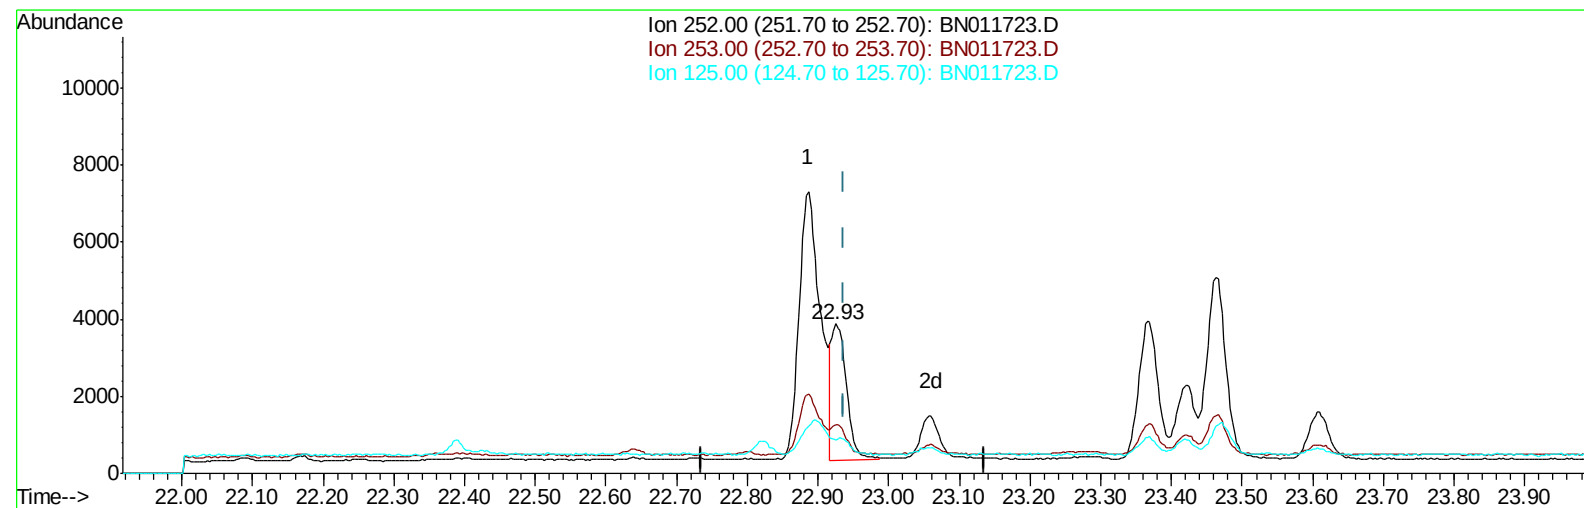

TIC: BN011723.D

(22) Benzo(k)fluoranthene

22.925min (-0.012) 3.35ng/ul m

response 5226

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	32.99#
125.00	11.40	22.47#
0.00	0.00	0.00