
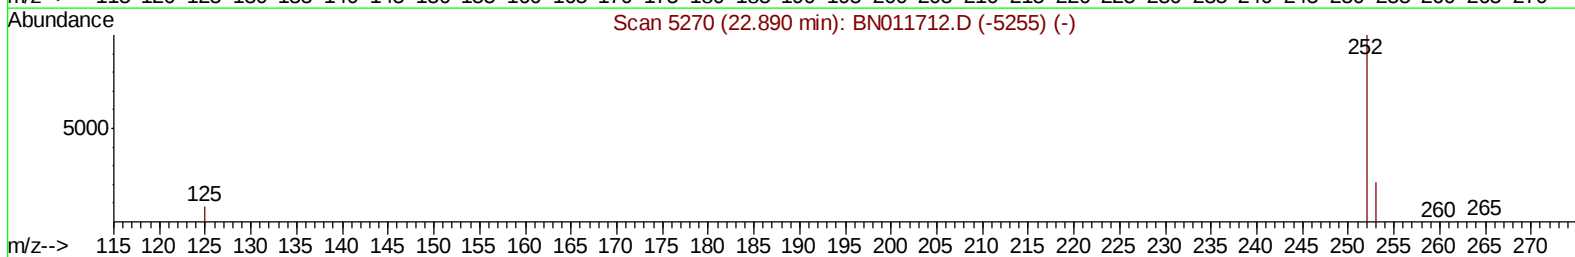
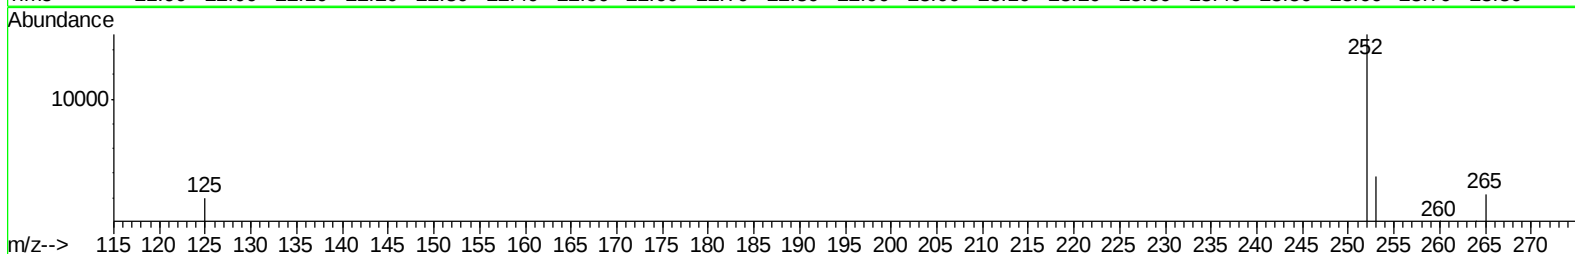


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011724.D
Acq On : 05 Sep 2020 05:36
Operator : CG/JU
Sample : L3843-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Sep 05 06:44:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

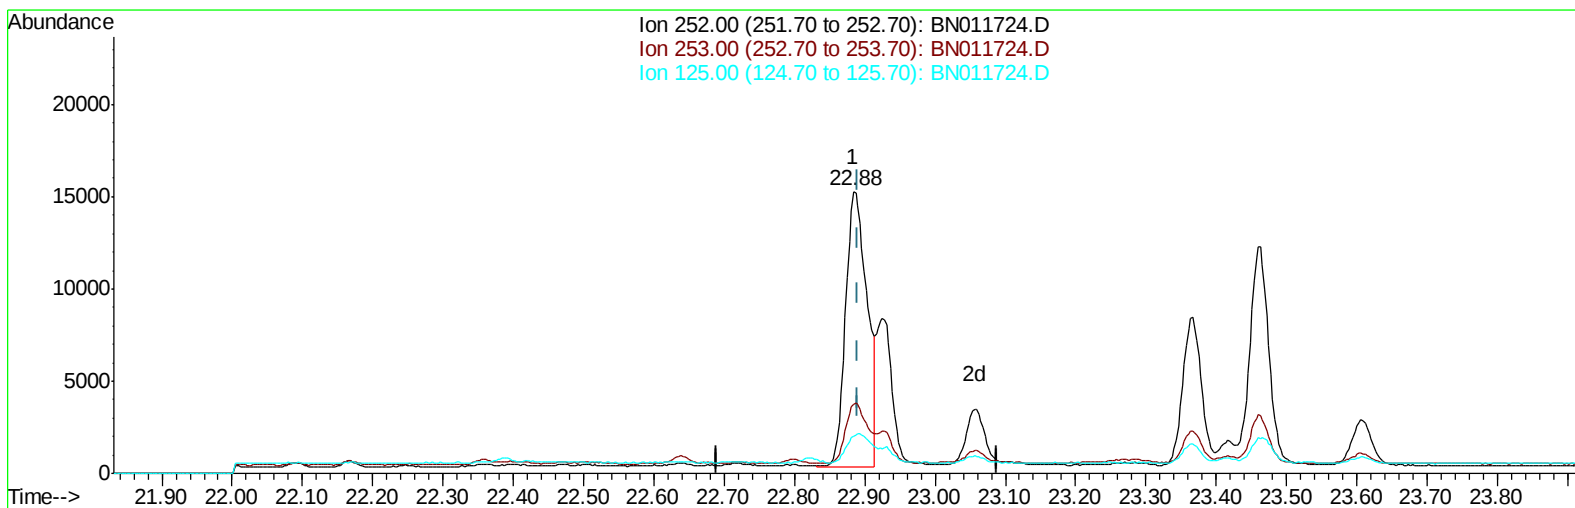

TIC: BN011724.D

(21) Benzo(b)fluoranthene

22.884min (-0.006) 0.52ng/ul m

response 31734

Ion	Exp%	Act%
252.00	100	100
253.00	27.40	24.69
125.00	11.10	13.07
0.00	0.00	0.00