
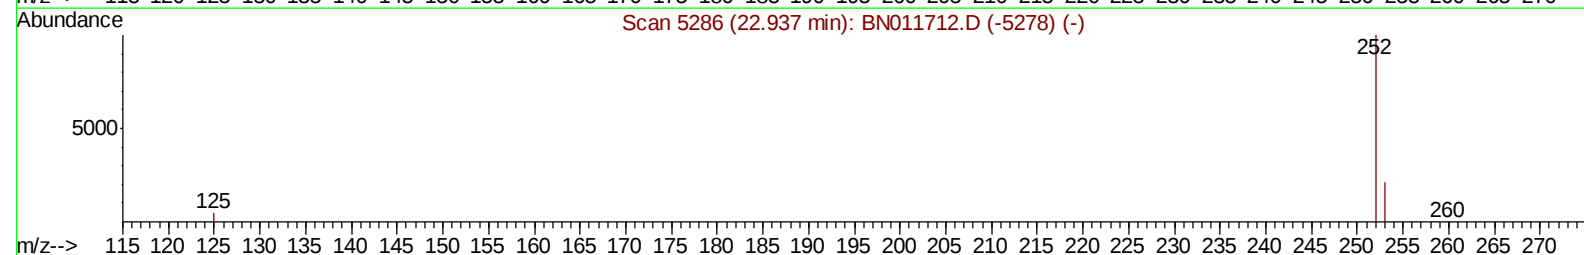
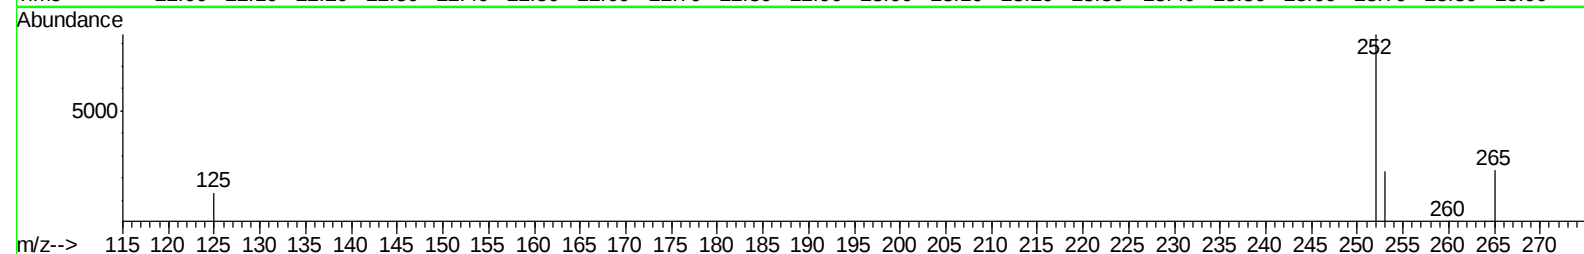


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011724.D
 Acq On : 05 Sep 2020 05:36
 Operator : CG/JU
 Sample : L3843-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Quant Time: Sep 05 06:44:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

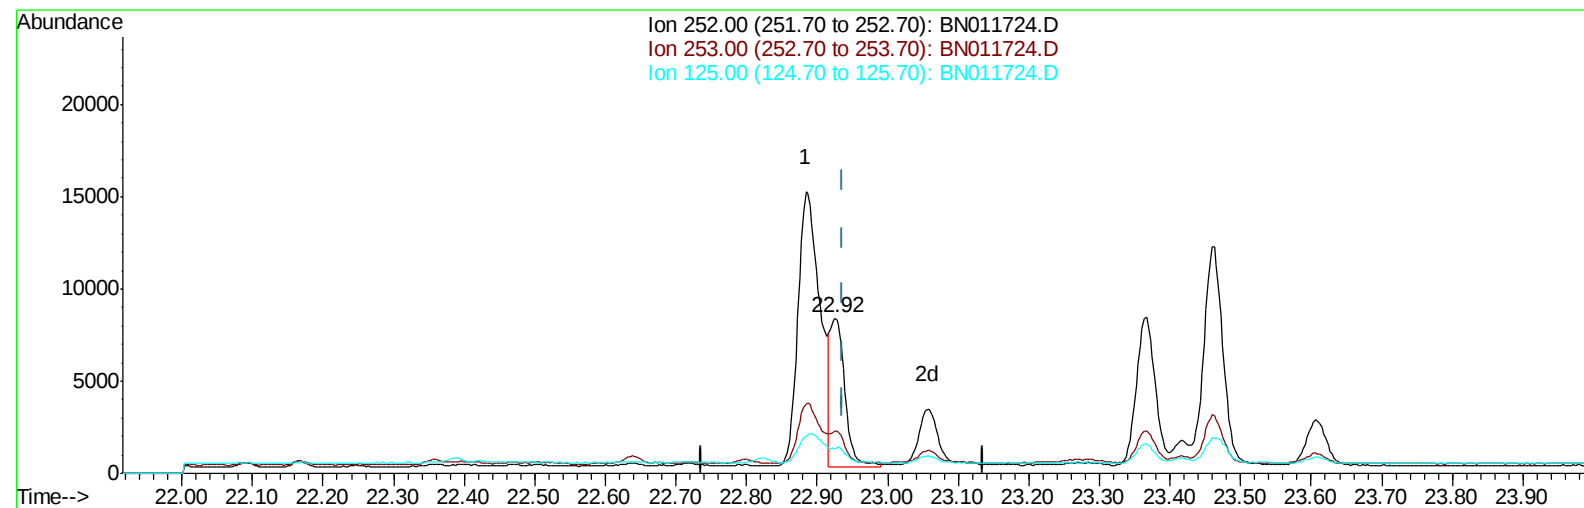

TIC: BN011724.D

(22) Benzo(k)fluoranthene

22.925min (-0.012) 0.17ng/ul m

response 11436

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	27.43
125.00	11.40	16.07#
0.00	0.00	0.00