
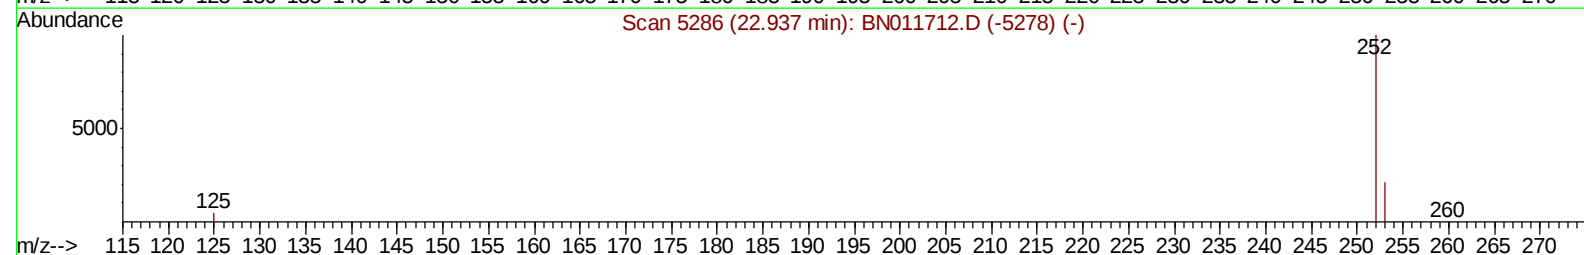
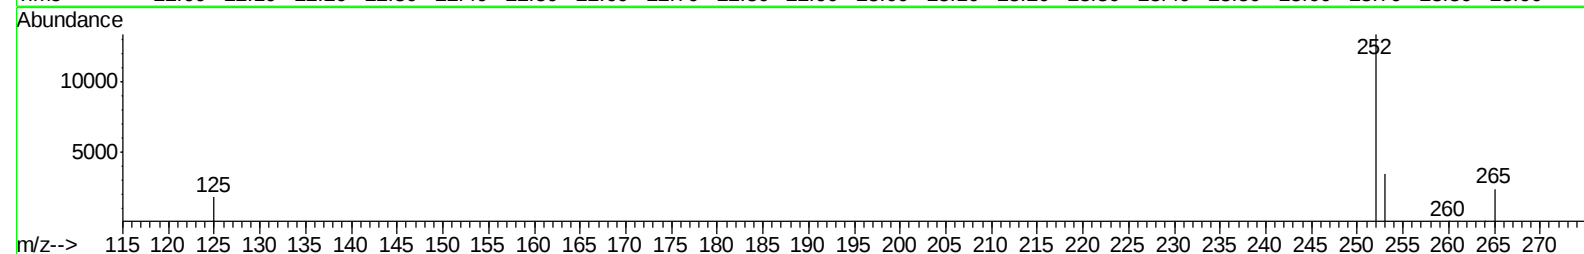


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
 Data File : BN011725.D
 Acq On : 05 Sep 2020 06:12
 Operator : CG/JU
 Sample : L3843-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Quant Time: Sep 05 06:44:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 05 05:40:34 2020
 Response via : Initial Calibration

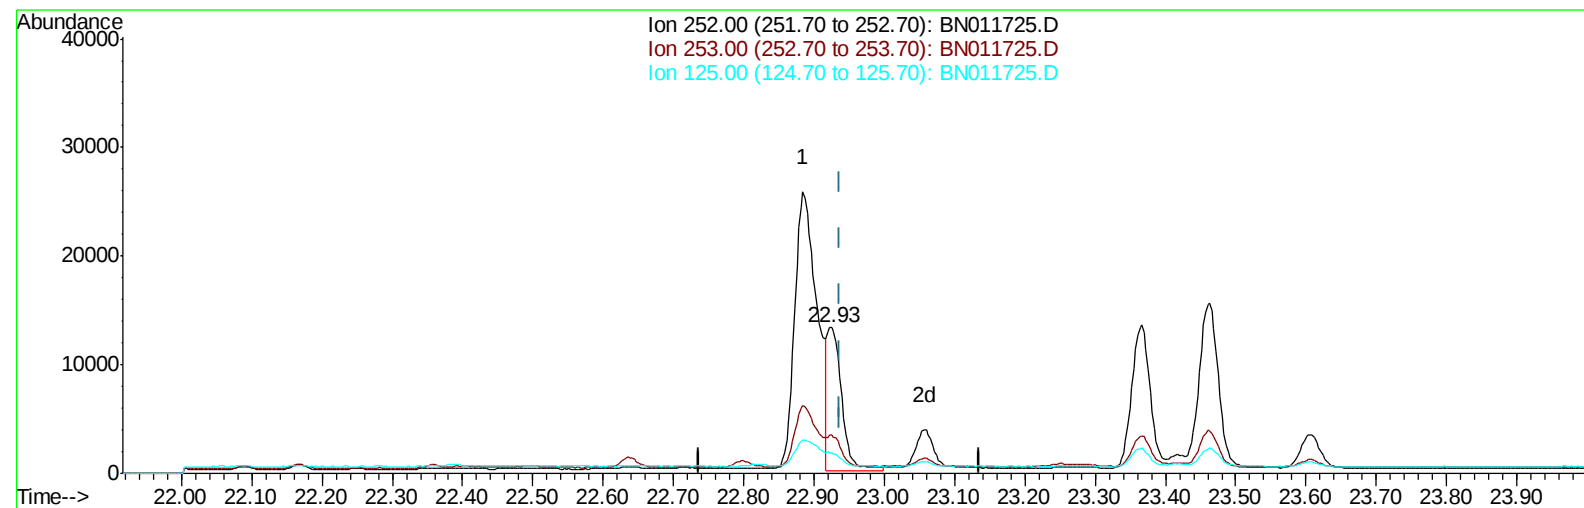

TIC: BN011725.D

(22) Benzo(k)fluoranthene

22.925min (-0.012) 0.28ng/ul m

response 18840

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	26.25
125.00	11.40	13.68#
0.00	0.00	0.00