
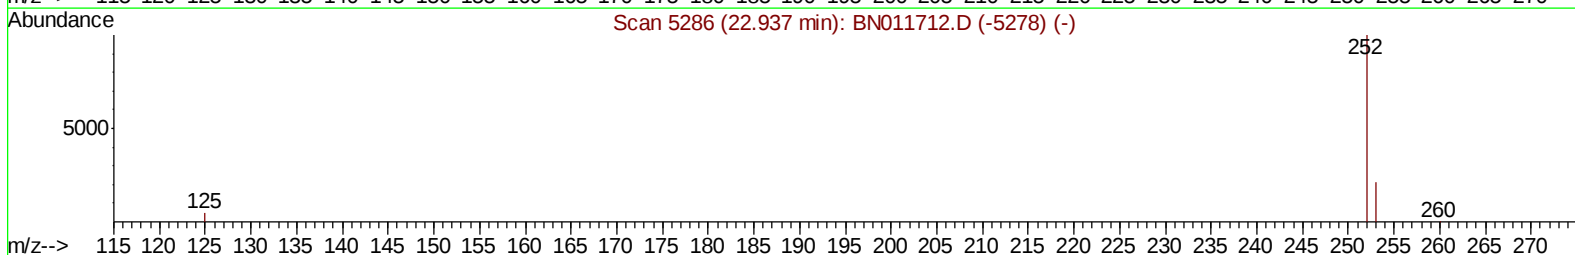
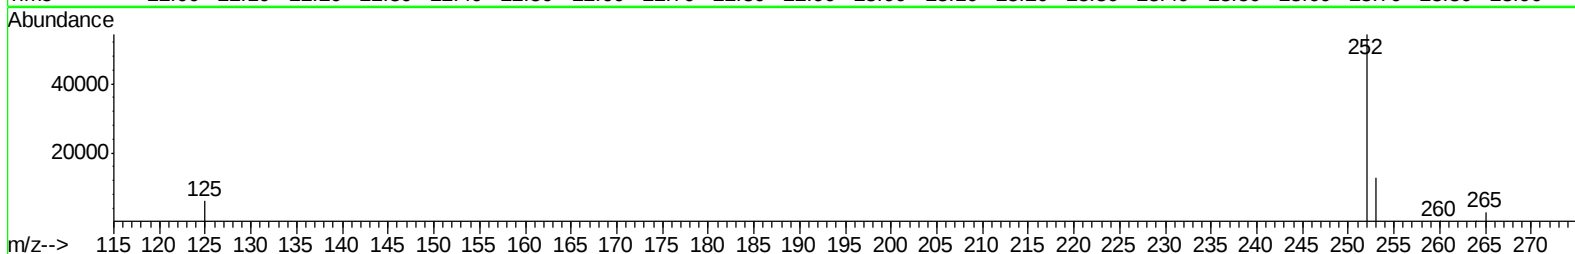


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090420\
Data File : BN011726.D
Acq On : 05 Sep 2020 06:48
Operator : CG/JU
Sample : L3843-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Sep 05 07:20:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN081220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 05 05:40:34 2020
Response via : Initial Calibration

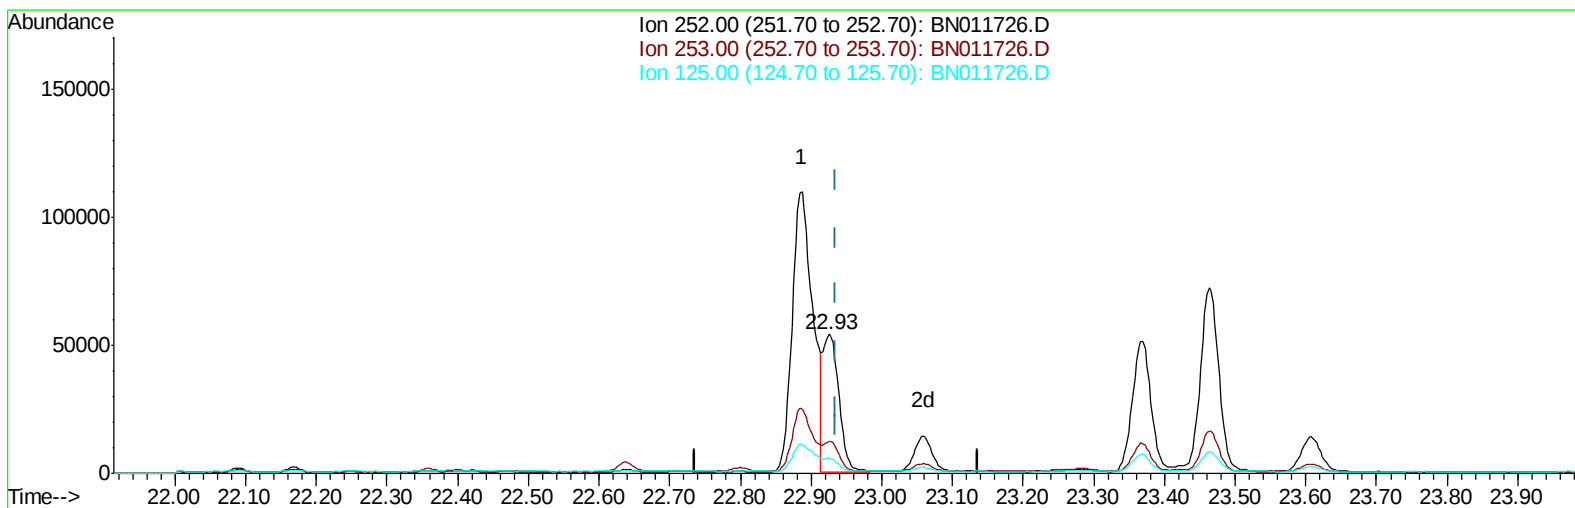

TIC: BN011726.D

(22) Benzo(k)fluoranthene

22.925min (-0.012) 1.16ng/ul m

response 84053

Ion	Exp%	Act%
252.00	100	100
253.00	27.20	23.23
125.00	11.40	11.10
0.00	0.00	0.00